




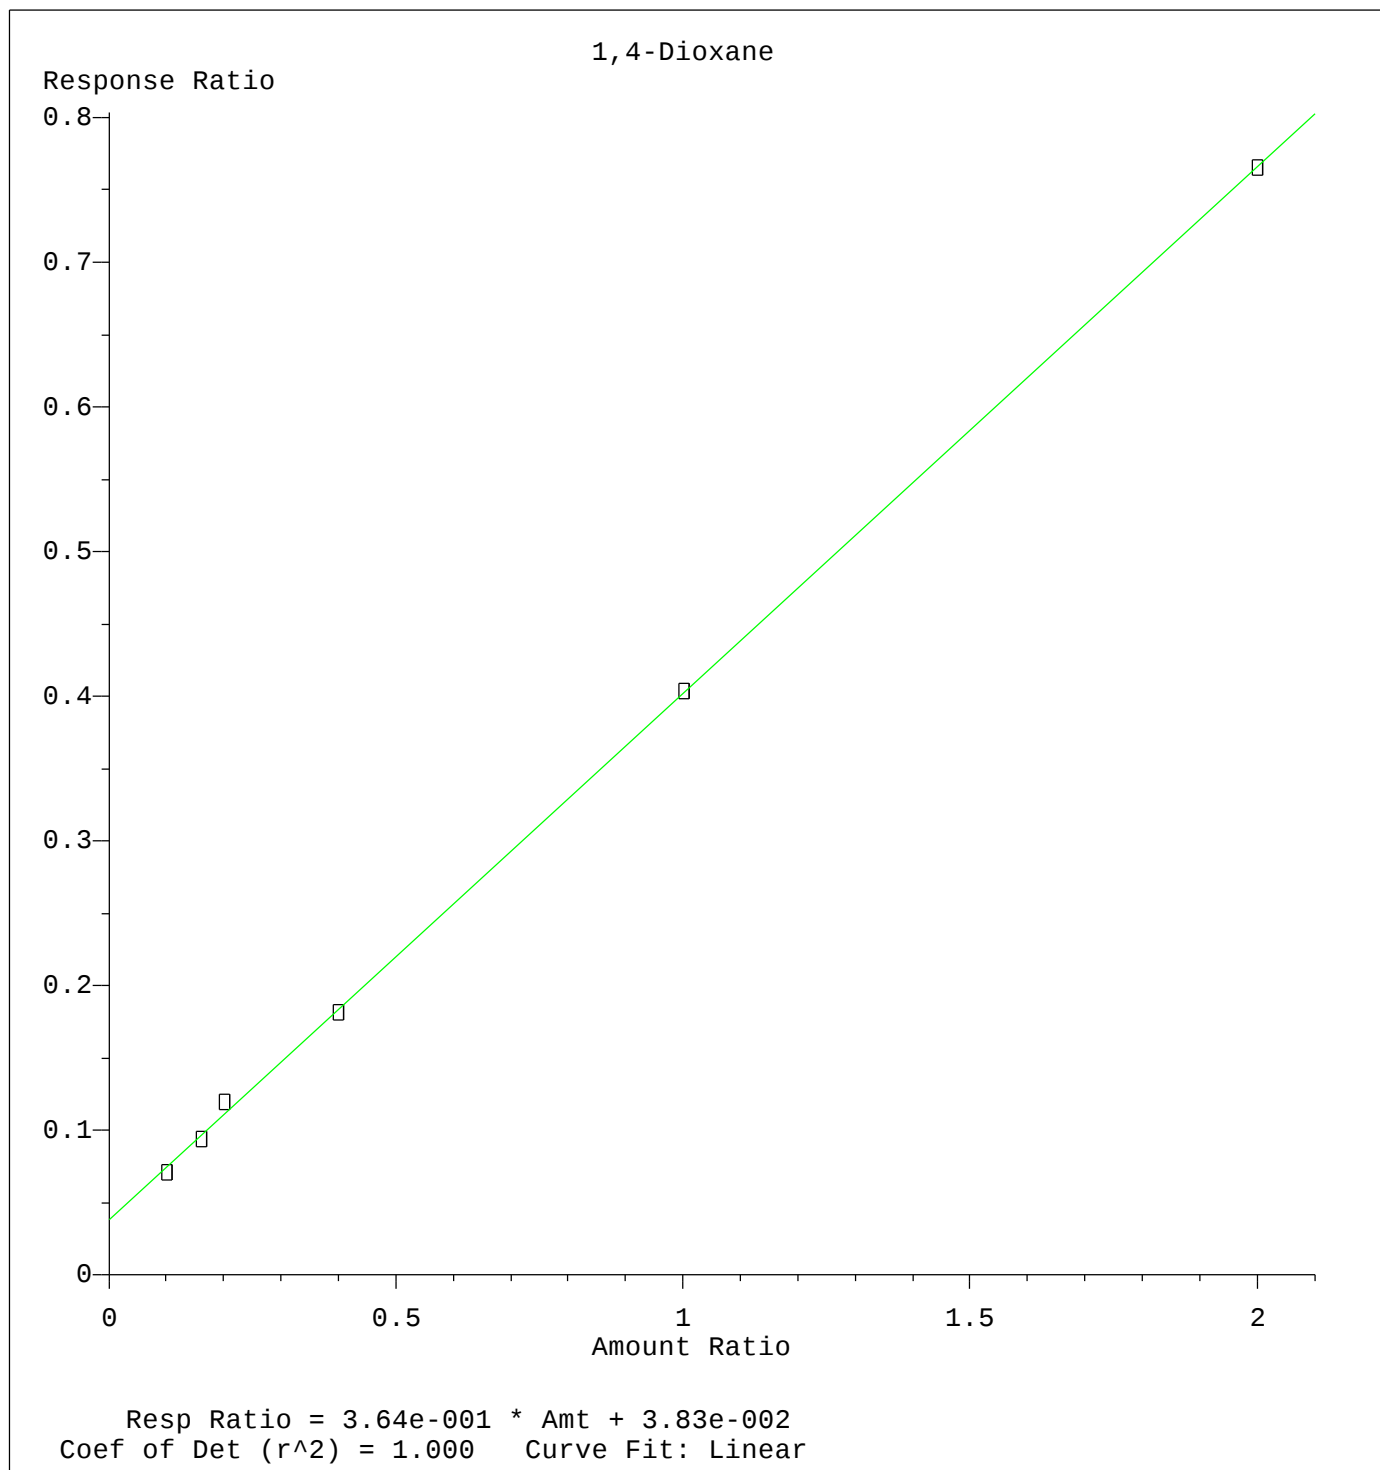


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015

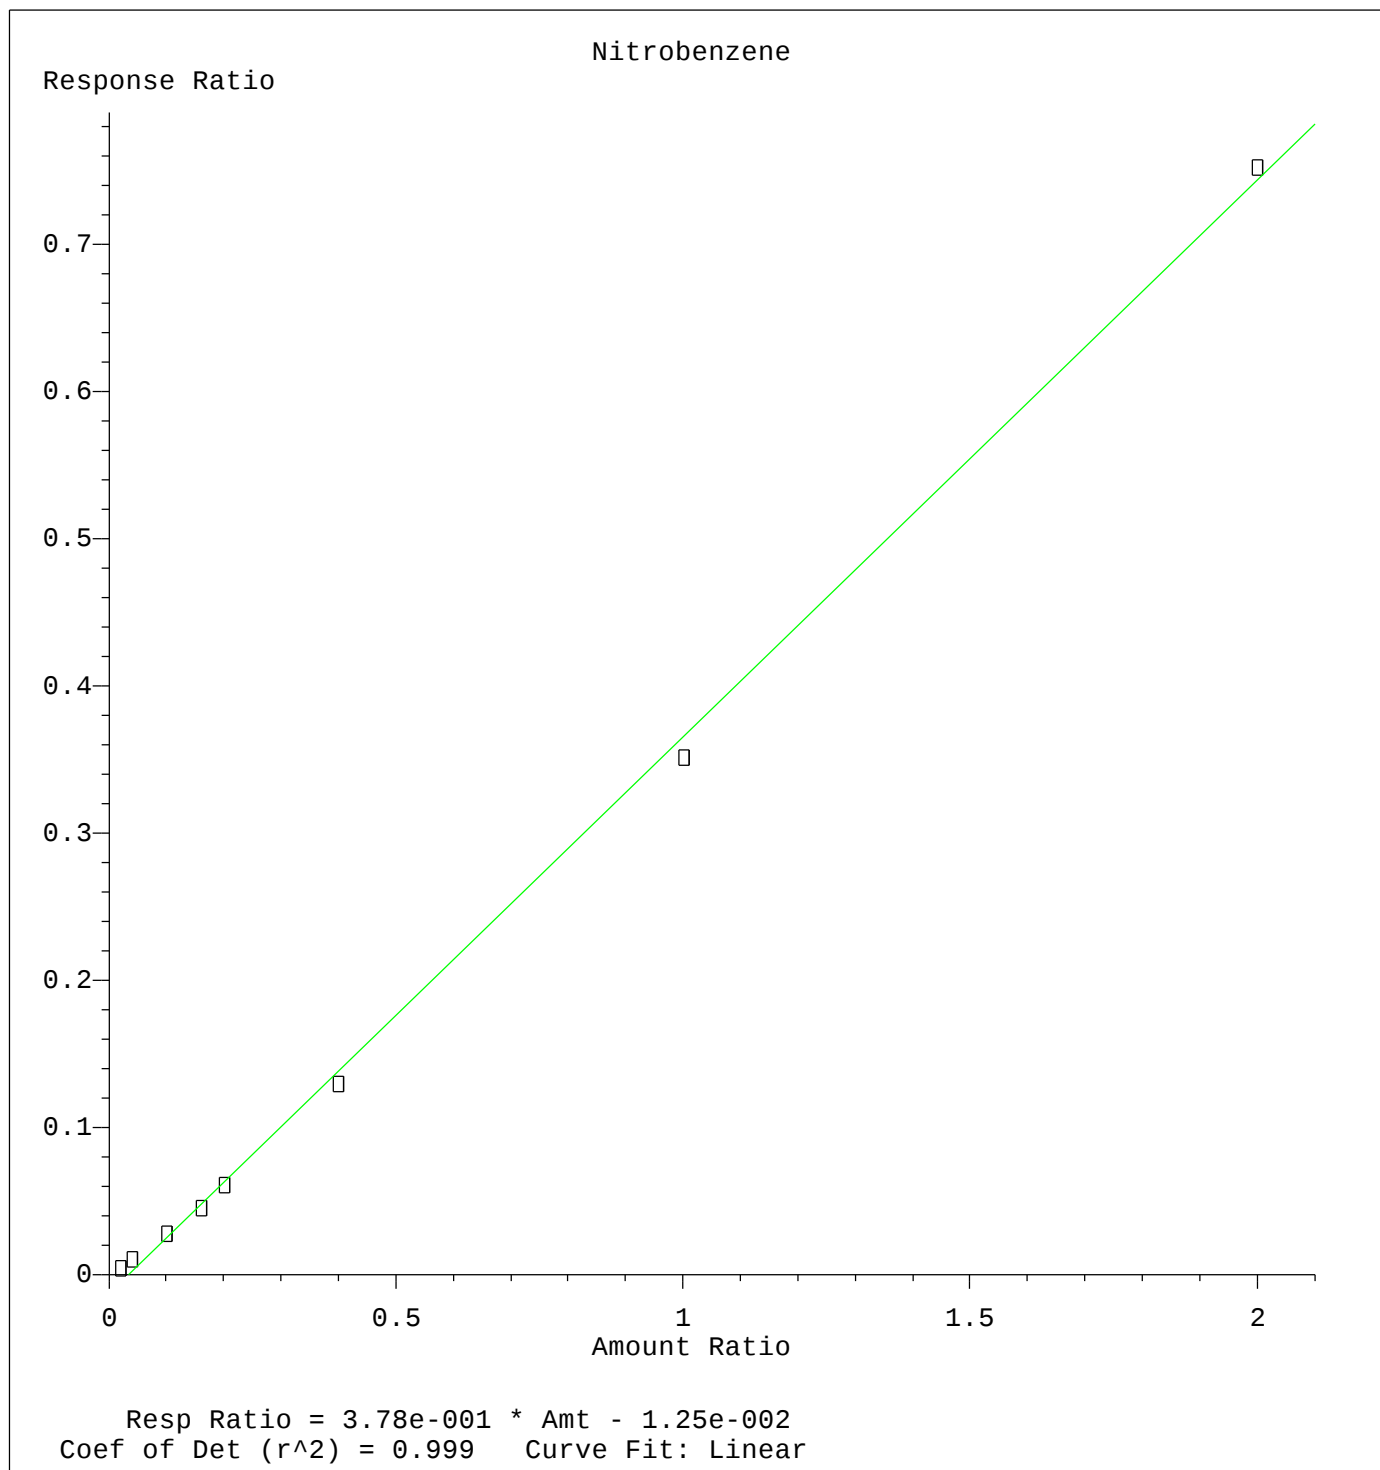


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015

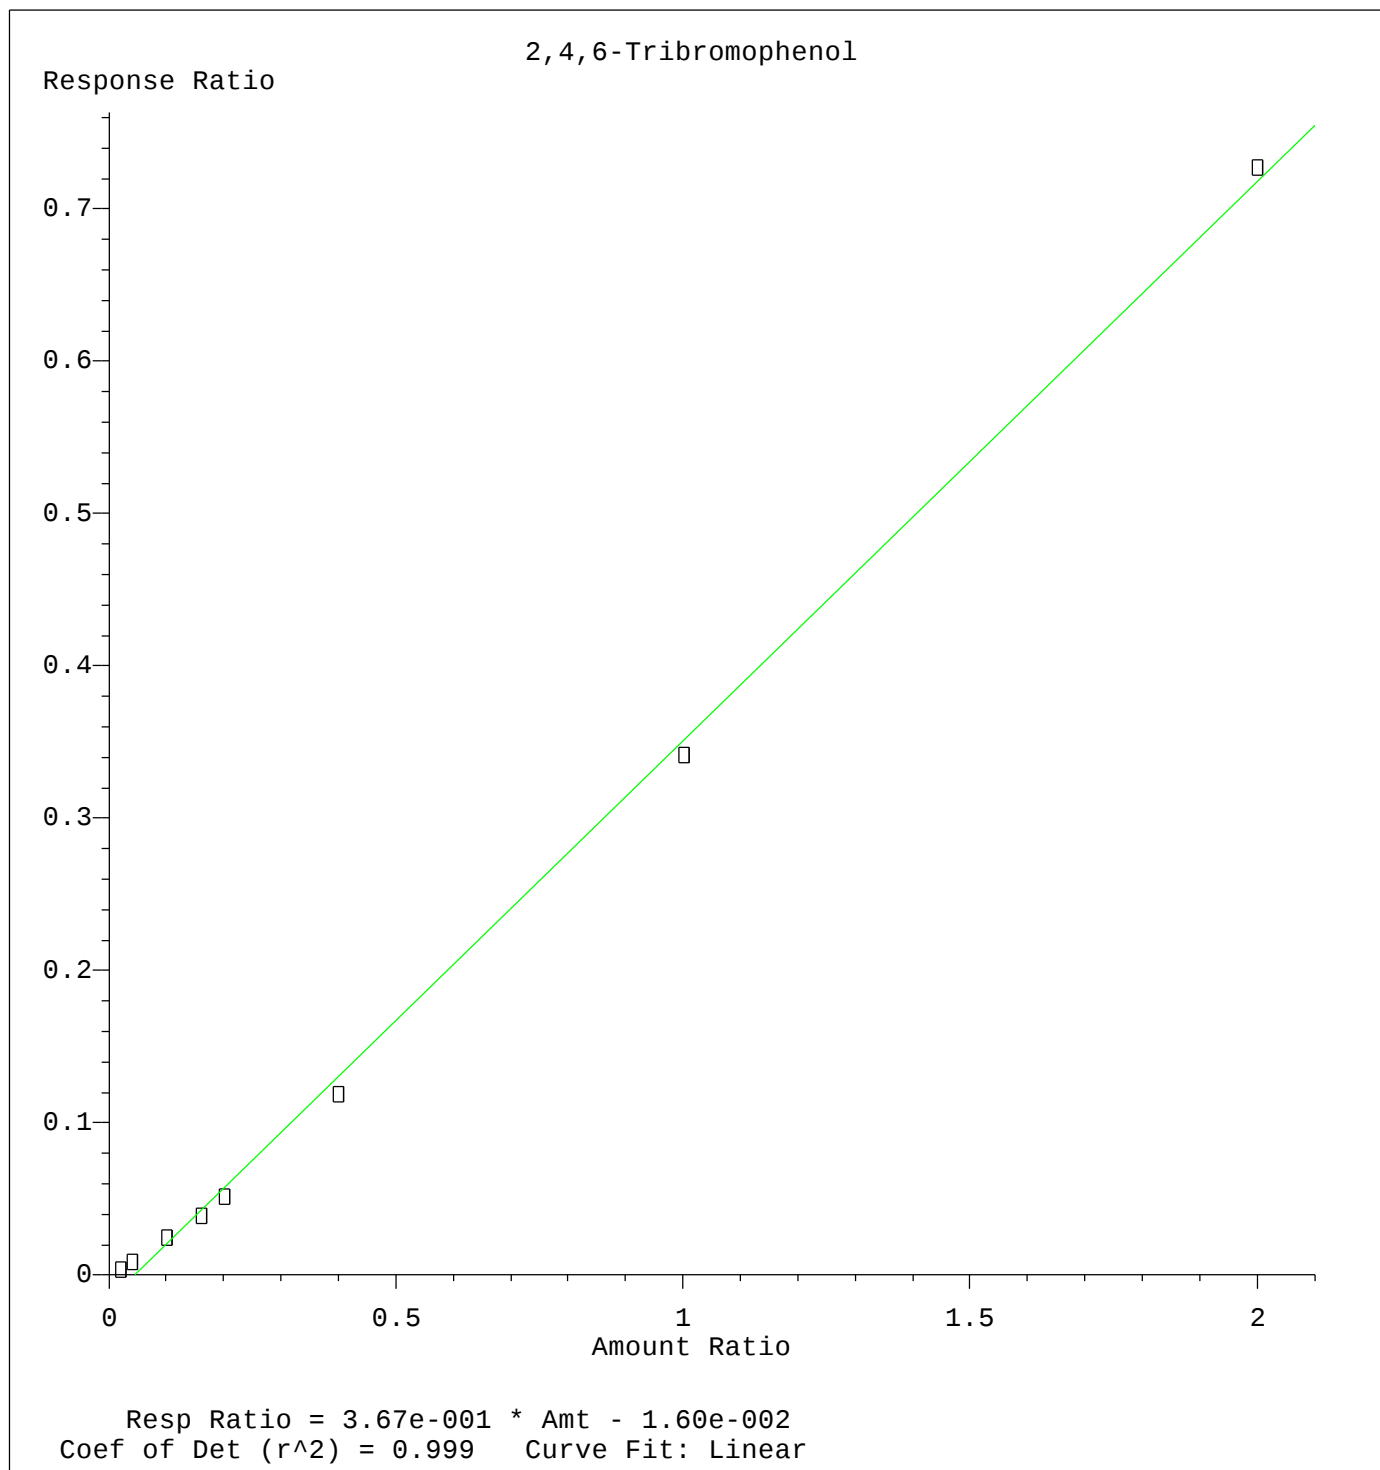


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015

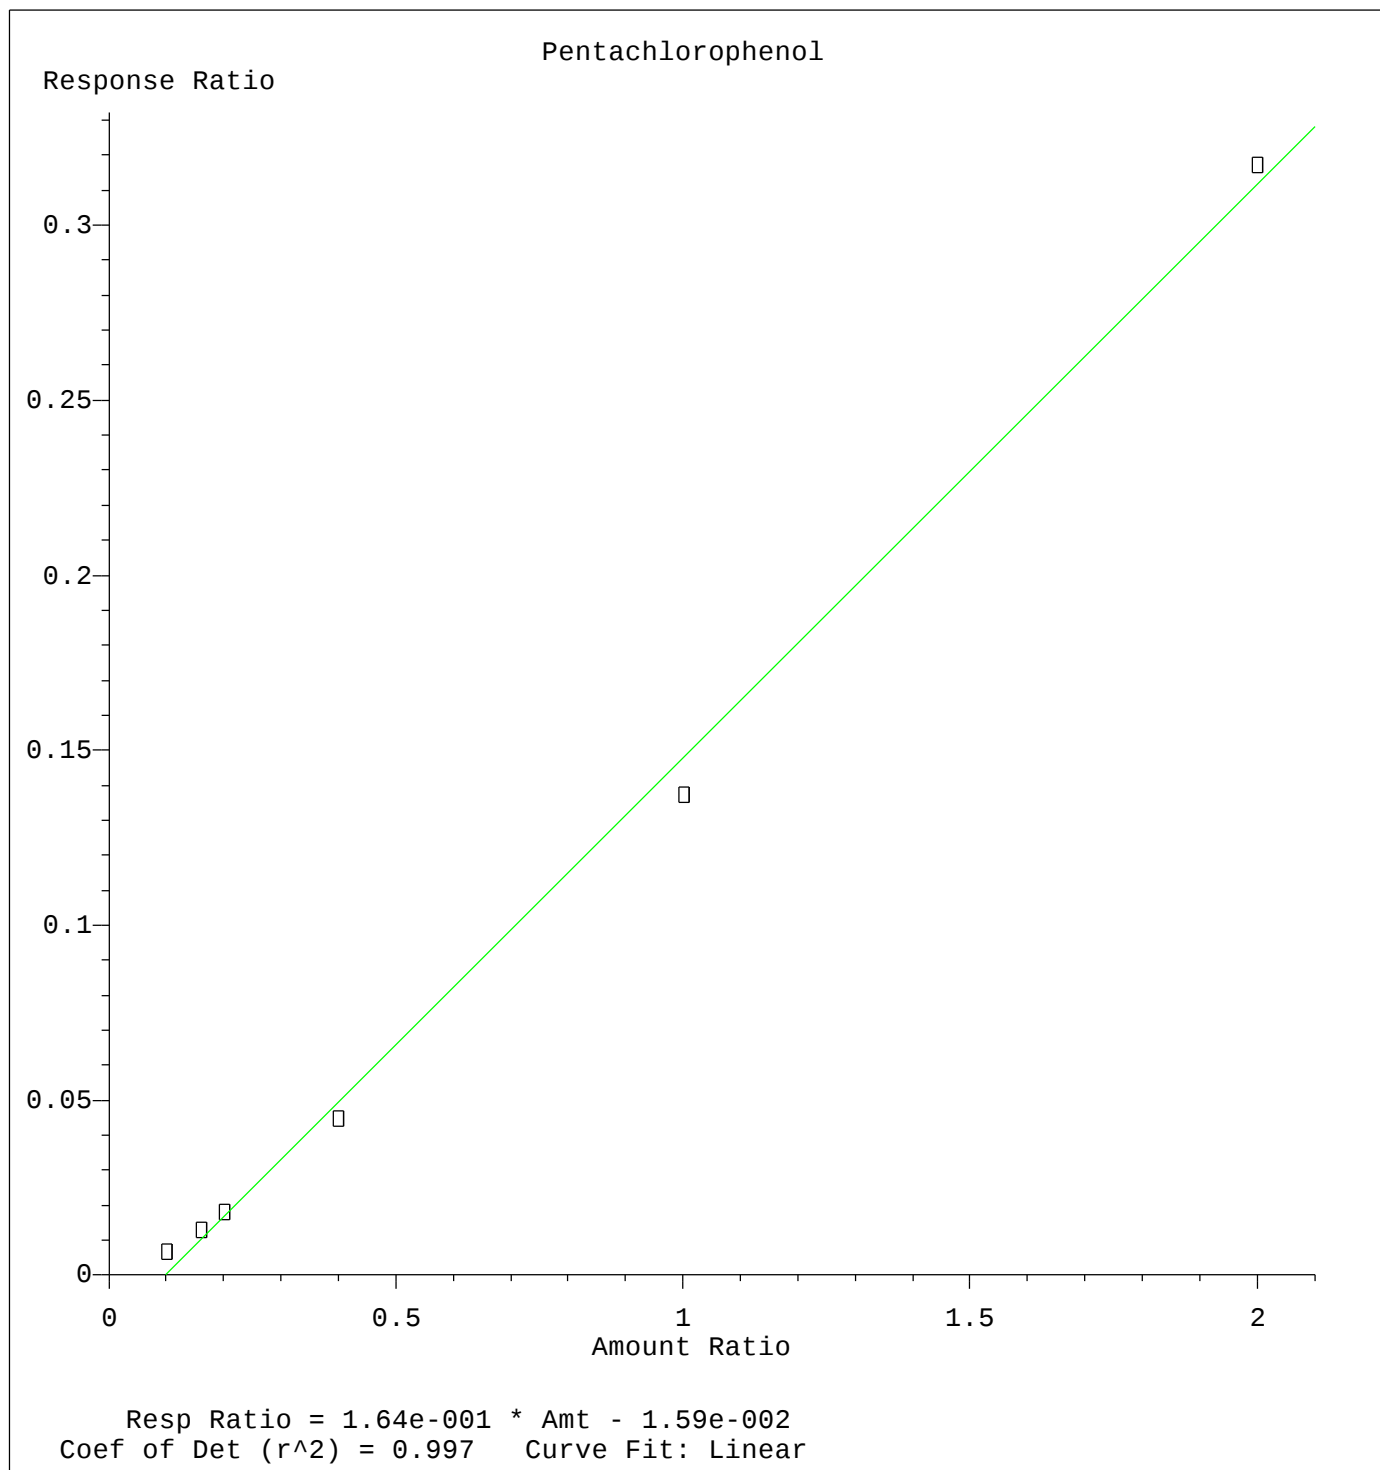

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015

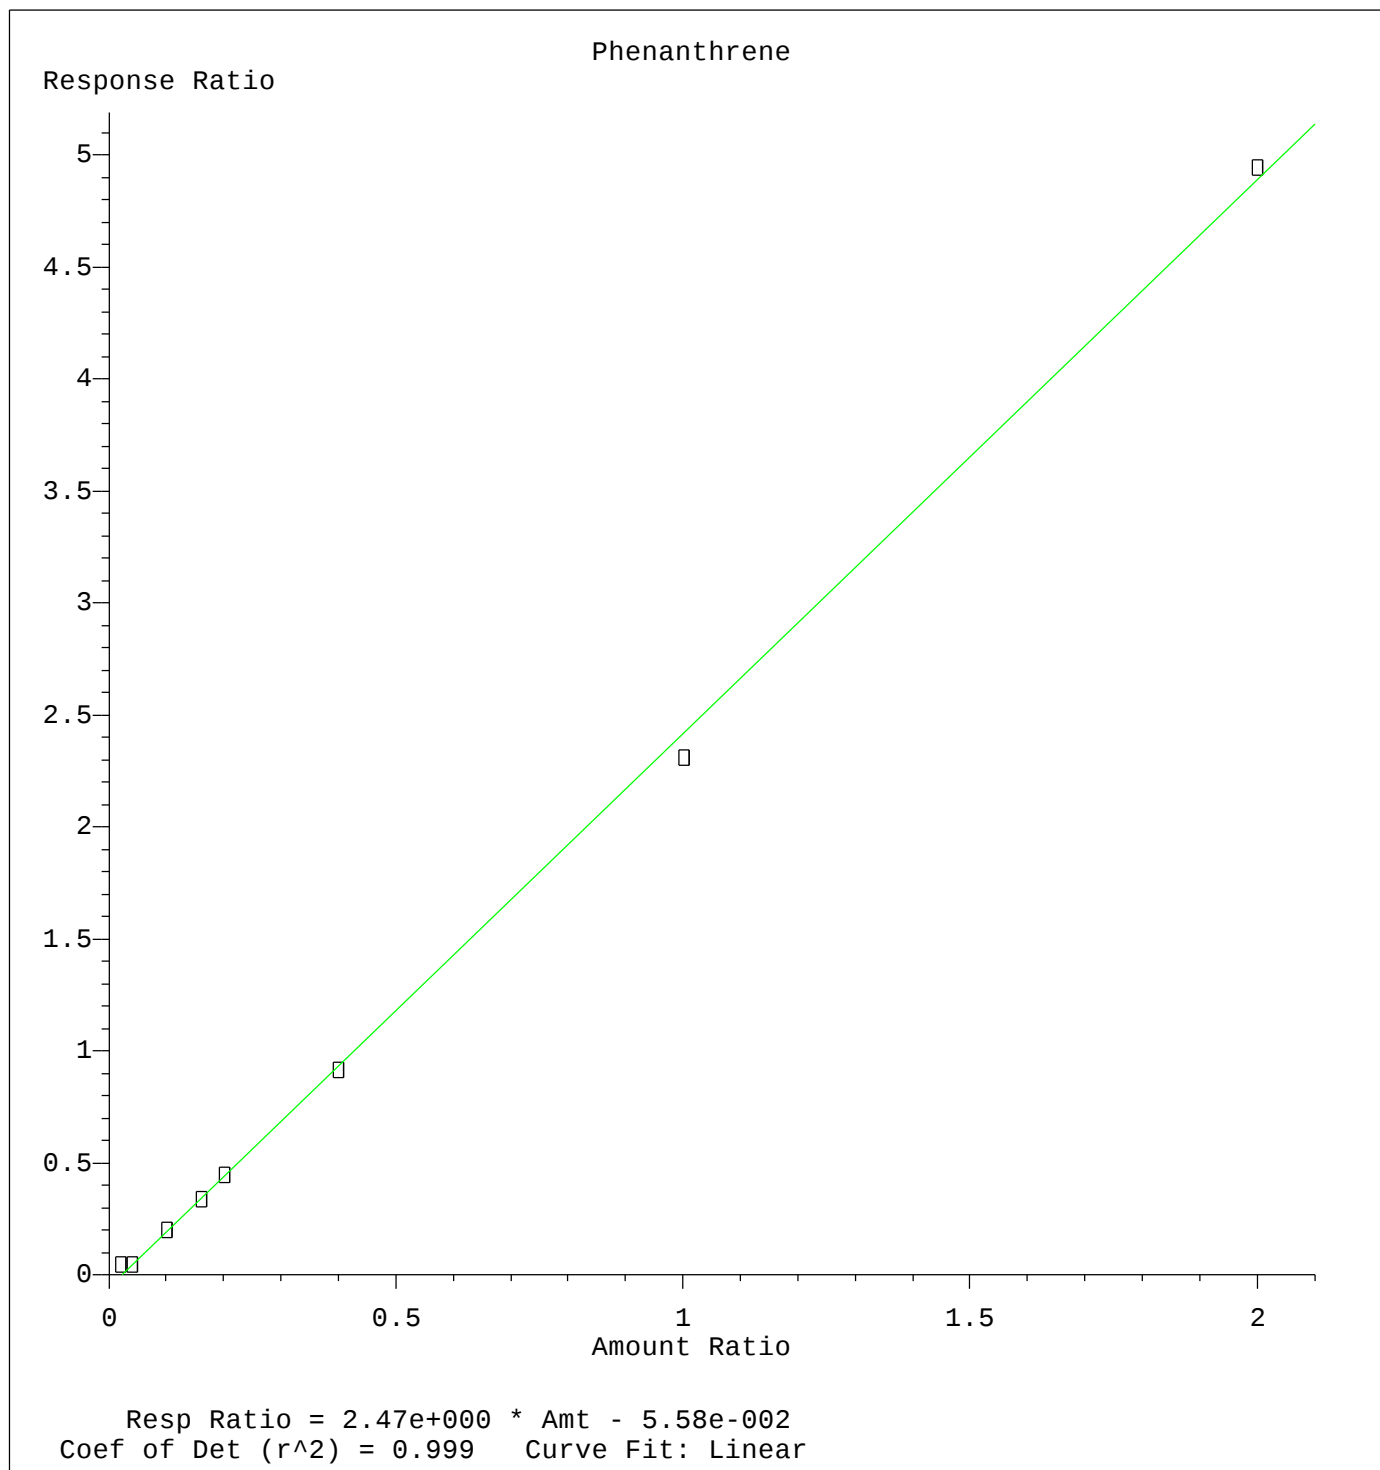

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015

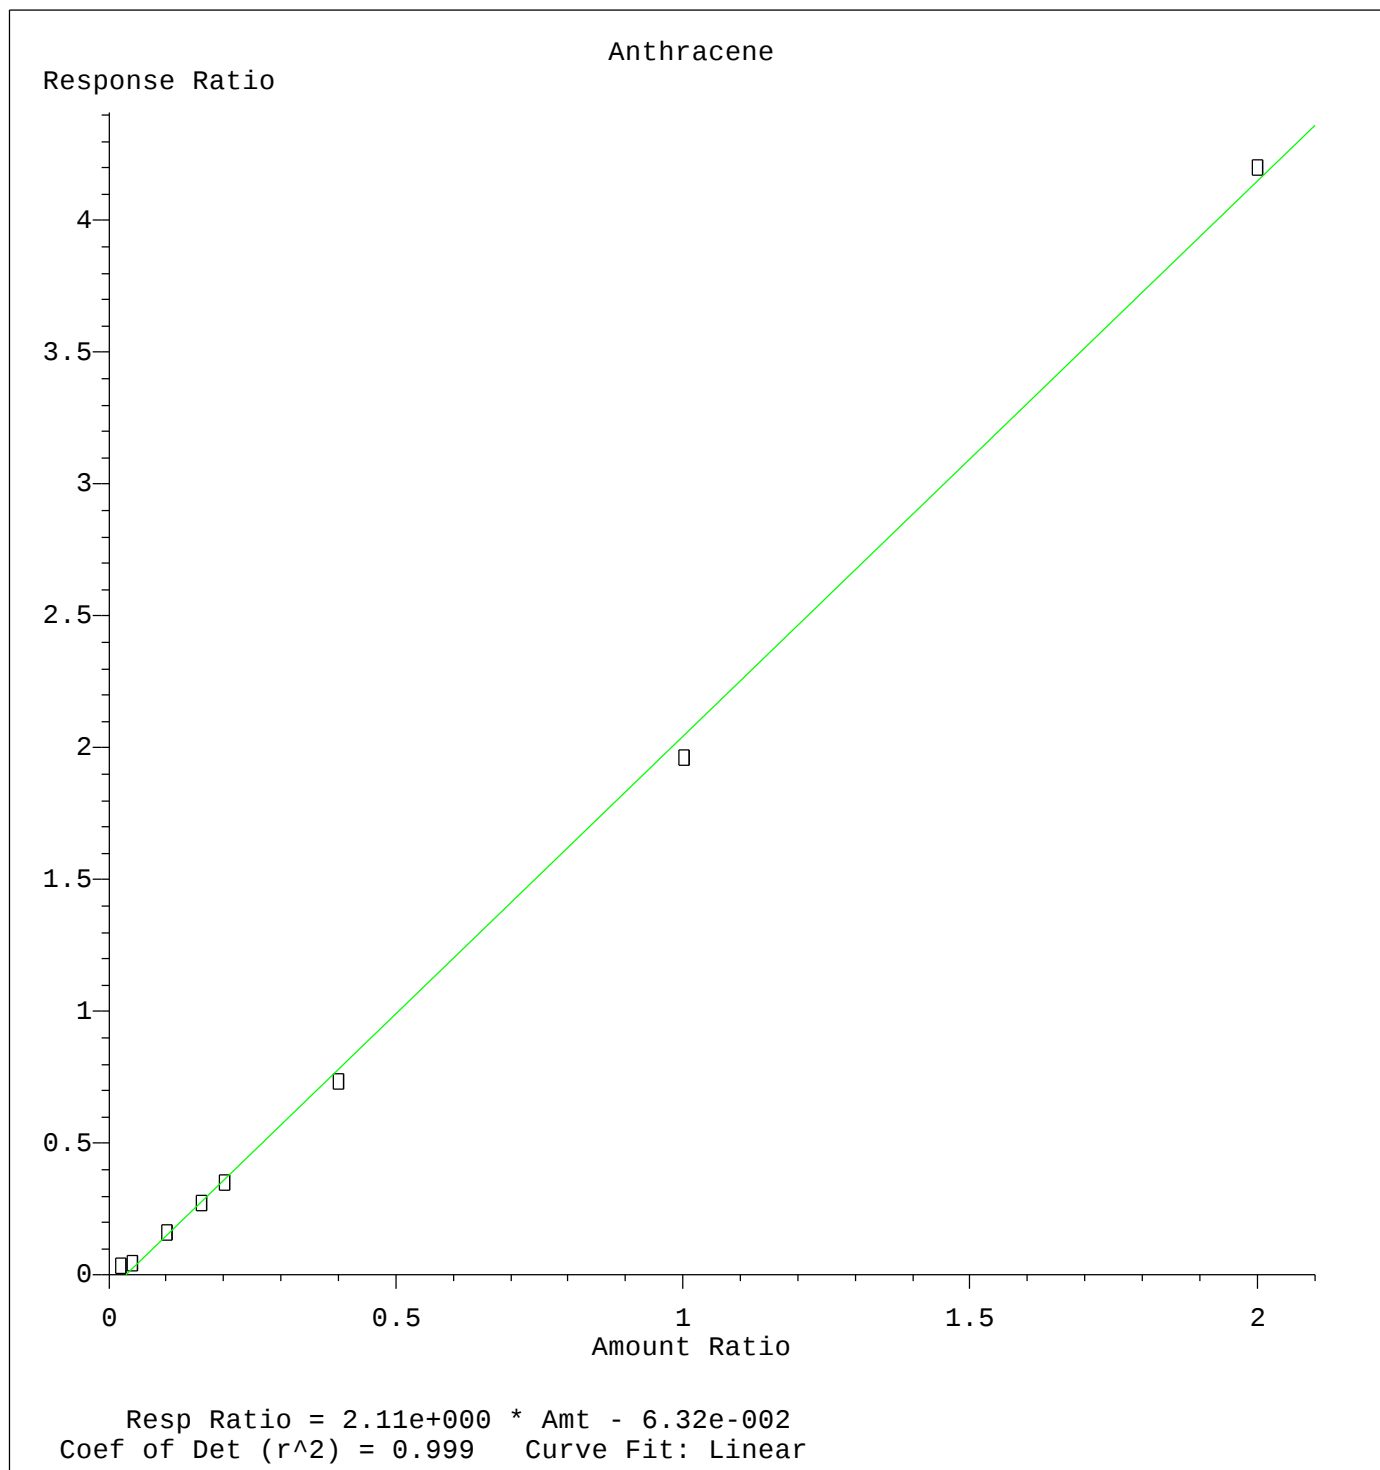

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050515.M
Calibration Table Last Updated: Wed May 06 05:58:57 2015