


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050515\
 Data File : BM001206.D
 Acq On : 05 May 2015 13:16
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

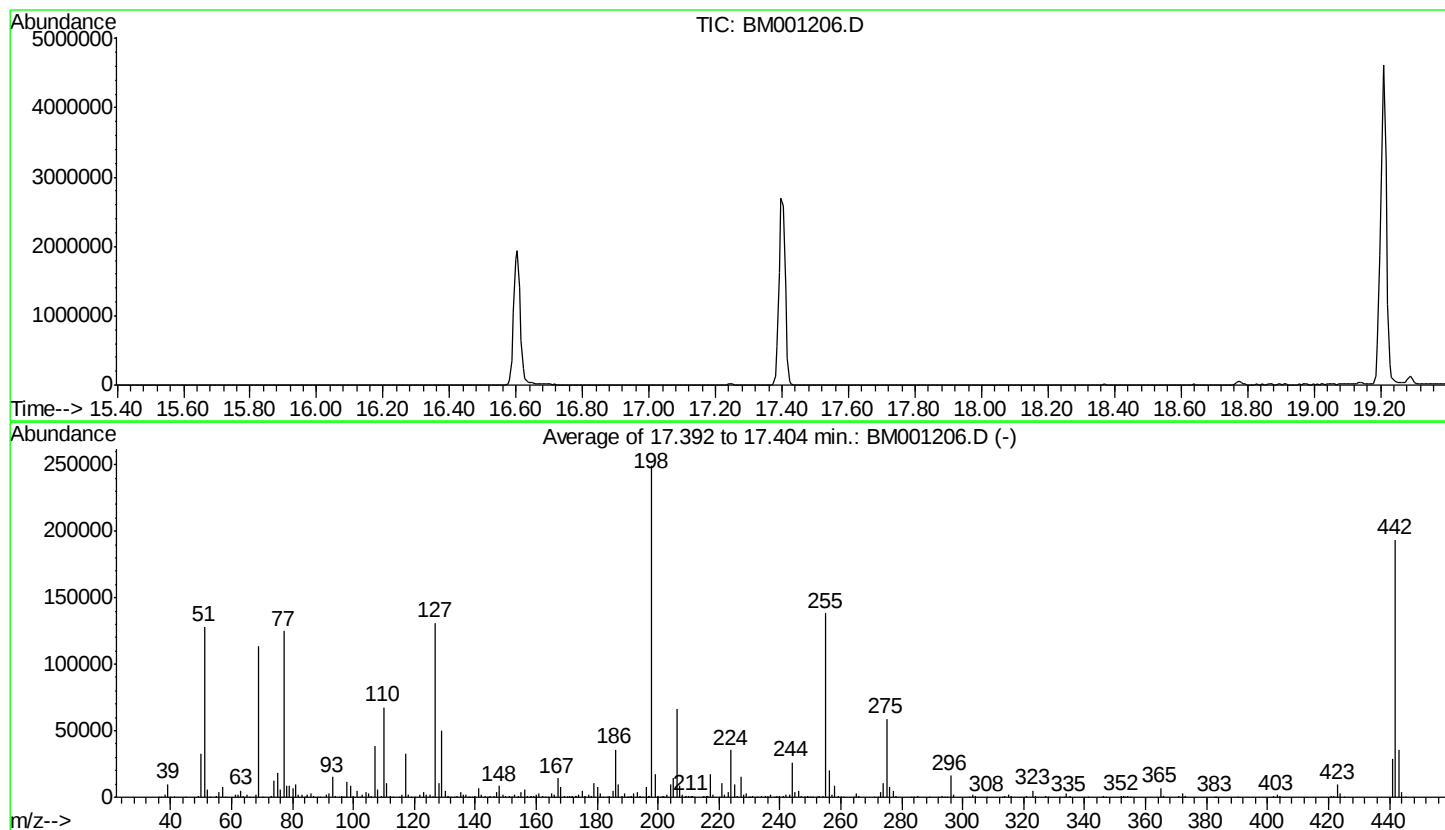

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	128232	PASS
68	69	0.00	2	2.0	2223	PASS
69	198	0.00	100	45.6	113722	PASS
70	69	0.00	2	0.4	490	PASS
127	198	10	80	52.5	130954	PASS
197	198	0.00	2	0.3	793	PASS
198	198	100	100	100.0	249237	PASS
199	198	5	9	6.9	17286	PASS
275	198	10	60	23.6	58770	PASS
365	198	1	100	2.7	6737	PASS
441	442	0.01	24	15.1	29204	PASS
442	198	50	100	77.8	193816	PASS
443	442	15	24	18.5	35773	PASS