


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050515\
 Data File : BM001220.D
 Acq On : 06 May 2015 09:23
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

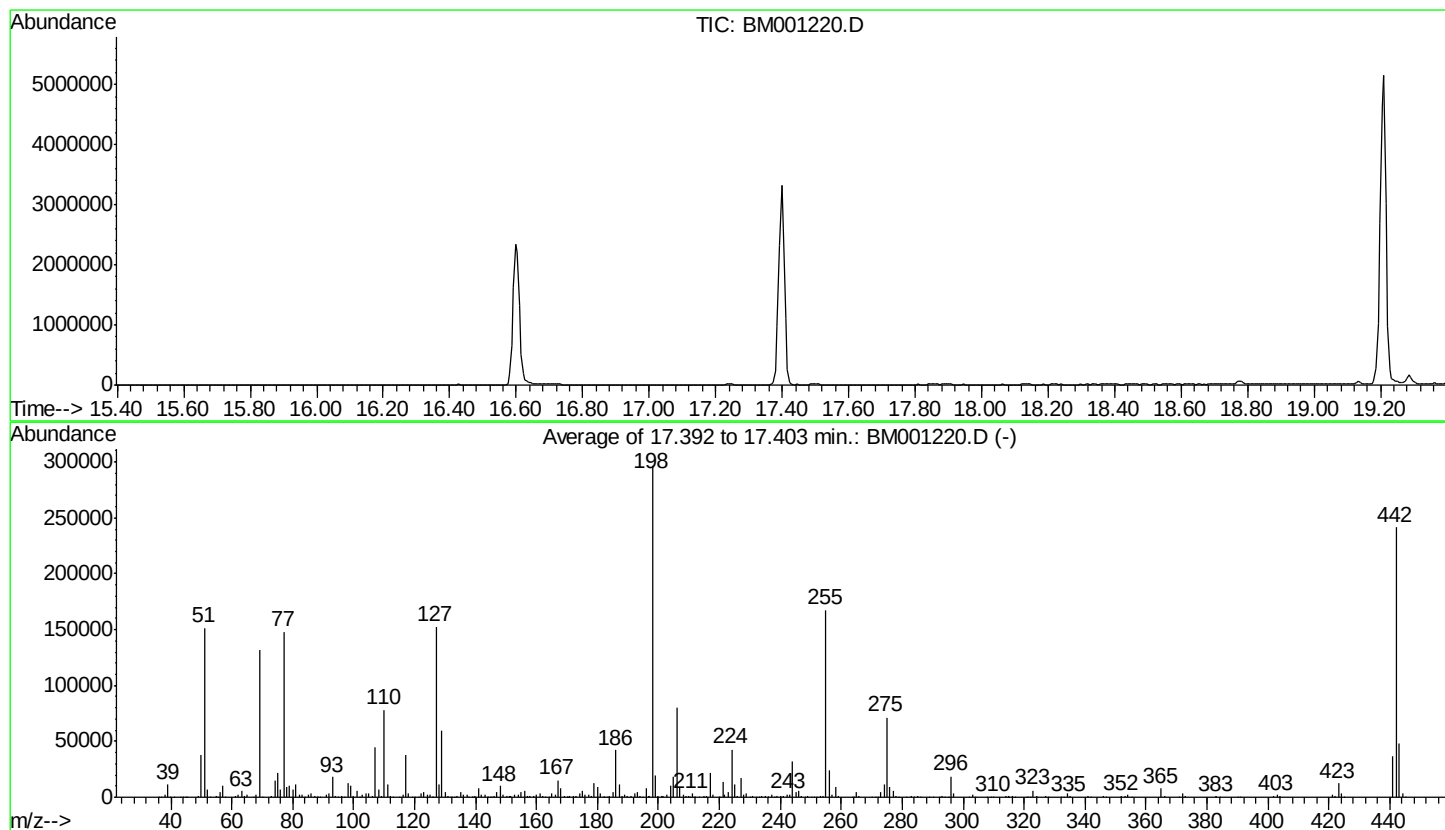

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	151426	PASS
68	69	0.00	2	1.6	2066	PASS
69	198	0.00	100	44.5	132000	PASS
70	69	0.00	2	0.4	504	PASS
127	198	10	80	51.4	152618	PASS
197	198	0.00	2	0.3	787	PASS
198	198	100	100	100.0	296810	PASS
199	198	5	9	6.6	19698	PASS
275	198	10	60	24.0	71218	PASS
365	198	1	100	2.6	7815	PASS
441	442	0.01	24	15.4	37224	PASS
442	198	50	100	81.4	241472	PASS
443	442	15	24	19.8	47752	PASS