
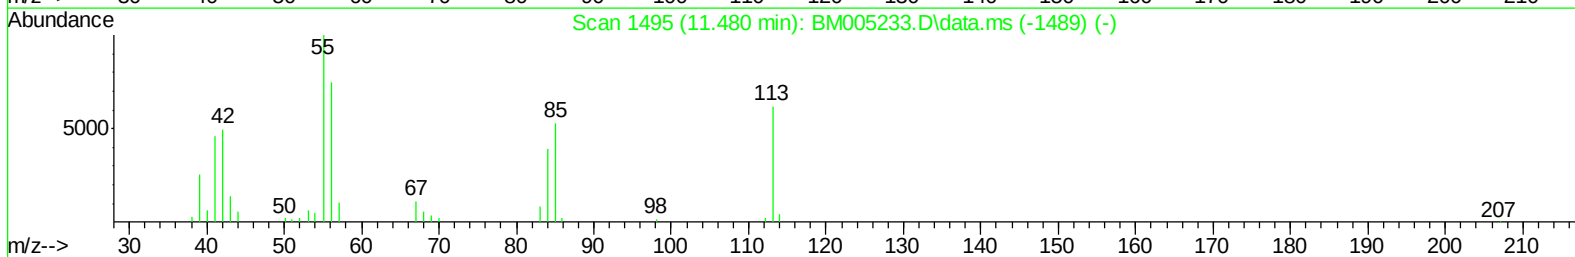
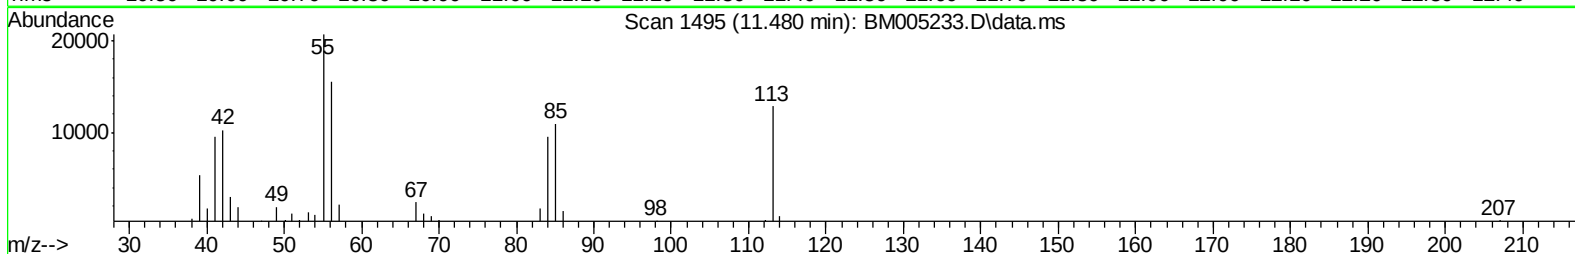


Data Path : Z:\HPCHEM1\BNA M\Data\BM050516\  
Data File : BM005233.D  
Acq On : 05 May 2016 12:21  
Operator : UM/SJ  
Sample : SSTD02042  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 05 13:42:18 2016  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu May 05 13:39:01 2016  
Response via : Initial Calibration

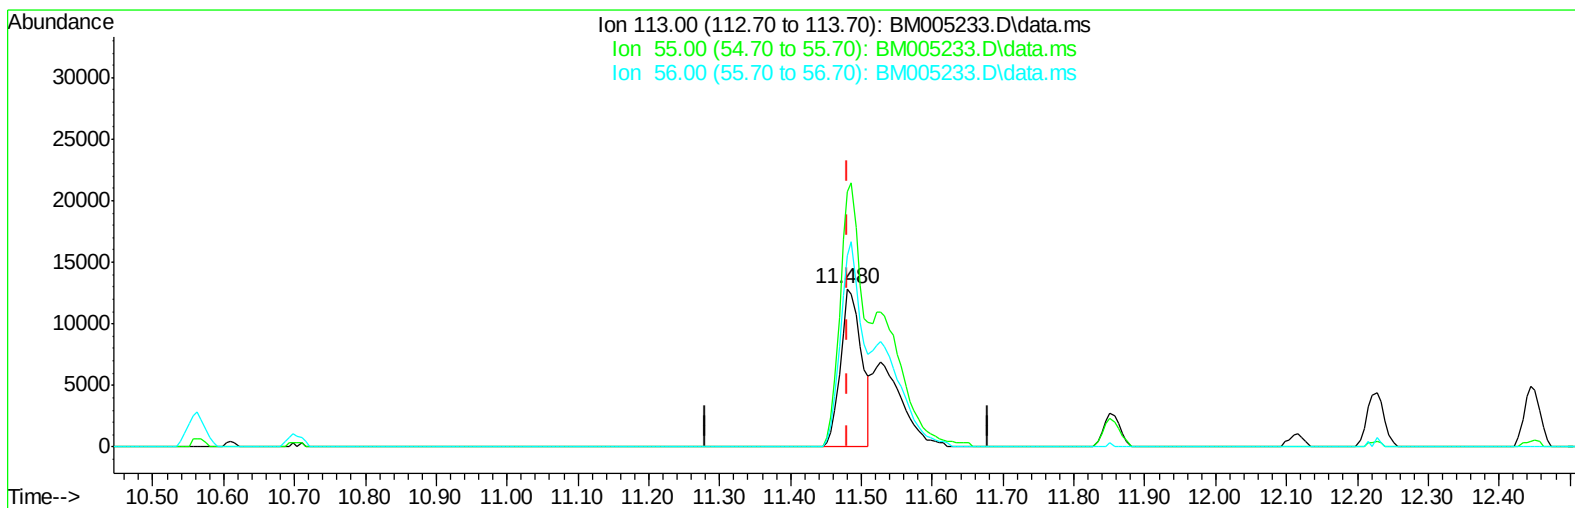

TIC: BM005233.D\data.ms

(32) Caprolactam




11.480min (0.000) 12.53 ng/ul

response 26716

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 168.20 | 161.31 |
| 56.00  | 120.80 | 120.84 |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\HPCHEM1\BNA M\Data\BM050516\  
Data File : BM005233.D  
Acq On : 05 May 2016 12:21  
Operator : UM/SJ  
Sample : SSTD02042  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 05 13:42:18 2016  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu May 05 13:39:01 2016  
Response via : Initial Calibration

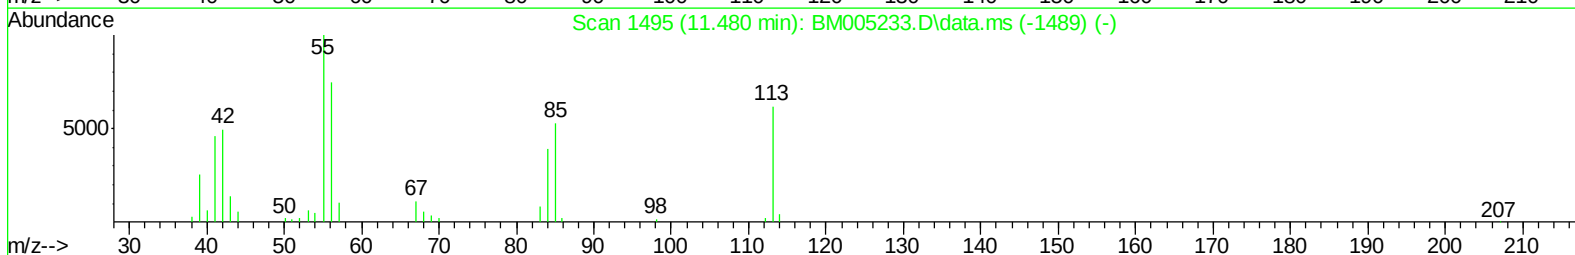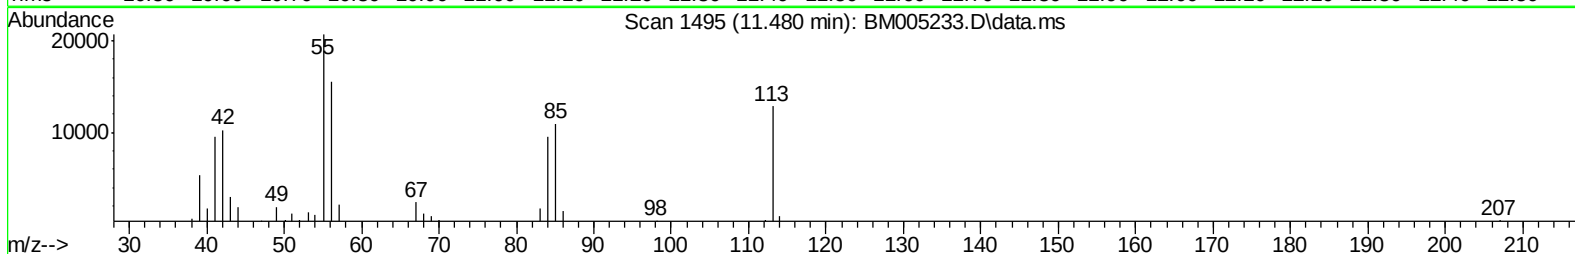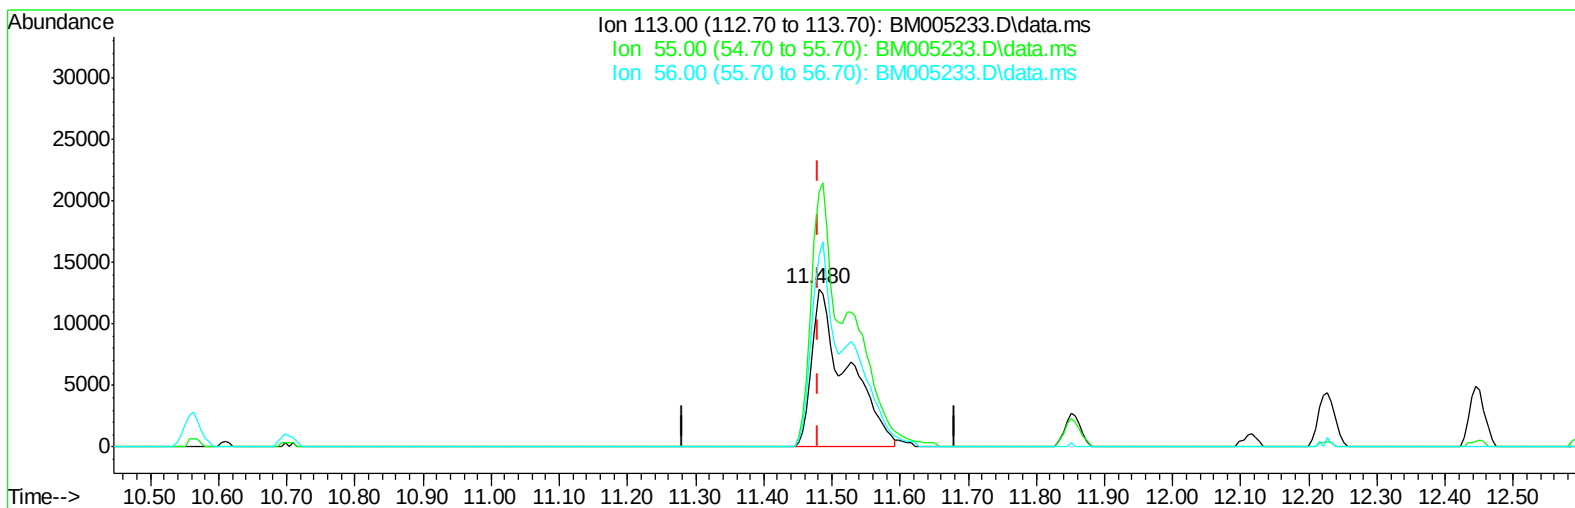

TIC: BM005233.D\data.ms

(32) Caprolactam

11.480min (0.000) 21.73 ng/ul m

response 46330

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 168.20 | 161.31 |
| 56.00  | 120.80 | 120.84 |
| 0.00   | 0.00   | 0.00   |