

(QT Reviewed)


```
Data Path   : Z:\HPCHEM1\BNA_M\Data\BM050516\  
Data File  : BM005236.D  
Acq On     : 05 May 2016   15:53  
Operator   : UM/SJ  
Sample     : SSTD16045  
Misc       :  
ALS Vial   : 8      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
SSTD16045

Manual Integrations

sohil
5/6/2016 7:15:04 PM

Quant Time: May 05 16:34:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 05 14:34:52 2016
Response via : Initial Calibration

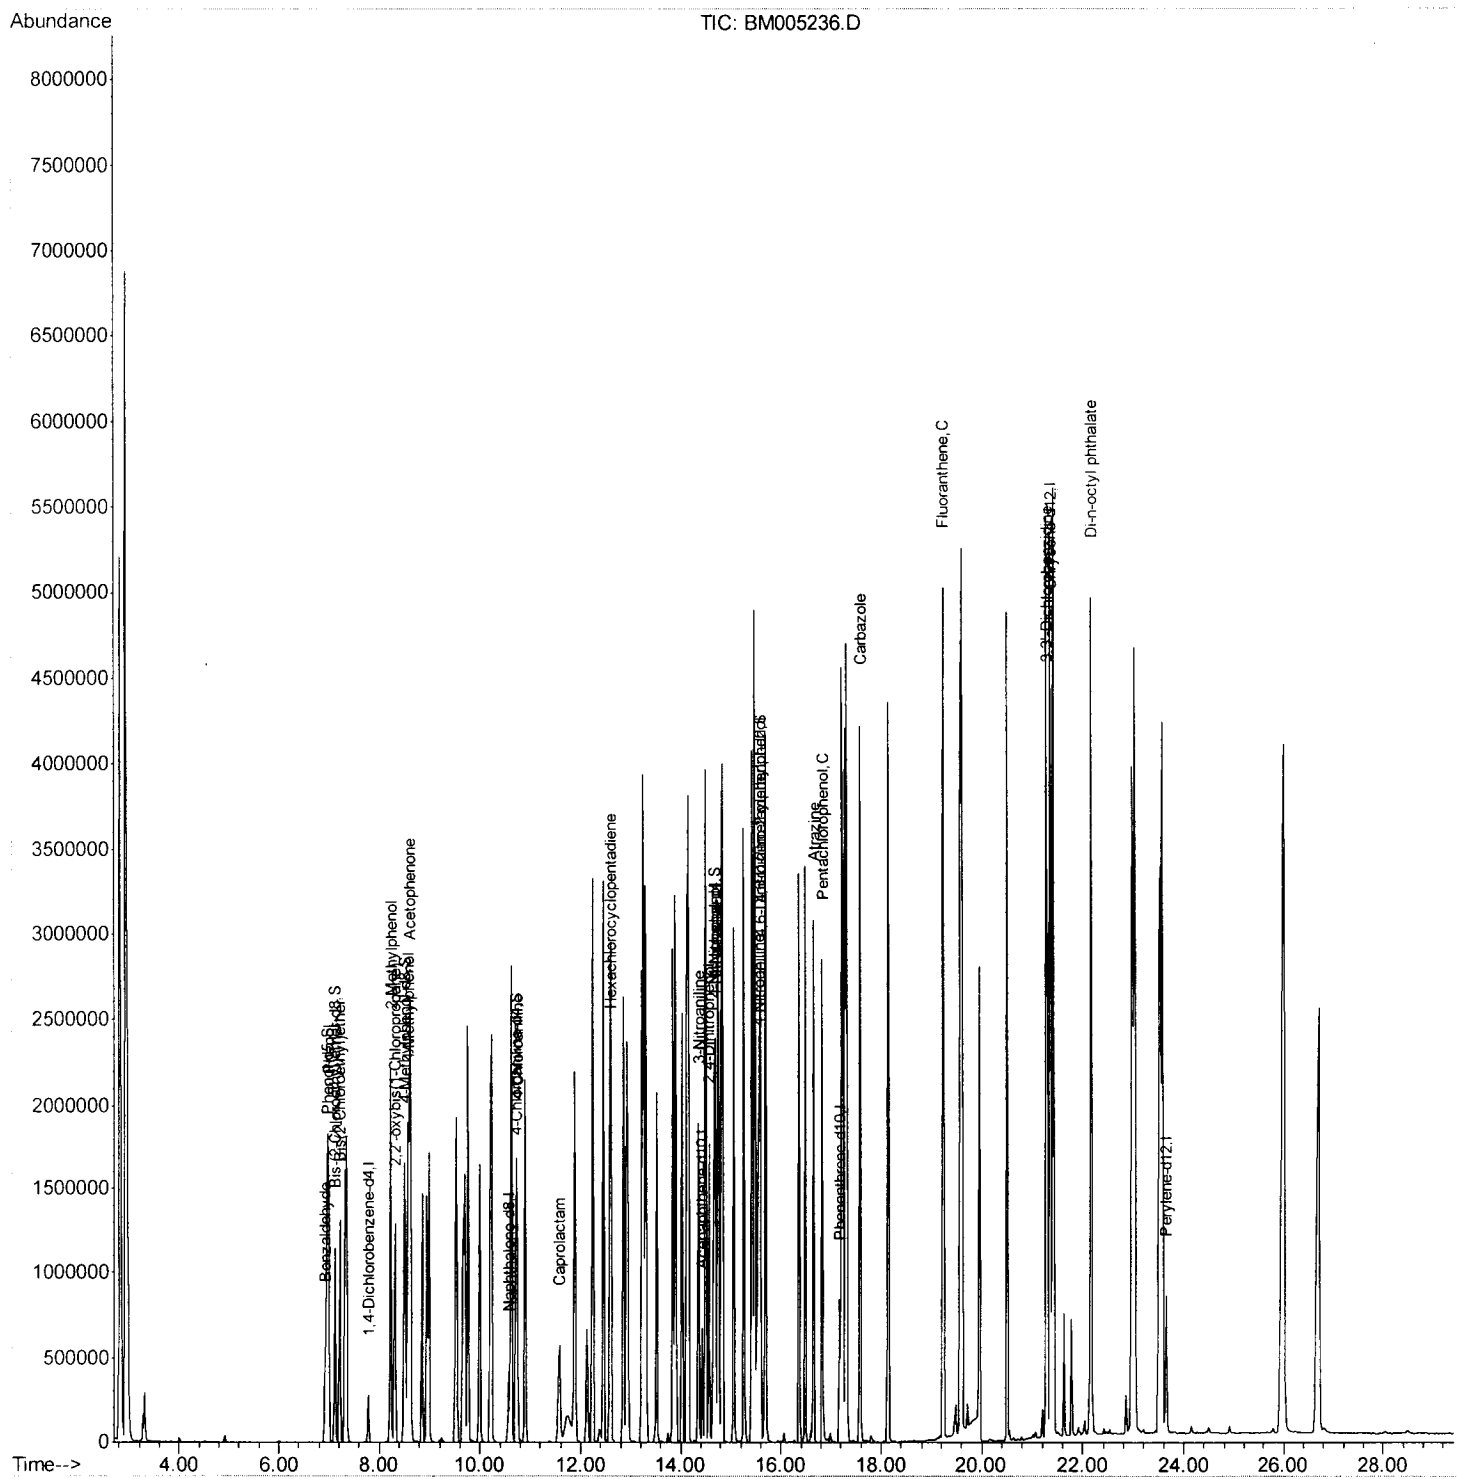

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
 Data File : BM005236.D
 Acq On : 05 May 2016 15:53
 Operator : UM/SJ
 Sample : SSTD16045
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16045

Manual Integrations
 APPROVED

sohil
 5/6/2016 7:15:04 PM

Quant Time: May 05 16:30:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 05 14:34:52 2016
 Response via : Initial Calibration

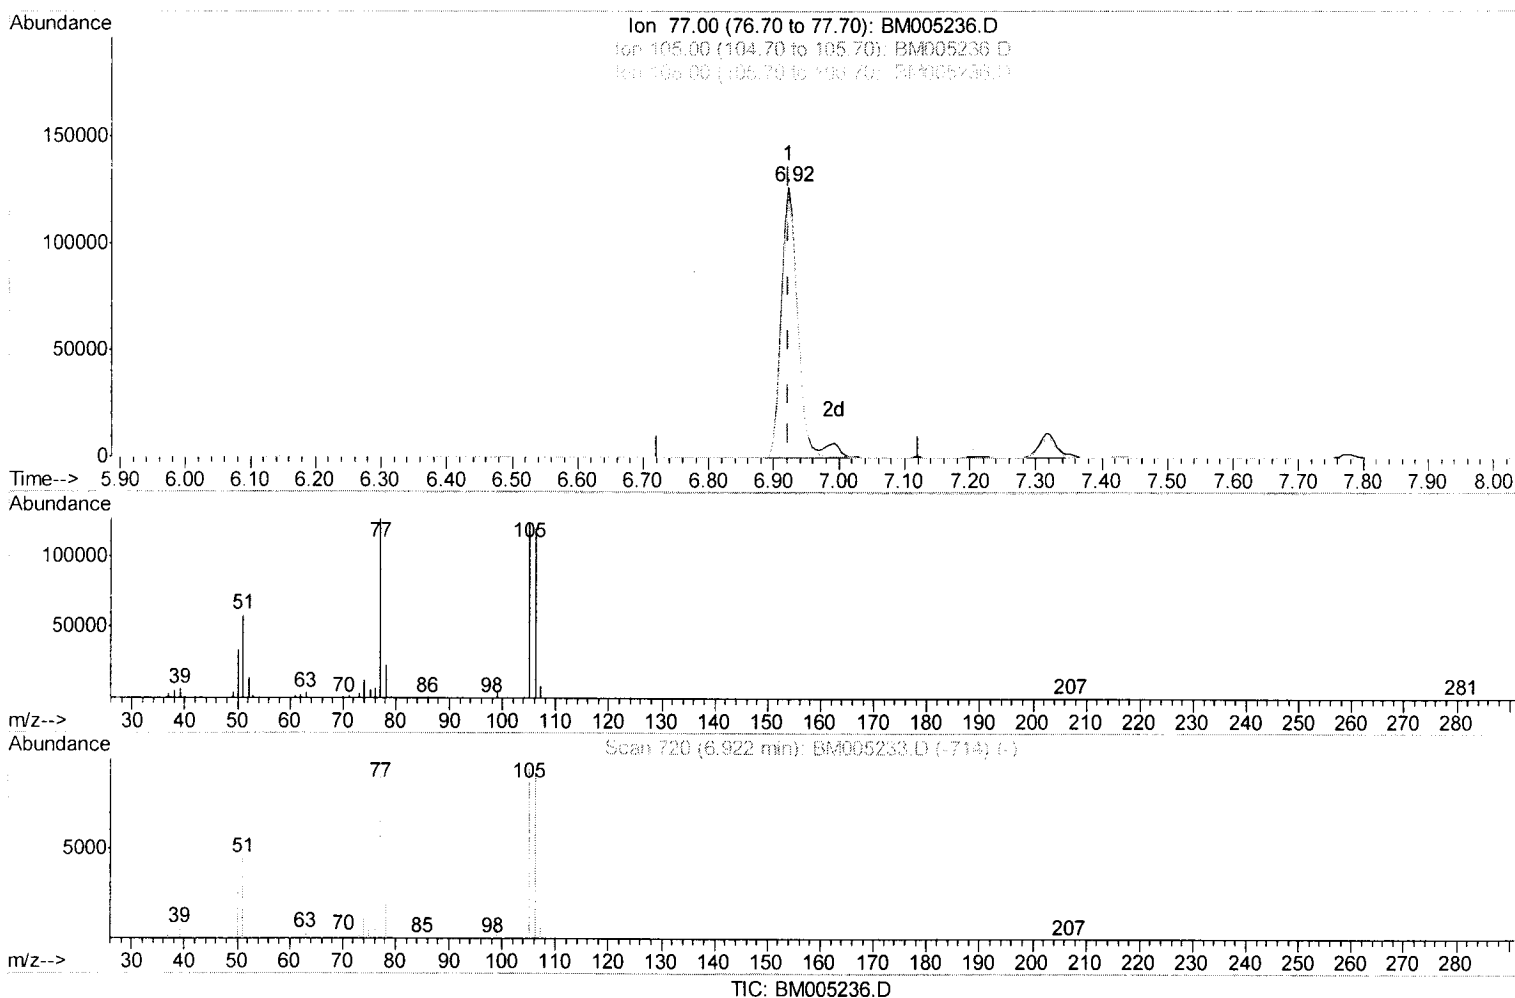

(4) Benzaldehyde

6.922min (+0.000) 70.51ng/ul m U.M

response 226824

Ion	Exp%	Act%
77.00	100	100
105.00	97.00	97.33
106.00	97.40	94.23
0.00	0.00	0.00

05/07/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
 Data File : BM005236.D
 Acq On : 05 May 2016 15:53
 Operator : UM/SJ
 Sample : SSTD16045
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16045

Quant Time: May 05 16:30:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 05 14:34:52 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 5/6/2016 7:15:04 PM

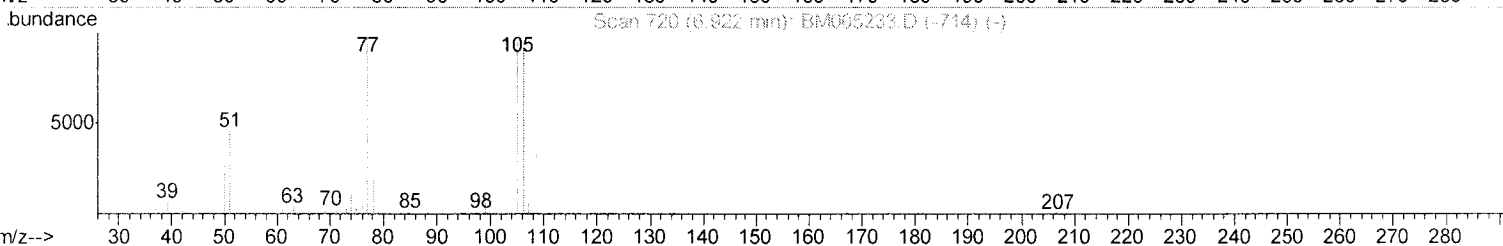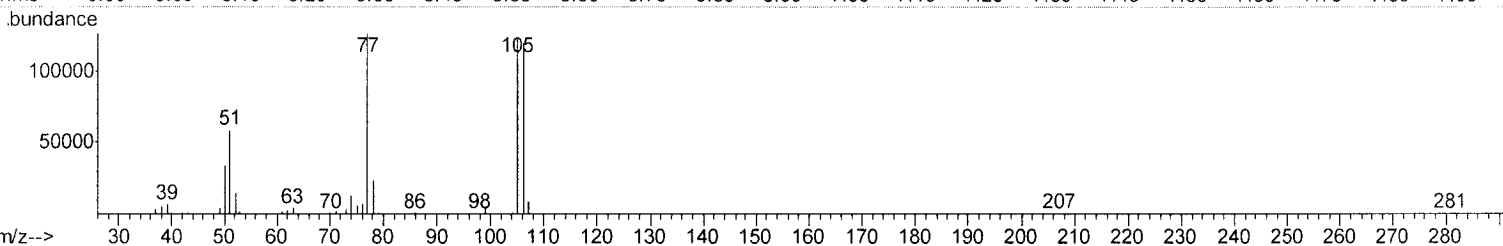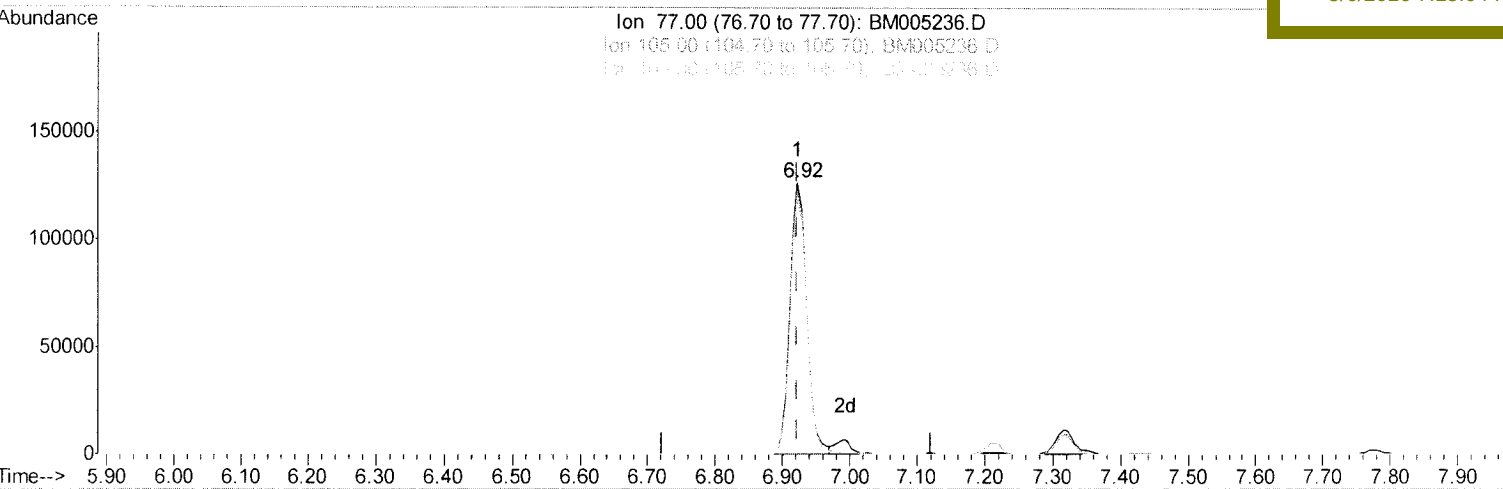

TIC: BM005236.D

(4) Benzaldehyde

6.922min (+0.000) 66.89ng/ul

response 215195

Ion	Exp%	Act%
77.00	100	100
105.00	97.00	97.33
106.00	97.40	94.23
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
 Data File : BM005236.D
 Acq On : 05 May 2016 15:53
 Operator : UM/SJ
 Sample : SSTD16045
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16045

Manual Integrations
 APPROVED

sohil
 5/6/2016 7:15:04 PM

Quant Time: May 05 16:30:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 05 14:34:52 2016
 Response via : Initial Calibration

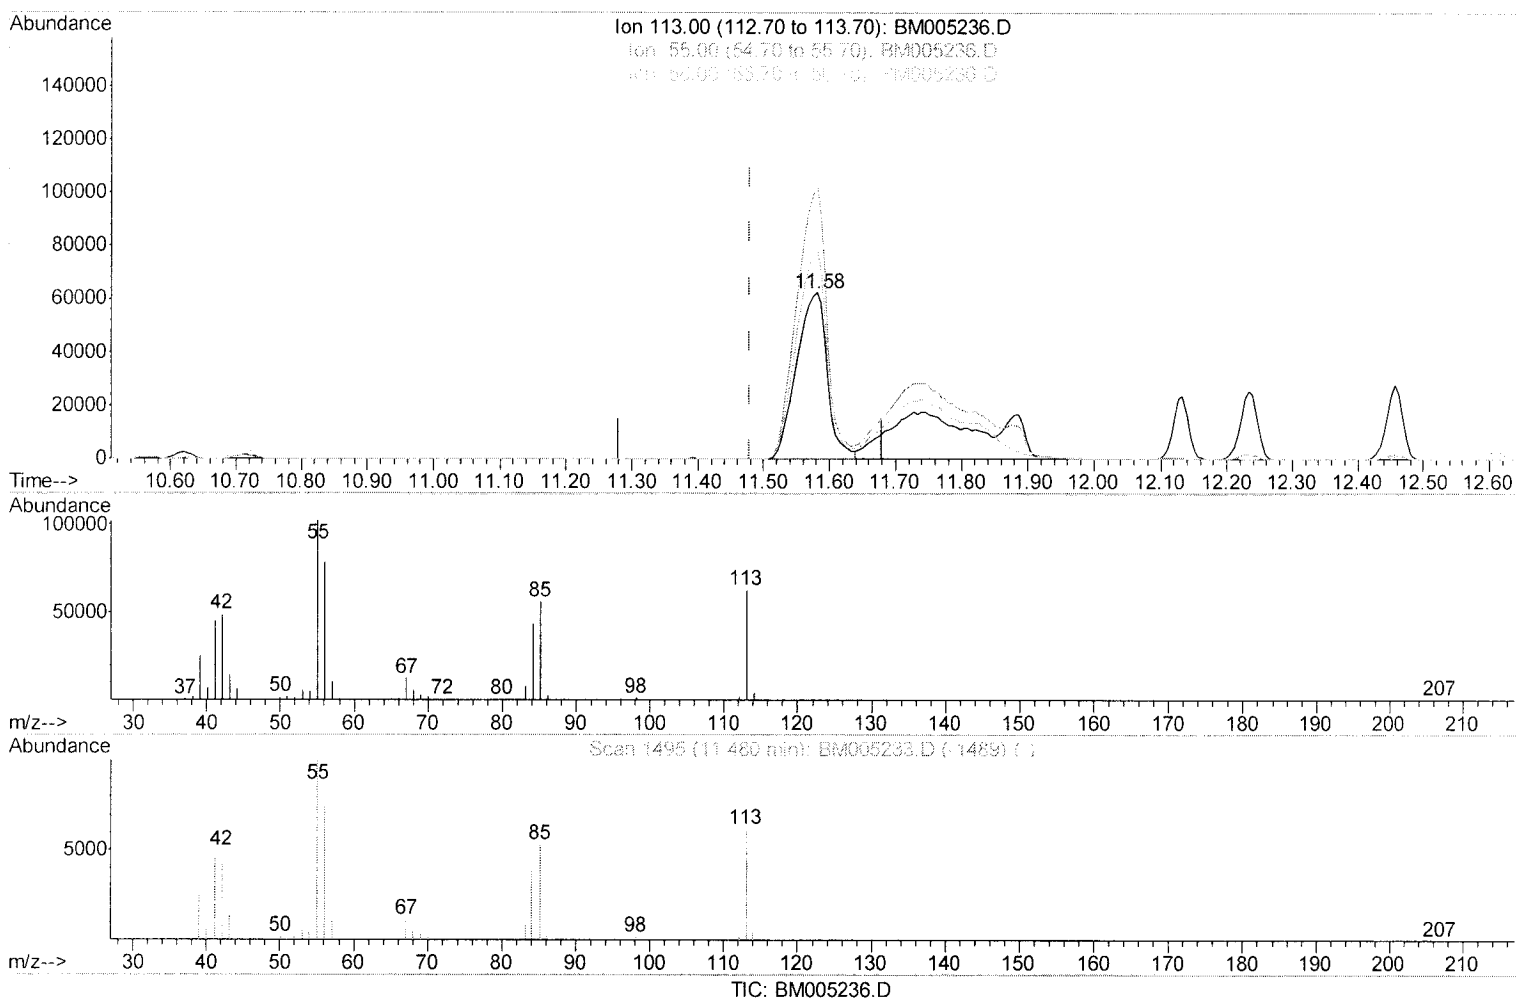

(32) Caprolactam

11.581min (+0.100) 94.71ng/ul

response 200962

Ion	Exp%	Act%
113.00	100	100
55.00	168.20	163.17
56.00	120.80	124.86
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
 Data File : BM005236.D
 Acq On : 05 May 2016 15:53
 Operator : UM/SJ
 Sample : SSTD16045
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD16045

Manual Integrations
APPROVED

sohil
 5/6/2016 7:15:04 PM

Quant Time: May 05 16:30:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 05 14:34:52 2016
 Response via : Initial Calibration

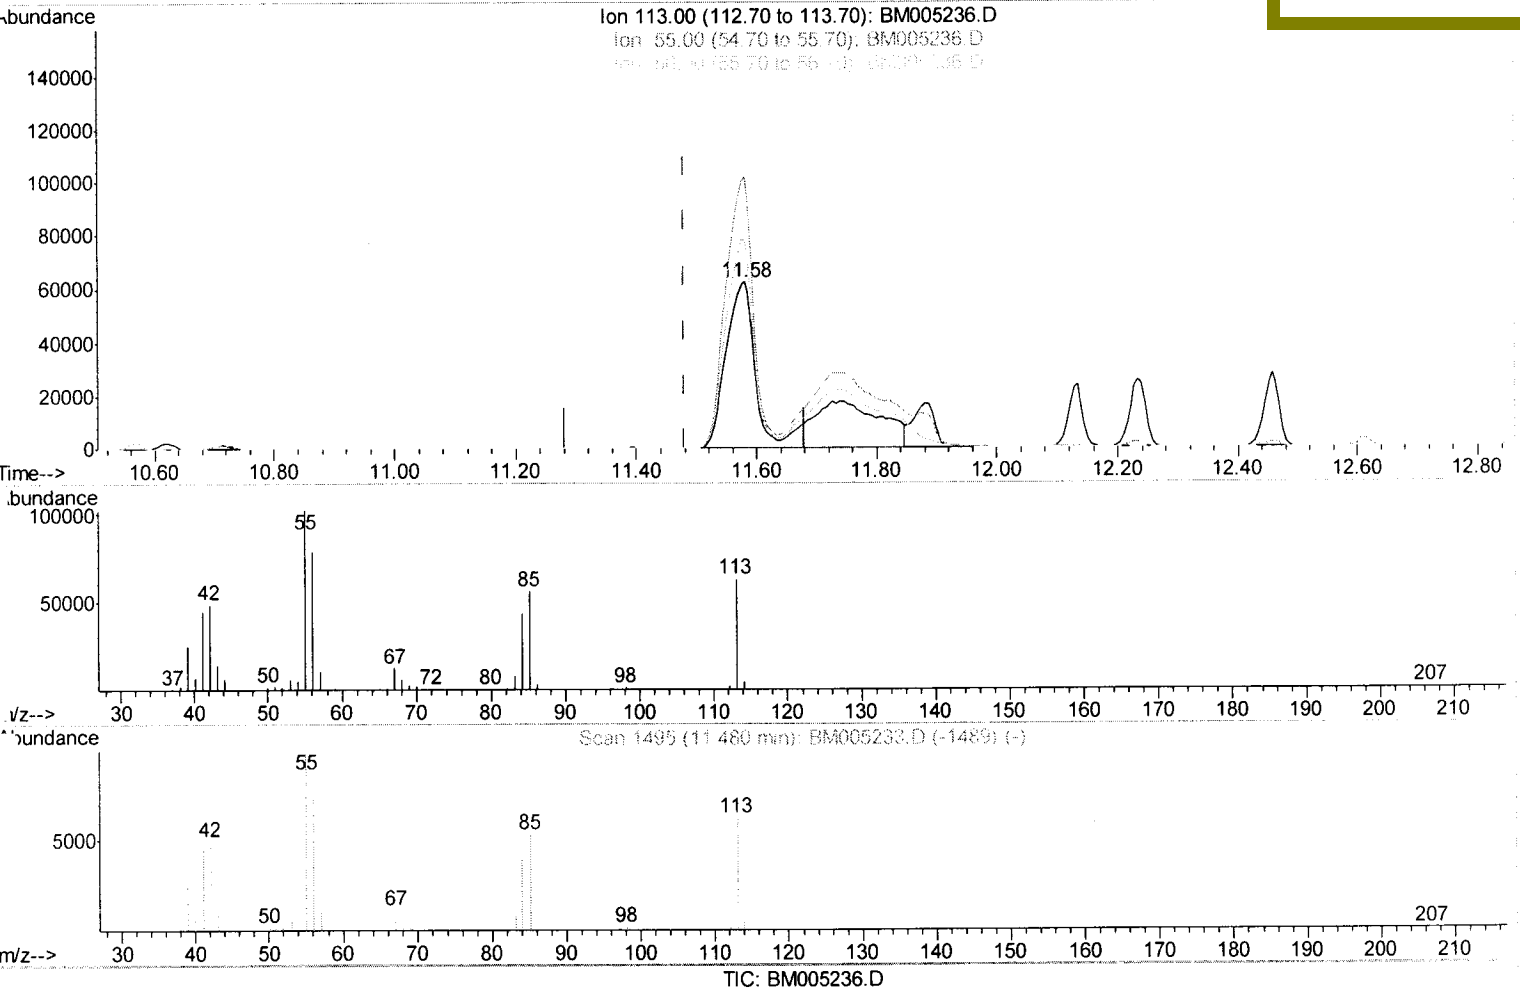

(32) Caprolactam

11.581min (+0.100) 163.70ng/ul m U.M
05/07/16
 response 347344

Ion	Exp%	Act%
113.00	100	100
55.00	168.20	163.17
56.00	120.80	124.86
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
 Data File : BM005236.D
 Acq On : 05 May 2016 15:53
 Operator : UM/SJ
 Sample : SSTD16045
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16045

Manual Integrations
 APPROVED

sohil
 5/6/2016 7:15:04 PM

Quant Time: May 05 16:34:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 05 14:34:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	75056	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	363283	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	233509	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	561822	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	497720	20.00	ng/ul	0.01
83) Perylene-d12	23.65	264	563686	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.96	99	1075165	158.15	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.12	67	567293	146.18	ng/ul	0.01
9) 2-Chlorophenol-d4	0.00	132	0d	0.00	ng/ul	
13) 4-Methylphenol-d8	8.50	113	886525	157.84	ng/ul	0.02
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.71	131	732409	111.84	ng/ul	0.00
43) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul	
51) 4-Nitrophenol-d4	14.67	143	537109	157.83	ng/ul	0.04
57) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
62) 4,6-Dinitro-2-methylphenol	15.57	200	509862	162.21	ng/ul	0.03
70) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
76) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
87) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	

Target Compounds

						Qvalue
4) Benzaldehyde	6.92	77	226824m	70.51	ng/ul	
6) Phenol	6.99	94	1085067	154.48	ng/ul	99
8) Bis(2-Chloroethyl)ether	7.22	93	768562	145.00	ng/ul	98
11) 2-Methylphenol	8.23	108	841458	155.00	ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.32	45	1027856	143.11	ng/ul	98
14) Acetophenone	8.61	105	1175531	141.43	ng/ul	99
16) 4-Methylphenol	8.58	108	923518	153.36	ng/ul	94
30) 4-Chloroaniline	10.74	127	757005	113.61	ng/ul	98
32) Caprolactam	11.58	113	347344m	163.70	ng/ul	
37) Hexachlorocyclopentadiene	12.58	237	626609	173.01	ng/ul	95
48) 3-Nitroaniline	14.36	138	569448	145.96	ng/ul	99
50) 2,4-Dinitrophenol	14.56	184	428328	202.75	ng/ul	93
52) 4-Nitrophenol	14.69	109	445714	157.24	ng/ul	92
60) 4-Nitroaniline	15.54	138	639334	154.35	ng/ul	93
63) 4,6-Dinitro-2-methylphenol	15.59	198	522473	157.93	ng/ul#	87
67) Atrazine	16.66	200	758834	135.68	ng/ul	99
68) Pentachlorophenol	16.83	266	558124	166.98	ng/ul	97
72) Carbazole	17.59	167	3315288	128.31	ng/ul	98
74) Fluoranthene	19.24	202	3900552	119.85	ng/ul	96
79) 3,3'-Dichlorobenzidine	21.29	252	1289339	144.50	ng/ul	98
84) Di-n-octyl phthalate	22.17	149	4331133	131.76	ng/ul#	94

U.M
 05/07/16

Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
Data File : BM005236.D
Acq On : 05 May 2016 15:53
Operator : UM/SJ
Sample : SSTD16045
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD16045

Quant Time: May 05 16:34:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 05 14:34:52 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
5/6/2016 7:15:04 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
--------------------	------	------	----------	------	-------	-----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed