

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
 Data File : BM005271.D
 Acq On : 06 May 2016 15:53
 Operator : UM/SJ
 Sample : H2813-10DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7S8DL

Quant Time: May 06 17:28:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 04:26:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	75610	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	373607	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	259999	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	638409	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	766442	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	717420	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.96	99	2464	0.36	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.11	67	10133	2.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.31	132	9294	1.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	5479	0.97	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	5002	1.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	5239	1.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	11102	1.98	ng/ul	0.01
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.82	166	55039	2.64	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	62010	2.54	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.40	176	54460	3.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	3326	0.93	ng/ul	0.00
70) Anthracene-d10	17.26	188	87834	3.11	ng/ul	0.00
76) Pyrene-d10	19.56	212	103791	2.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	91916	2.89	ng/ul	0.00

Target Compounds


						Qvalue
28) Naphthalene	10.61	128	726727	38.66	ng/ul	99
34) 2-Methylnaphthalene	12.22	142	176355	12.54	ng/ul	99
40) 1,1'-Biphenyl	13.25	154	37920	1.84	ng/ul	98
49) Acenaphthene	14.47	153	125239	7.35	ng/ul	99
53) Dibenzofuran	14.81	168	110336	4.46	ng/ul	99
58) Fluorene	15.46	166	80786	4.18	ng/ul	98
69) Phenanthrene	17.20	178	178342	5.31	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005271.D
Acq On : 06 May 2016 15:53
Operator : UM/SJ
Sample : H2813-10DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7S8DL

Quant Time: May 06 17:28:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 04:26:22 2016
Response via : Initial Calibration




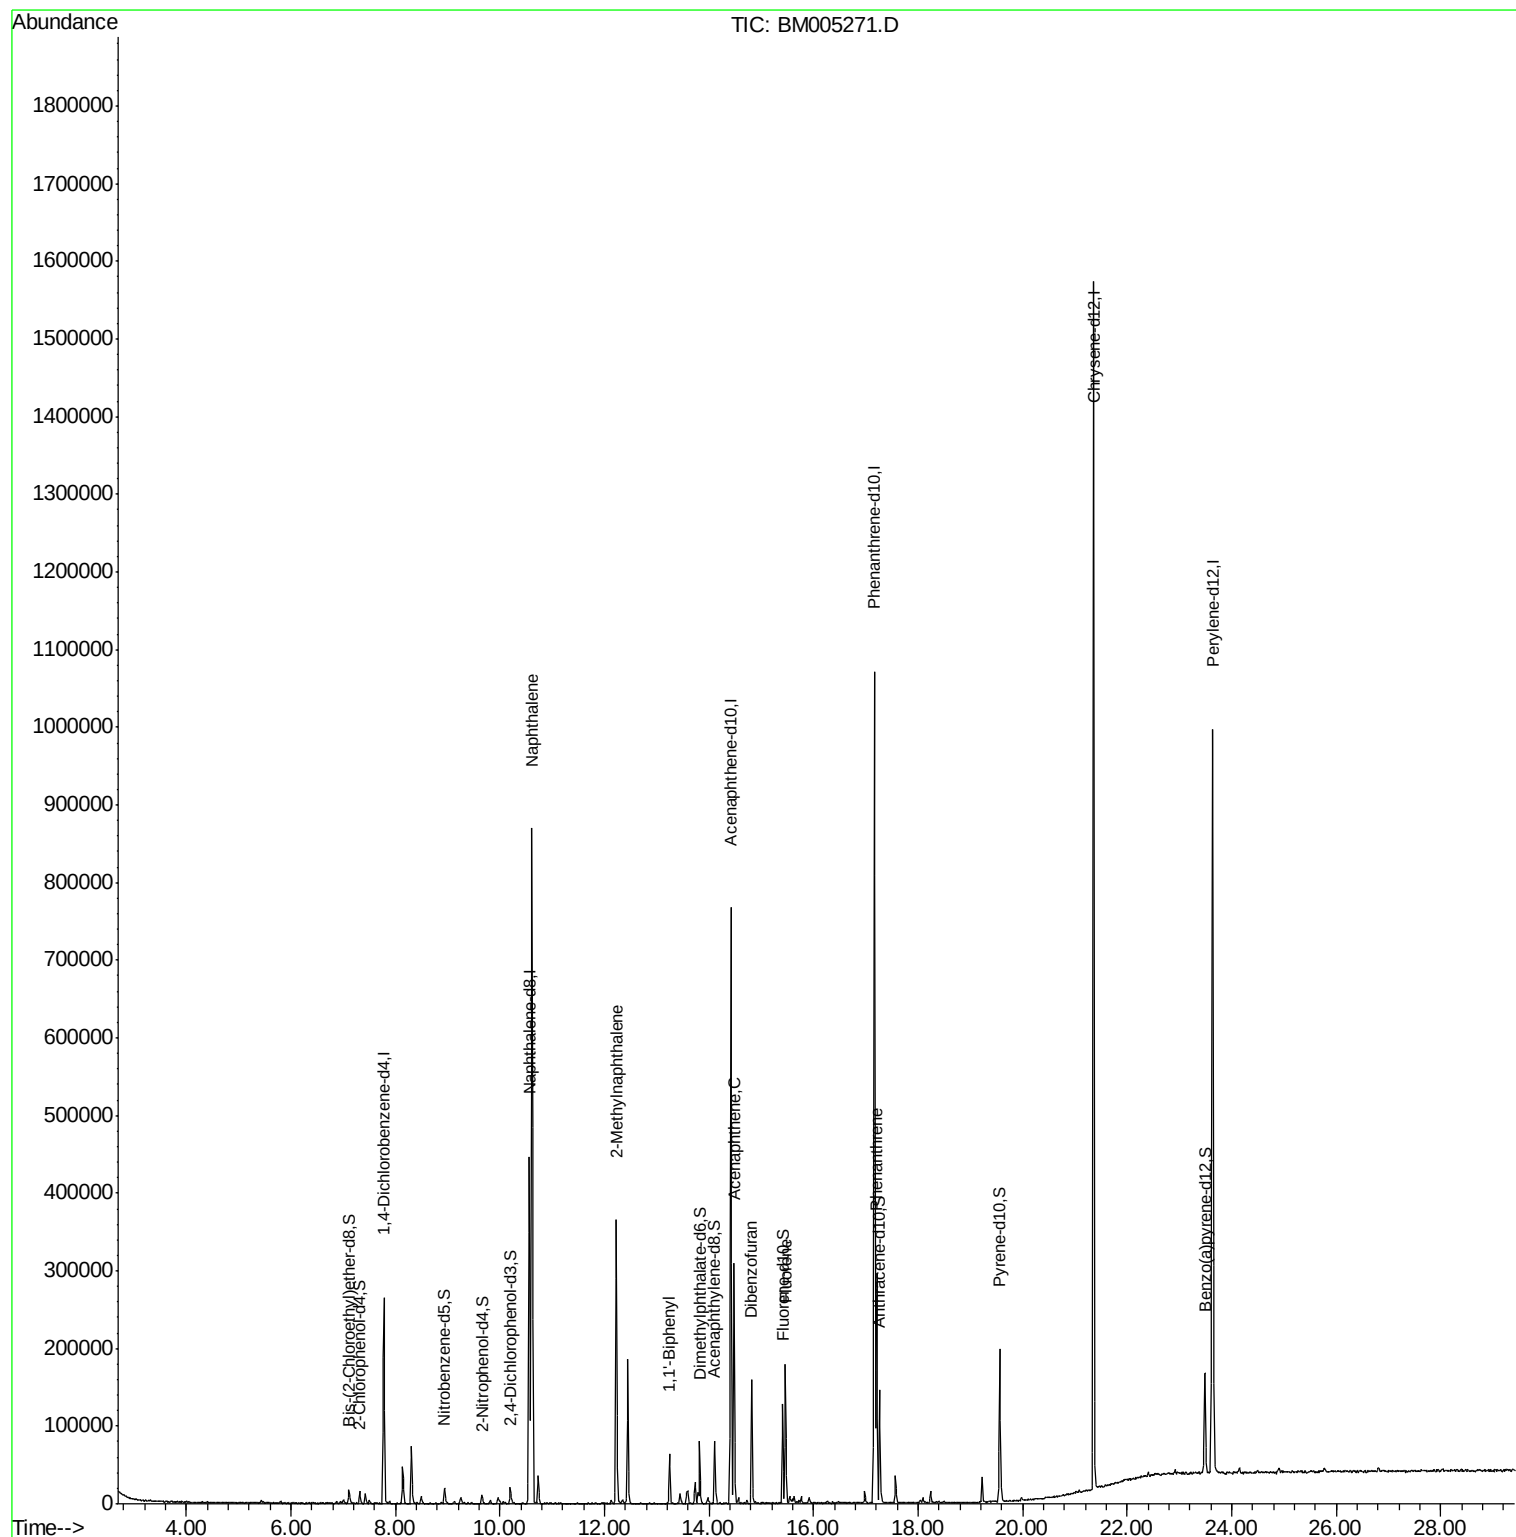


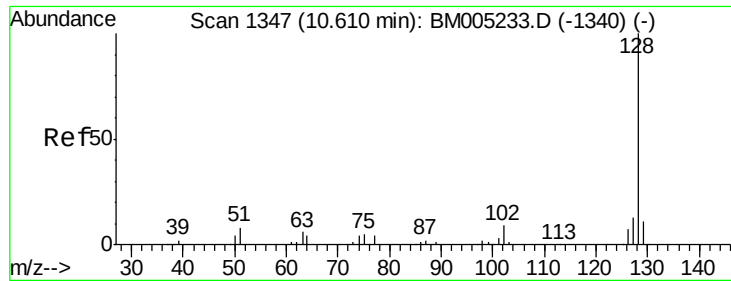

#28
Naphthalene
Concen: 38.66 ng/ul
RT: 10.61 min Scan# 1347
Delta R.T. 0.00 min
Lab File: BM005271.D
Acq: 06 May 2016 15:53




Instrument :
BNA_M
ClientSampleId :
BC7S8DL


Tgt Ion:128 Resp: 726727
Ion Ratio Lower Upper
128 100
129 10.9 8.4 12.6
127 13.4 10.8 16.2

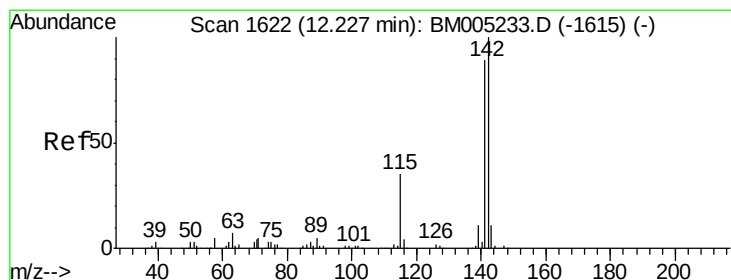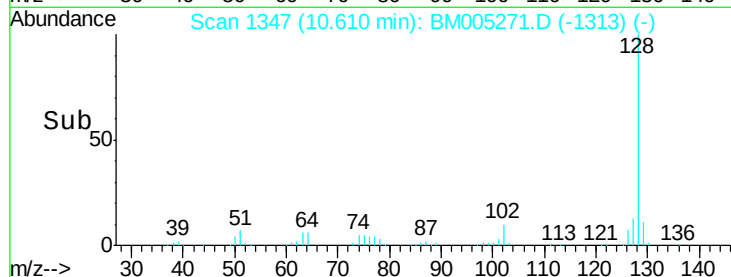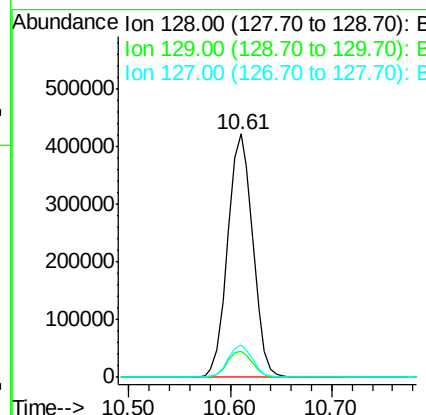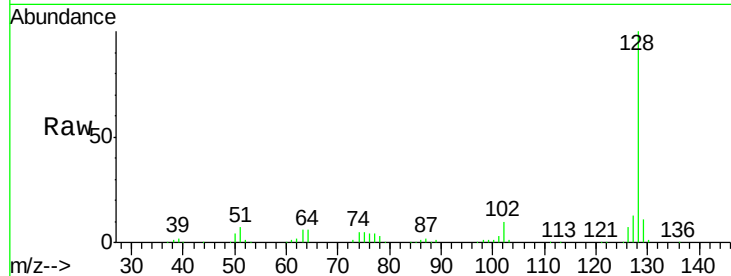

#34
2-Methylnaphthalene
Concen: 12.54 ng/ul
RT: 12.22 min Scan# 1621
Delta R.T. -0.01 min
Lab File: BM005271.D
Acq: 06 May 2016 15:53

Tgt Ion:142 Resp: 176355
Ion Ratio Lower Upper
142 100
141 87.7 71.3 106.9


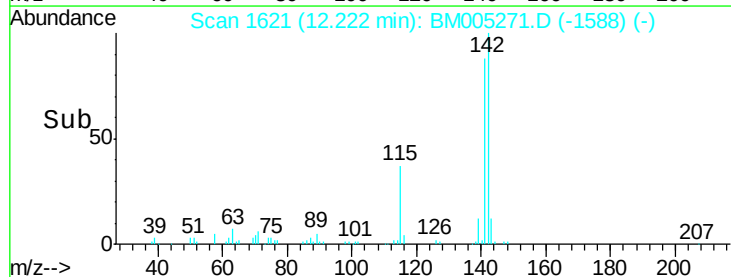
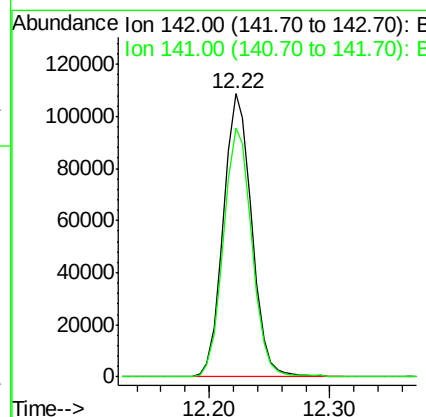
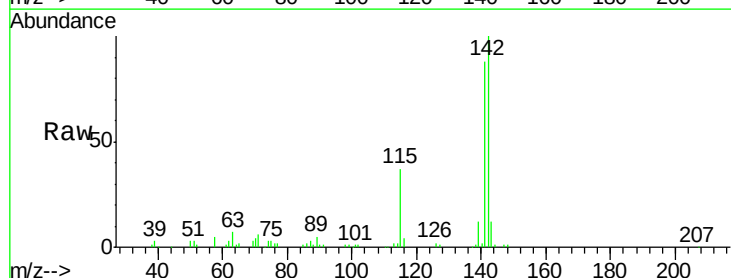


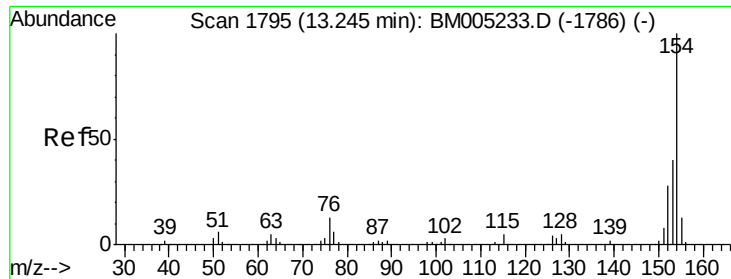

#40
 1,1'-Biphenyl
 Concen: 1.84 ng/ul
 RT: 13.25 min Scan# 1795
 Delta R.T. 0.00 min
 Lab File: BM005271.D
 Acq: 06 May 2016 15:53




Instrument :
 BNA_M
 ClientSampleId :
 BC7S8DL


Tgt Ion:154 Resp: 37920
 Ion Ratio Lower Upper
 154 100
 153 39.0 32.1 48.1
 76 12.3 10.6 15.8

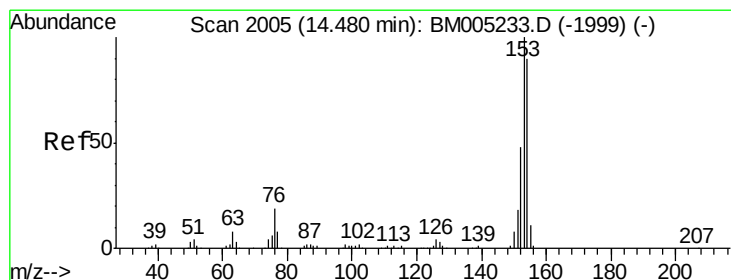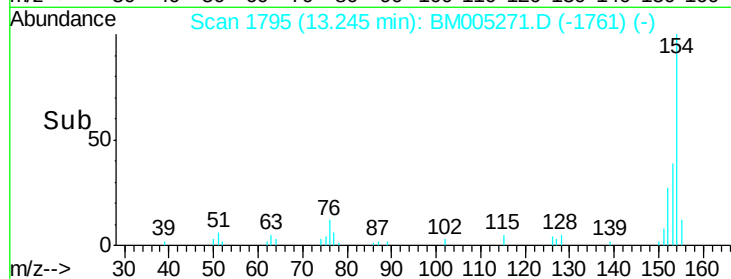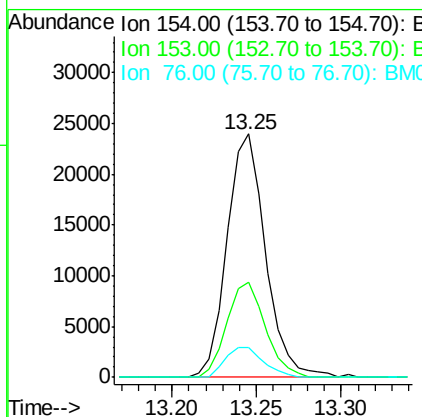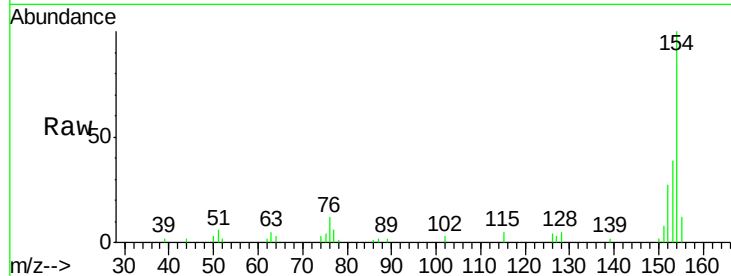

#49
 Acenaphthene
 Concen: 7.35 ng/ul
 RT: 14.47 min Scan# 2004
 Delta R.T. -0.01 min
 Lab File: BM005271.D
 Acq: 06 May 2016 15:53

Tgt Ion:153 Resp: 125239
 Ion Ratio Lower Upper
 153 100
 152 48.1 38.9 58.3
 154 89.4 70.3 105.5

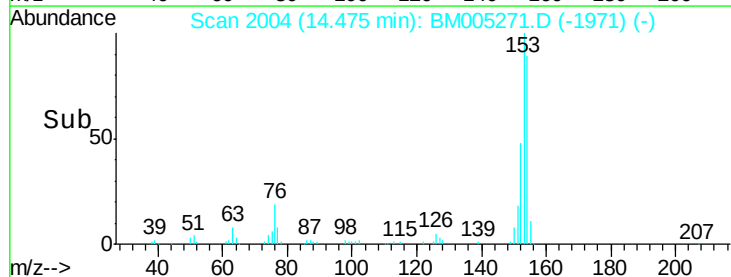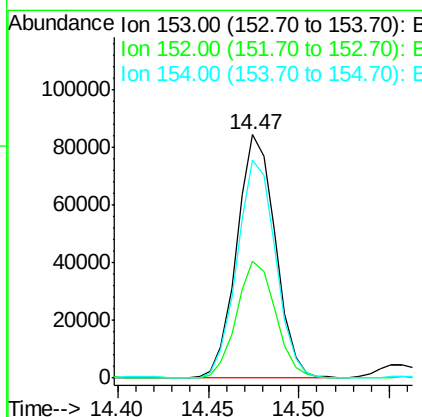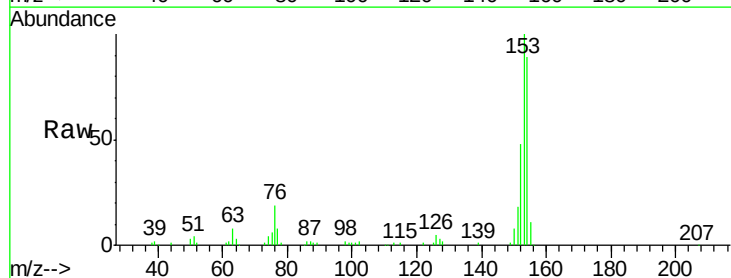

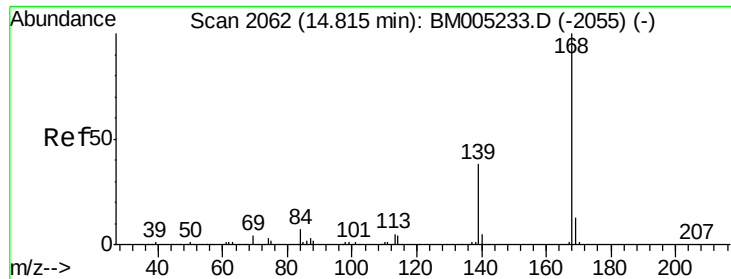

#53

Dibenzenofuran

Concen: 4.46 ng/ul

RT: 14.81 min Scan# 2061

Delta R.T. -0.01 min

Lab File: BM005271.D

Acq: 06 May 2016 15:53

Instrument :

BNA_M

ClientSampleId :


BC7S8DL

Tgt Ion:168 Resp: 110336

Ion Ratio Lower Upper

168 100

139 37.1 30.3 45.5

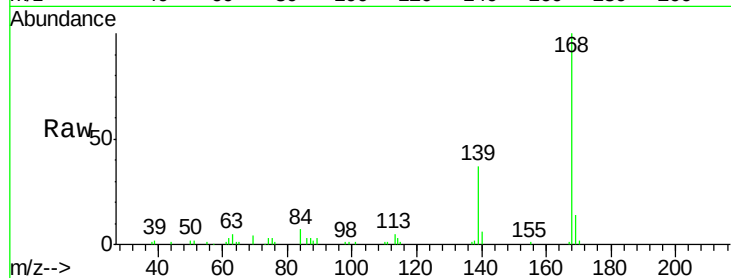

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.81

80000

60000



40000

20000

0

14.75 14.80 14.85

Time-->

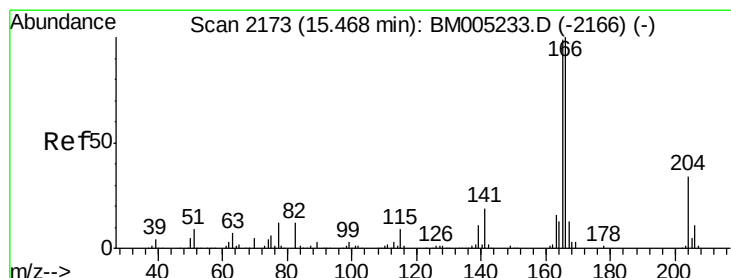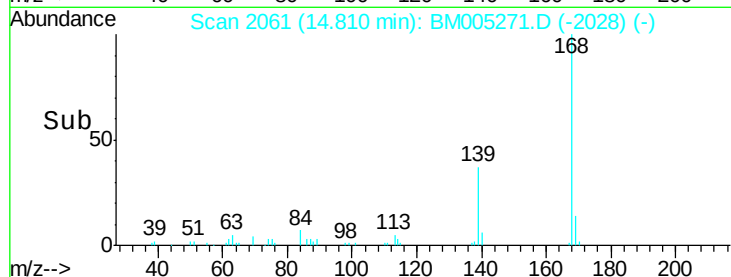

#58

Fluorene

Concen: 4.18 ng/ul

RT: 15.46 min Scan# 2172

Delta R.T. -0.01 min

Lab File: BM005271.D

Acq: 06 May 2016 15:53


Tgt Ion:166 Resp: 80786

Ion Ratio Lower Upper

166 100

165 95.8 77.9 116.9

167 14.4 10.6 16.0

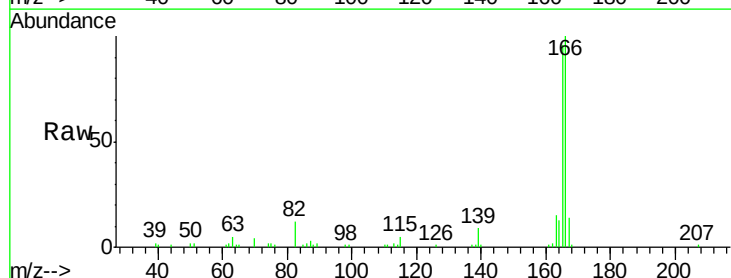

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.46

60000


40000


20000

0

15.40 15.45 15.50

Time-->

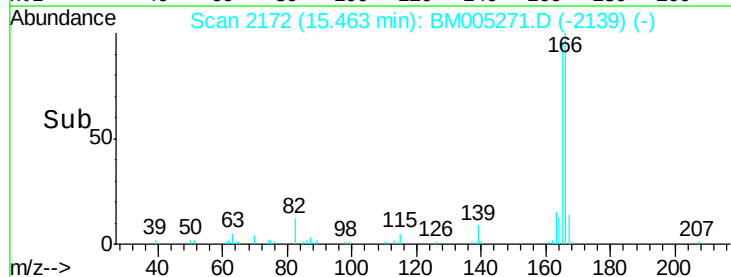

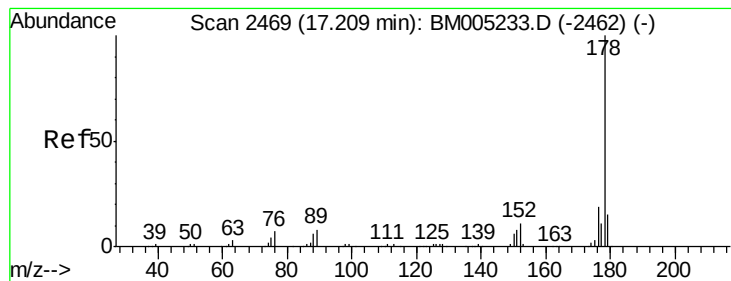

#69

Phenanthrene

Concen: 5.31 ng/ul

RT: 17.20 min Scan# 2468

Delta R.T. -0.01 min

Lab File: BM005271.D


Acq: 06 May 2016 15:53

Instrument :

BNA_M

ClientSampleId :

BC7S8DL

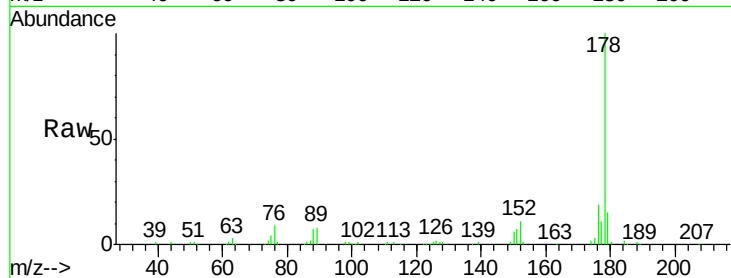


Tgt Ion:178 Resp: 178342

Ion Ratio Lower Upper

178 100

179 15.1 12.3 18.5

176 18.8 15.2 22.8

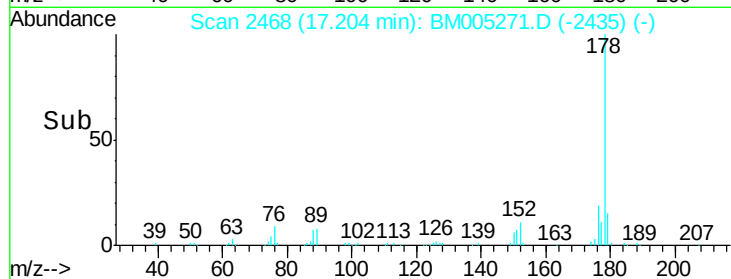

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

