

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
 Data File : BM005260.D
 Acq On : 06 May 2016 08:35
 Operator : UM/SJ
 Sample : H2813-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC810

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.945	719	724	732	rBV	72609	118793	4.10%	0.471%
2	7.104	745	751	765	rVB	262612	410122	14.14%	1.625%
3	7.304	779	785	795	rBV	266002	432278	14.90%	1.713%
4	7.775	855	865	876	rBV	290386	485501	16.74%	1.924%
5	8.475	979	984	1003	rVB	236922	382363	13.18%	1.515%
6	8.928	1055	1061	1075	rBV	327818	547324	18.87%	2.169%
7	9.645	1177	1183	1194	rBV	279545	462498	15.95%	1.833%
8	10.181	1268	1274	1293	rBV	393099	693153	23.90%	2.747%
9	10.557	1331	1338	1346	rBV	467144	796674	27.47%	3.157%
10	13.821	1887	1893	1901	rBV	906385	1296499	44.70%	5.137%
11	14.104	1935	1941	1953	rBV	993158	1508925	52.03%	5.979%
12	14.416	1987	1994	2003	rVB2	788103	1214549	41.88%	4.812%
13	14.627	2025	2030	2047	rBV	49630	97515	3.36%	0.386%
14	15.410	2156	2163	2170	rBV	1363420	2013750	69.43%	7.979%
15	15.533	2179	2184	2199	rBV	457525	624362	21.53%	2.474%
16	17.162	2455	2461	2467	rBV2	1113426	1598154	55.10%	6.332%
17	17.262	2472	2478	2494	rVB	1595795	2311612	79.70%	9.159%
18	19.562	2863	2869	2882	rBV2	2028133	2848870	98.23%	11.288%
19	21.362	3169	3175	3187	rBV	1597082	2168919	74.78%	8.594%
20	22.409	3349	3353	3358	rBV2	31861	44935	1.55%	0.178%
21	22.921	3436	3440	3444	rVB2	28655	38368	1.32%	0.152%
22	23.491	3529	3537	3550	rBV2	1457554	2900227	100.00%	11.492%
23	23.638	3554	3562	3573	rVB2	1076643	2070384	71.39%	8.204%
24	24.144	3643	3648	3657	rVB2	43079	83977	2.90%	0.333%
25	24.903	3771	3777	3784	rVB	41992	87870	3.03%	0.348%


Sum of corrected areas: 25237622

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005260.D
Acq On : 06 May 2016 08:35
Operator : UM/SJ
Sample : H2813-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC810

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

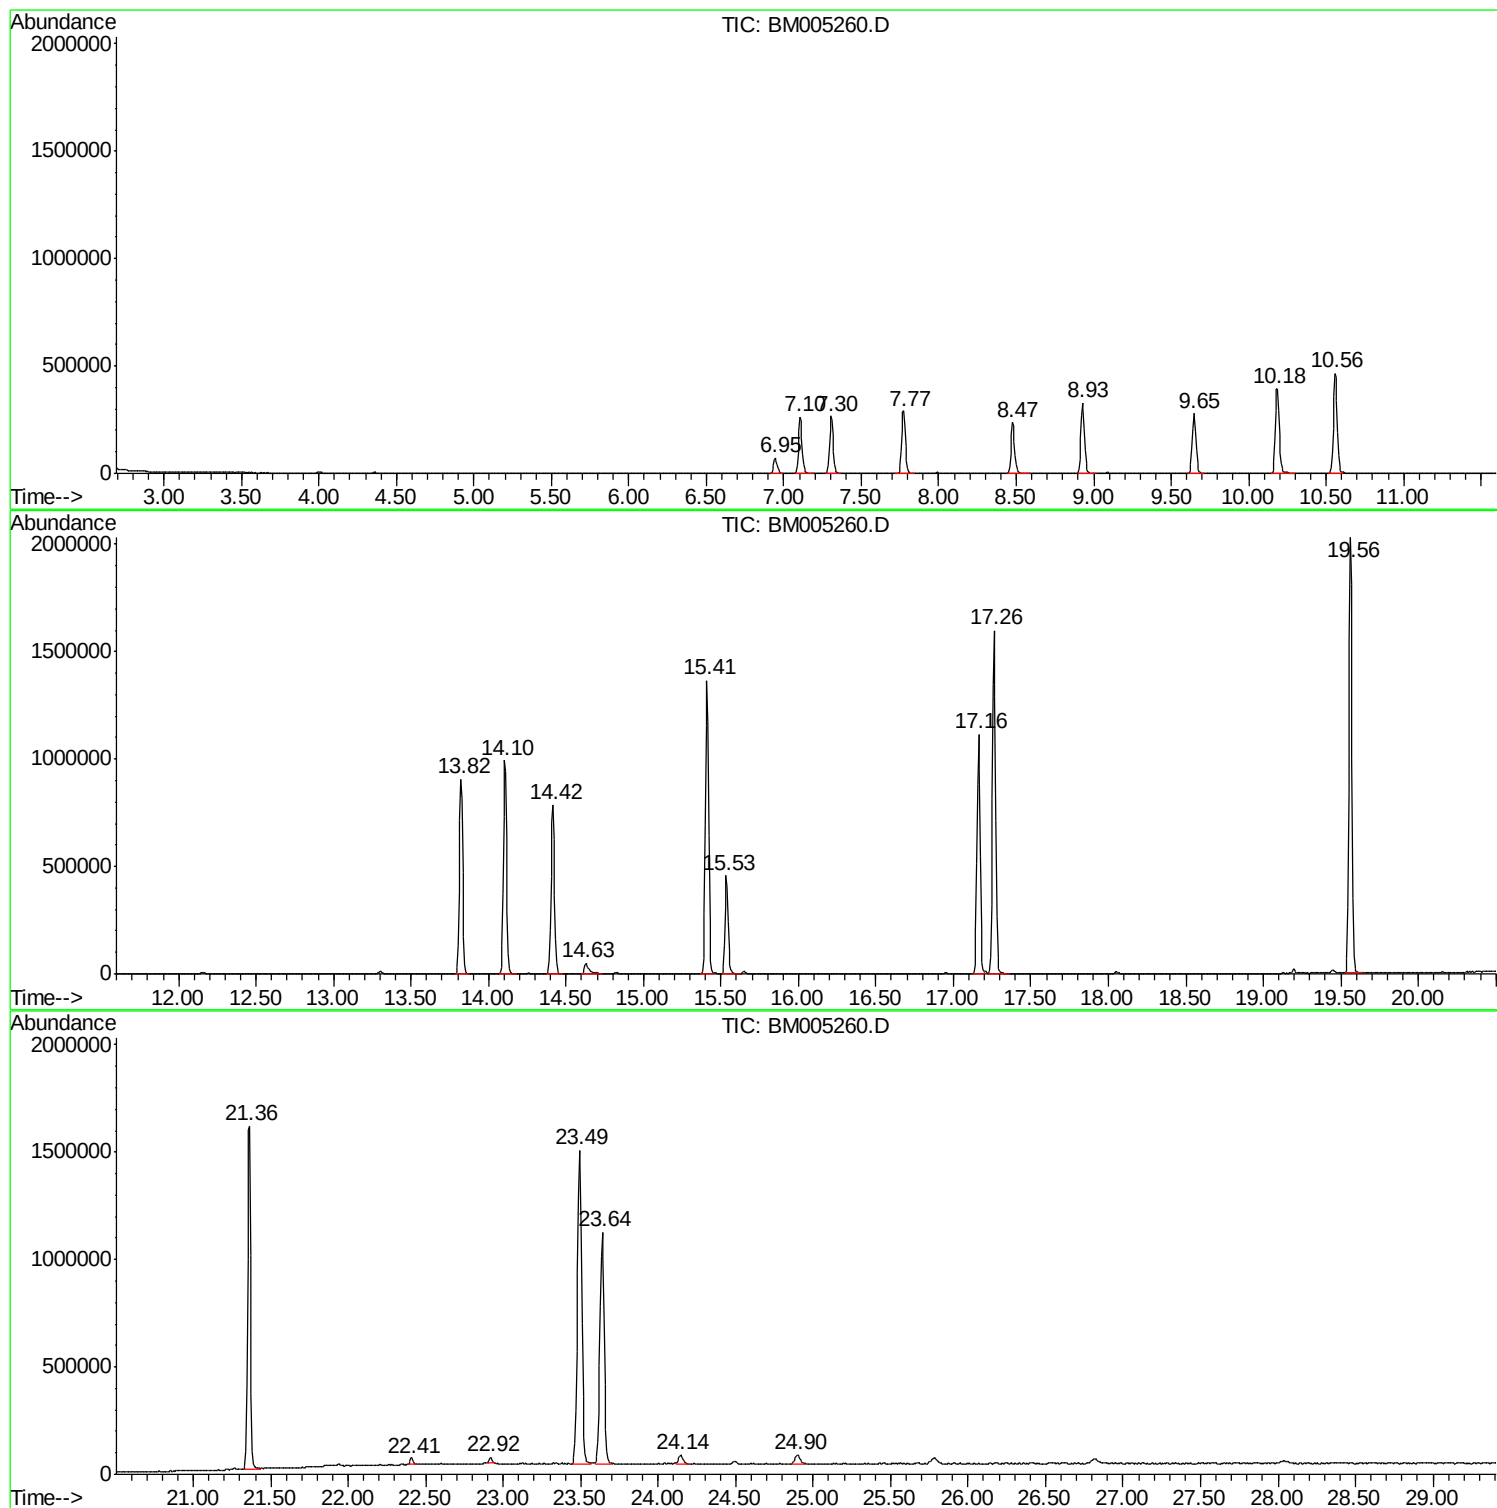

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005260.D
Acq On : 06 May 2016 08:35
Operator : UM/SJ
Sample : H2813-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC810

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005260.D
Acq On : 06 May 2016 08:35
Operator : UM/SJ
Sample : H2813-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC810

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc