

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
 Data File : BM005261.D
 Acq On : 06 May 2016 09:11
 Operator : UM/SJ
 Sample : H2813-18
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC811

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	719	724	735	rVB	65265	105977	3.52%	0.421%
2	7.104	745	751	764	rBV	271839	431385	14.34%	1.713%
3	7.304	779	785	796	rBV	276681	440839	14.65%	1.751%
4	7.769	855	864	875	rVB	261725	439787	14.62%	1.747%
5	8.475	979	984	1000	rVB	223739	366011	12.16%	1.454%
6	8.928	1055	1061	1073	rBV	354487	573726	19.07%	2.279%
7	9.645	1177	1183	1193	rBV	297919	482939	16.05%	1.918%
8	10.181	1268	1274	1286	rBV	392487	700722	23.29%	2.783%
9	10.557	1331	1338	1345	rBV	435598	734887	24.42%	2.919%
10	13.822	1887	1893	1902	rBV	969030	1342915	44.63%	5.334%
11	14.104	1934	1941	1951	rBV	1042676	1571822	52.24%	6.243%
12	14.416	1987	1994	2001	rBV2	724691	1133561	37.67%	4.502%
13	14.627	2022	2030	2048	rBV	40463	86277	2.87%	0.343%
14	15.410	2156	2163	2170	rBV	1436031	2106138	70.00%	8.366%
15	15.533	2178	2184	2196	rBV	458569	646500	21.49%	2.568%
16	17.163	2454	2461	2466	rBV	1045926	1481036	49.22%	5.883%
17	17.262	2472	2478	2490	rVB	1629890	2392333	79.51%	9.502%
18	19.562	2862	2869	2885	rBV	2086367	2962219	98.45%	11.766%
19	21.356	3168	3174	3186	rBV	1570706	2008242	66.74%	7.977%
20	22.403	3348	3352	3359	rBV	43931	62099	2.06%	0.247%
21	22.915	3436	3439	3446	rVB	25399	33748	1.12%	0.134%
22	23.486	3528	3536	3553	rVB2	1522101	3008970	100.00%	11.952%
23	23.633	3553	3561	3573	rBV	1002605	1920635	63.83%	7.629%
24	24.139	3643	3647	3656	rVB	36557	66949	2.22%	0.266%
25	24.891	3771	3775	3785	rVB	36751	76607	2.55%	0.304%


Sum of corrected areas: 25176324

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005261.D
Acq On : 06 May 2016 09:11
Operator : UM/SJ
Sample : H2813-18
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC811

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

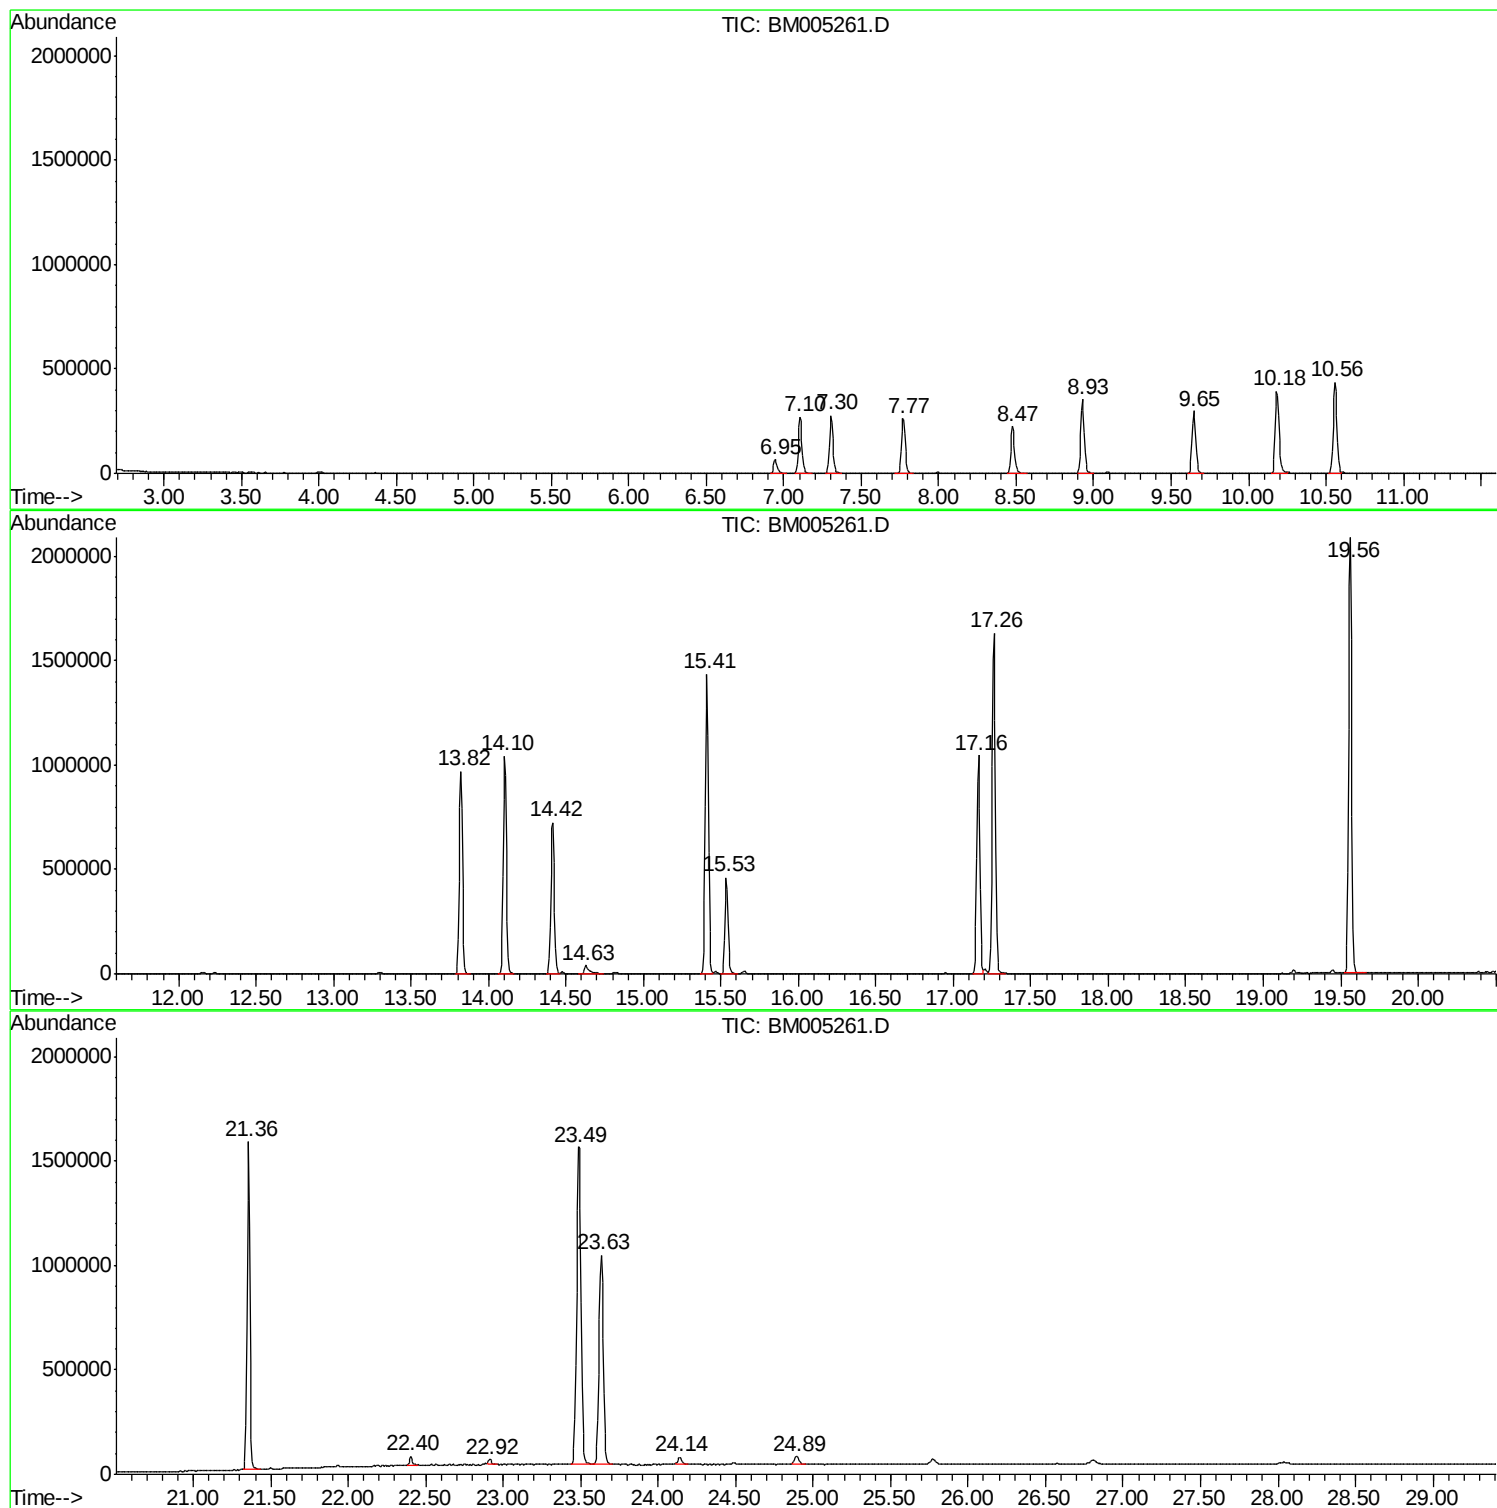

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005261.D
Acq On : 06 May 2016 09:11
Operator : UM/SJ
Sample : H2813-18
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC811

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050516\
Data File : BM005261.D
Acq On : 06 May 2016 09:11
Operator : UM/SJ
Sample : H2813-18
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC811

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc