

Scan 2530 (17.568 min): BM005230.D
DFTPP64

m/z	Abundance
44.00	519.0
47.00	617.0
49.00	2627.0
51.00	900.0
84.00	2048.0
86.00	1264.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.00	406.0
39.10	2380.0
44.00	354.0
47.00	345.0
49.00	2022.0
50.10	9141.0
51.10	36032.0
52.10	1876.0
56.00	1048.0
57.00	2579.0
61.00	451.0
62.00	500.0
63.00	1540.0
65.10	757.0
68.00	668.0
69.00	35840.0
73.00	405.0
74.10	3676.0
75.00	6149.0
76.10	2327.0
77.10	45112.0
78.10	3248.0
79.00	3053.0
80.00	2218.0
81.00	3242.0
82.00	790.0
83.00	823.0
84.00	1527.0
85.00	673.0
86.00	1887.0
87.00	423.0
87.90	327.0
91.00	611.0
92.00	752.0
93.00	5149.0
94.00	321.0
98.00	3964.0
99.00	3167.0
101.00	1833.0
103.00	496.0
104.00	1015.0
105.00	1090.0
106.10	351.0
107.00	13953.0
108.00	2163.0
109.10	387.0
110.00	25256.0
111.00	3942.0
112.00	505.0
116.00	742.0
117.00	11558.0
118.00	927.0
122.00	841.0
123.00	1346.0
124.00	594.0
124.90	662.0
126.20	322.0
127.10	46136.0
128.00	3539.0
129.00	17656.0
130.00	1569.0
134.00	527.0
135.00	1362.0
136.00	598.0
137.10	852.0
141.00	2457.0
142.00	837.0
143.00	495.0
146.00	405.0
147.00	1262.0
148.00	2869.0
149.00	595.0
151.00	303.0
153.00	823.0
154.00	542.0
155.00	1384.0
156.00	2064.0
157.10	395.0
158.00	465.0
159.00	309.0
160.00	736.0
161.00	1172.0
162.00	312.0
165.00	936.0
166.10	725.0
167.00	5242.0
168.00	2705.0
169.00	469.0
172.00	373.0
173.00	607.0
174.00	1029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

175.10	1947.0
176.10	544.0
177.00	920.0
179.00	3586.0
180.10	2706.0
181.00	1174.0
184.10	331.0
185.00	1711.0
186.10	14171.0
187.00	4055.0
188.00	538.0
189.00	852.0
191.00	395.0
192.00	1174.0
193.00	1409.0
194.10	318.0
196.00	2657.0
197.20	710.0
198.00	101448.0
199.00	7050.0
200.00	595.0
201.50	438.0
203.00	730.0
204.10	3526.0
205.10	6507.0
206.10	26568.0
207.10	3747.0
208.00	887.0
209.00	326.0
210.10	376.0
211.10	1027.0
216.00	613.0
217.00	7204.0
218.00	910.0
221.10	4006.0
221.80	896.0
223.00	1489.0
224.10	14596.0
225.10	3736.0
226.10	419.0
227.00	6253.0
228.00	917.0
229.00	1294.0
231.00	504.0
234.00	349.0
235.00	398.0
236.00	313.0
237.00	675.0
242.00	739.0
243.10	801.0
244.10	10751.0
245.10	1396.0
246.00	2293.0
247.00	419.0
249.00	397.0
254.20	610.0
255.10	55232.0
256.10	8495.0
257.10	608.0
258.00	3267.0
259.00	545.0
265.00	1351.0
273.00	1582.0
274.10	4311.0
275.10	24848.0
276.10	3422.0
277.00	2159.0
278.00	367.0
285.00	384.0
293.00	477.0
296.10	6372.0
297.00	980.0
303.00	795.0
315.00	736.0
316.00	419.0
323.10	2082.0
324.00	383.0
327.00	355.0
334.00	1295.0
335.00	312.0
346.00	470.0
352.00	596.0
353.00	408.0
354.10	694.0
365.00	2620.0
366.00	410.0
372.00	1049.0
402.00	402.0
403.00	595.0
421.00	509.0
422.00	457.0
423.10	3403.0
424.00	1020.0
441.10	9920.0
442.10	65048.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

443.1013117.0

444.101258.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.00	419.0
39.10	2594.0
44.00	336.0
47.00	334.0
49.00	1974.0
50.10	9883.0
51.10	39344.0
52.10	2013.0
56.00	1141.0
57.00	2770.0
61.00	485.0
62.00	650.0
63.10	1559.0
65.10	786.0
68.10	794.0
69.00	41640.0
73.00	414.0
74.10	4578.0
75.00	6712.0
76.10	2430.0
77.10	50088.0
78.10	3595.0
79.00	3328.0
80.00	2425.0
81.00	3377.0
82.00	898.0
83.00	895.0
84.00	1530.0
85.00	747.0
86.00	1848.0
87.00	492.0
88.00	305.0
91.00	839.0
92.00	908.0
93.00	5722.0
94.00	359.0
98.00	4719.0
99.00	3525.0
100.00	344.0
101.00	1980.0
103.00	717.0
104.00	1127.0
105.00	1216.0
106.10	422.0
107.00	16848.0
108.00	2481.0
109.00	470.0
110.00	29520.0
111.00	4312.0
112.00	556.0
116.00	892.0
117.00	13797.0
118.00	1014.0
122.00	1057.0
123.00	1669.0
124.00	772.0
125.00	728.0
126.20	404.0
127.10	54592.0
128.10	4249.0
129.00	20968.0
130.00	1932.0
131.00	342.0
134.00	665.0
135.00	1813.0
136.00	668.0
137.00	929.0
141.00	2953.0
142.00	924.0
143.00	591.0
146.00	531.0
147.00	1549.0
148.00	3527.0
149.00	721.0
151.10	438.0
153.00	1016.0
154.00	704.0
155.00	1868.0
156.10	2431.0
157.10	515.0
158.00	489.0
159.00	380.0
160.00	932.0
161.00	1304.0
162.00	389.0
165.00	1146.0
166.00	923.0
167.00	6343.0
168.00	3390.0
169.10	587.0
171.90	524.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

173.00	671.0
174.00	1420.0
175.10	2581.0
176.00	653.0
177.00	1158.0
178.00	409.0
179.00	4619.0
180.00	3299.0
181.00	1383.0
184.00	361.0
185.10	2457.0
186.10	18096.0
187.10	5077.0
188.00	544.0
189.00	1158.0
191.00	554.0
192.00	1558.0
193.10	1730.0
194.00	359.0
196.10	3377.0
197.10	989.0
198.00	127632.0
199.00	8581.0
200.00	726.0
201.60	531.0
203.00	932.0
204.10	4975.0
205.10	8001.0
206.10	34160.0
207.10	4686.0
208.00	1157.0
209.00	387.0
210.10	484.0
211.00	1270.0
215.00	390.0
216.00	706.0
217.00	8852.0
218.00	1261.0
221.10	4774.0
221.90	1113.0
223.00	2088.0
224.10	18704.0
225.10	5011.0
226.10	515.0
227.10	7957.0
228.00	1073.0
229.00	1580.0
231.00	680.0
234.00	468.0
235.00	573.0
236.00	399.0
237.10	605.0
239.00	302.0
241.00	447.0
242.00	950.0
243.10	1044.0
244.10	14804.0
245.10	1847.0
246.00	2994.0
247.00	590.0
249.00	509.0
253.00	361.0
254.20	748.0
255.10	75072.0
256.10	10580.0
257.00	925.0
258.00	4270.0
259.10	657.0
265.00	1686.0
273.00	2137.0
274.10	5897.0
275.10	32728.0
276.10	4369.0
277.00	2956.0
278.00	569.0
283.00	348.0
285.10	525.0
293.00	678.0
296.10	9230.0
297.00	1238.0
303.00	1116.0
314.10	457.0
315.00	1120.0
316.10	607.0
321.00	333.0
323.10	2972.0
324.00	562.0
326.90	552.0
334.10	1936.0
335.00	476.0
341.00	321.0
346.00	691.0
352.10	843.0
353.00	692.0
354.10	1002.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

365.00	4035.0
366.00	594.0
372.10	1404.0
373.10	420.0
383.00	408.0
402.00	659.0
403.00	845.0
404.00	350.0
421.10	734.0
422.00	779.0
423.10	5572.0
424.10	1393.0
441.10	15921.0
442.10	103408.0
443.10	20496.0
444.10	1951.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.00	319.0
39.10	2000.0
44.00	420.0
46.90	406.0
49.00	2212.0
50.10	7343.0
51.10	29976.0
52.00	1412.0
56.00	885.0
57.00	2082.0
61.00	342.0
62.00	421.0
63.00	1147.0
65.00	647.0
68.00	515.0
69.00	29792.0
73.10	326.0
74.00	3172.0
75.00	4965.0
76.10	1791.0
77.10	36880.0
78.10	2547.0
79.00	2255.0
80.00	1635.0
81.00	2507.0
82.00	672.0
83.00	619.0
84.00	1668.0
85.00	575.0
86.00	1808.0
87.00	402.0
91.00	554.0
92.00	732.0
93.00	4178.0
94.00	311.0
98.00	3409.0
99.00	2683.0
101.00	1587.0
103.00	503.0
104.00	965.0
105.00	888.0
107.00	12040.0
108.00	1880.0
109.10	351.0
110.00	22032.0
111.00	3360.0
112.00	330.0
116.00	663.0
117.00	10030.0
118.00	776.0
122.00	788.0
123.00	1223.0
124.00	555.0
125.00	508.0
127.00	41912.0
128.00	3049.0
129.00	15742.0
130.00	1214.0
131.00	348.0
134.00	466.0
135.00	1384.0
136.00	506.0
137.00	678.0
141.00	2211.0
142.00	631.0
143.00	487.0
146.00	380.0
147.00	1110.0
148.00	2698.0
149.00	505.0
153.00	707.0
154.00	506.0
155.10	1241.0
156.10	1989.0
157.10	372.0
157.90	398.0
160.00	691.0
161.00	1017.0
162.00	334.0
165.00	834.0
166.00	734.0
167.00	5097.0
168.00	2387.0
169.00	372.0
172.00	452.0
173.00	577.0
174.00	980.0
175.10	2055.0
176.00	499.0
177.00	846.0
179.00	3431.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

180.00	2437.0
181.00	1168.0
185.10	1653.0
186.10	14153.0
187.10	3905.0
188.00	431.0
189.00	865.0
190.90	364.0
192.00	1118.0
193.00	1372.0
196.10	2820.0
197.10	677.0
198.00	101880.0
199.00	6692.0
200.00	522.0
201.50	445.0
203.00	697.0
204.10	3922.0
205.10	6423.0
206.10	26904.0
207.10	3684.0
208.00	937.0
209.00	317.0
210.20	378.0
211.10	1021.0
214.90	342.0
216.00	607.0
217.00	6882.0
218.00	975.0
221.10	4335.0
221.80	962.0
223.10	1544.0
224.10	15397.0
225.10	3782.0
226.00	445.0
227.10	6428.0
228.00	786.0
229.00	1347.0
231.00	606.0
234.00	346.0
235.00	475.0
237.00	565.0
241.00	323.0
242.00	726.0
243.10	935.0
244.10	12006.0
245.10	1522.0
246.00	2335.0
247.00	498.0
249.00	435.0
253.10	303.0
254.20	595.0
255.10	61520.0
256.10	8655.0
257.10	663.0
258.10	3496.0
259.00	584.0
265.00	1504.0
273.00	1896.0
274.00	4973.0
275.10	27488.0
276.10	3632.0
277.00	2495.0
278.00	468.0
285.00	421.0
293.00	576.0
296.00	7914.0
297.00	1166.0
303.00	897.0
314.00	392.0
315.00	949.0
316.00	509.0
323.10	2548.0
324.10	534.0
327.00	528.0
334.00	1582.0
335.00	462.0
346.00	571.0
352.00	852.0
353.00	501.0
354.10	862.0
365.00	3775.0
366.00	553.0
372.10	1439.0
373.10	339.0
383.00	351.0
402.00	609.0
403.10	817.0
421.00	779.0
422.00	694.0
423.10	5280.0
424.10	1272.0
441.10	15824.0
442.10	100744.0
443.10	18920.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

444.10

1722.0


Instrument :
BNA_M
ClientSampleId :
DFTPP64

Data Path : Z:\HPCHEM1\BNA_M\Data\BM050516\
Data File : BM005230.D
Acq On : 05 May 2016 10:23
Operator : UM/SJ
Sample : DFTPP64
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP64

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Title : SVOA CALIBRATION
Last Update : Sat May 07 07:05:19 2016

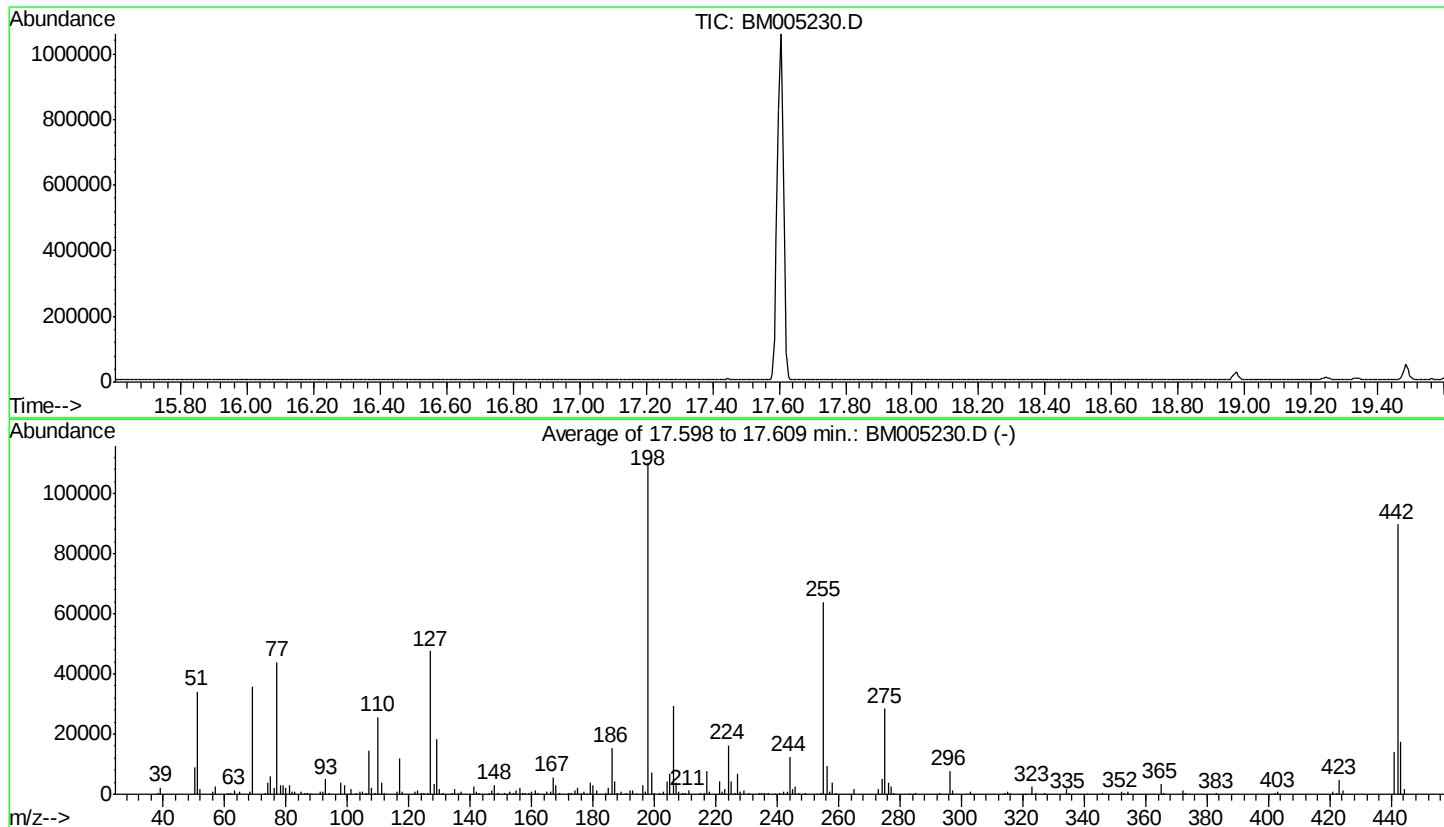

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	34217	PASS
68	69	0.00	2	1.8	659	PASS
69	198	0.00	100	32.4	35757	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	47546	PASS
197	198	0.00	2	0.7	792	PASS
198	198	100	100	100.0	110320	PASS
199	198	5	9	6.7	7441	PASS
275	198	10	60	25.7	28354	PASS
365	198	1	100	3.2	3476	PASS
441	443	0.01	100	79.3	13888	PASS
442	198	50	100	81.3	89733	PASS
443	442	15	24	19.5	17511	PASS