
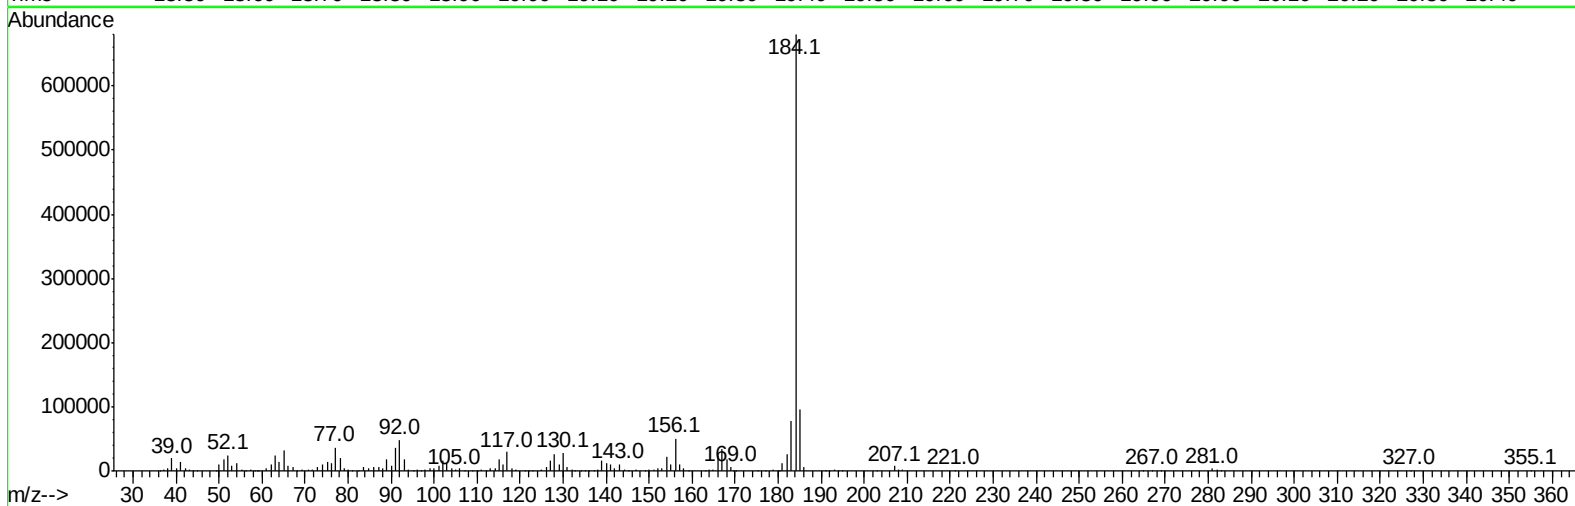


Data Path : Z:\HPCHEM1\BNA M\DATA\BM050517\
Data File : BM009903.D
Acq On : 05 May 2017 15:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:11:39 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:52:12 2017
Response via : Initial Calibration

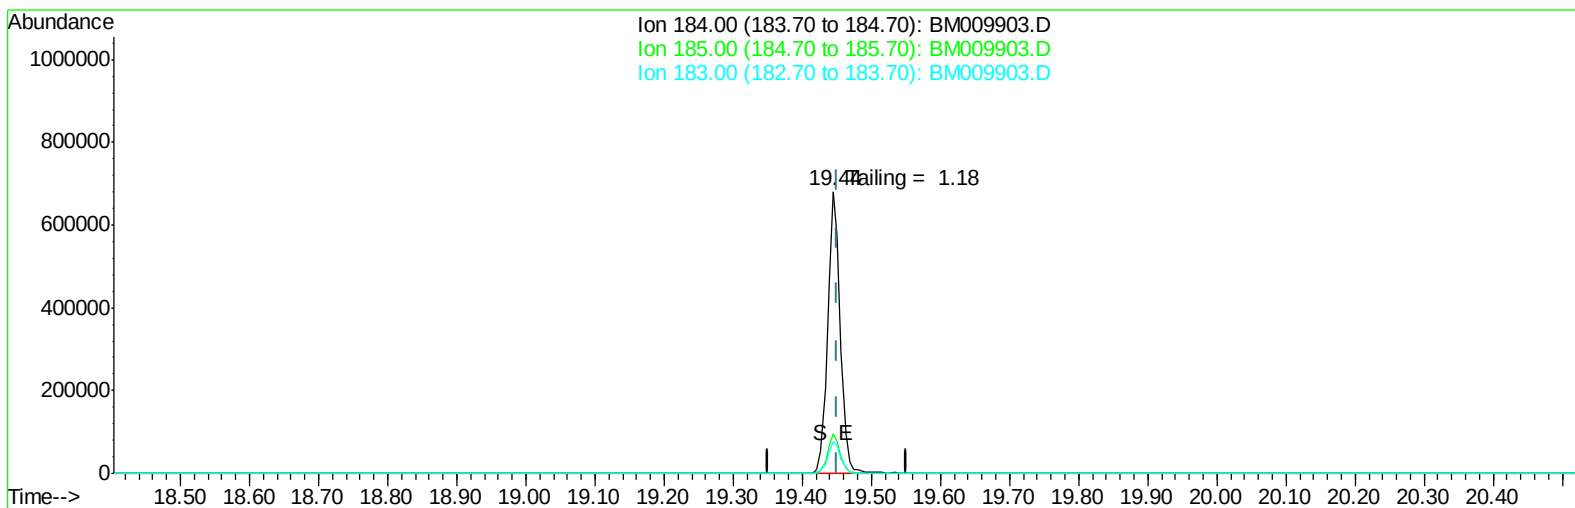

TIC: BM009903.D

(76) Benzidine



19.445min (-0.006) 7027.29ng

response 864068

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.16
183.00	11.10	11.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050517\
Data File : BM009903.D
Acq On : 05 May 2017 15:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:11:39 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:52:12 2017
Response via : Initial Calibration

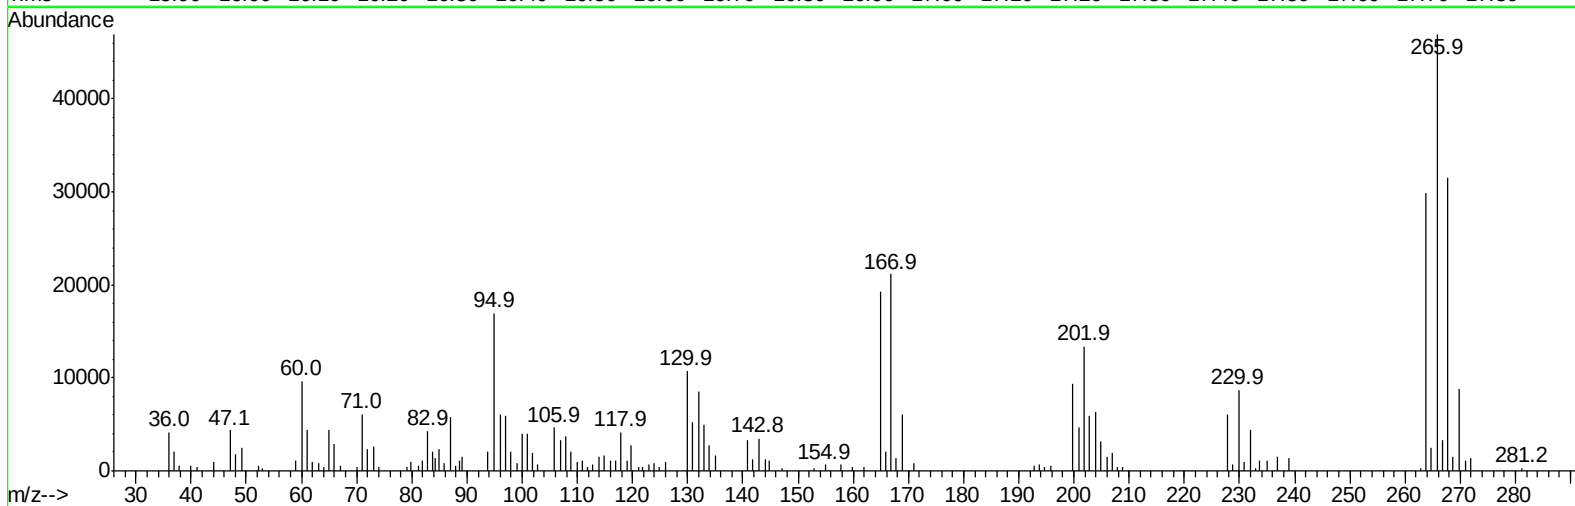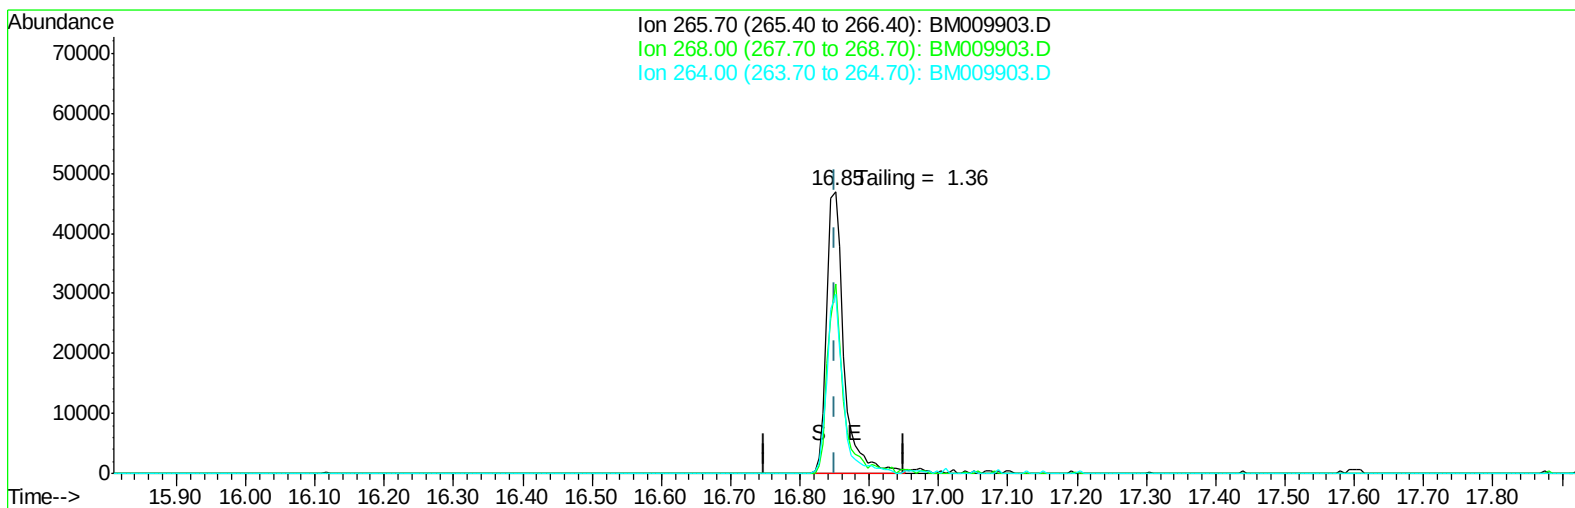

TIC: BM009903.D

(69) Pentachlorophenol (C)

16.851min (+0.001) 113458.55ng

response 79920

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	70.63
264.00	61.20	63.67
0.00	0.00	0.00