
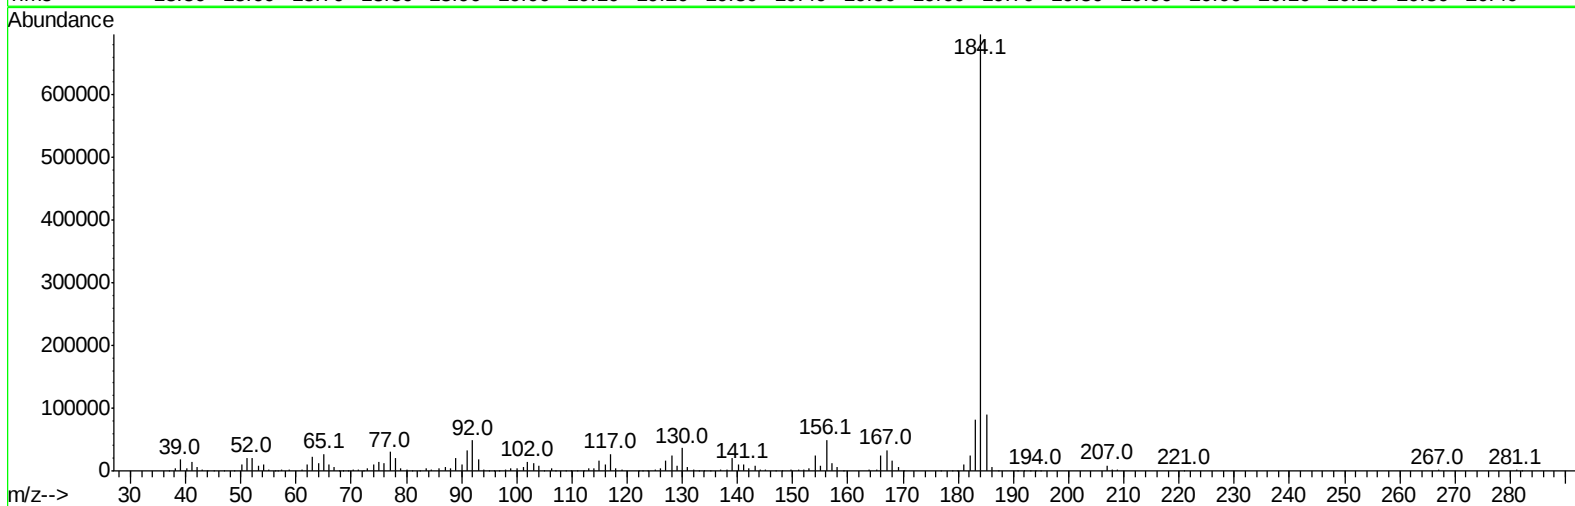


Data Path : Z:\HPCHEM1\BNA M\DATA\BM050517\  
Data File : BM009921.D  
Acq On : 06 May 2017 02:29  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:14:03 2017  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 05 14:52:12 2017  
Response via : Initial Calibration

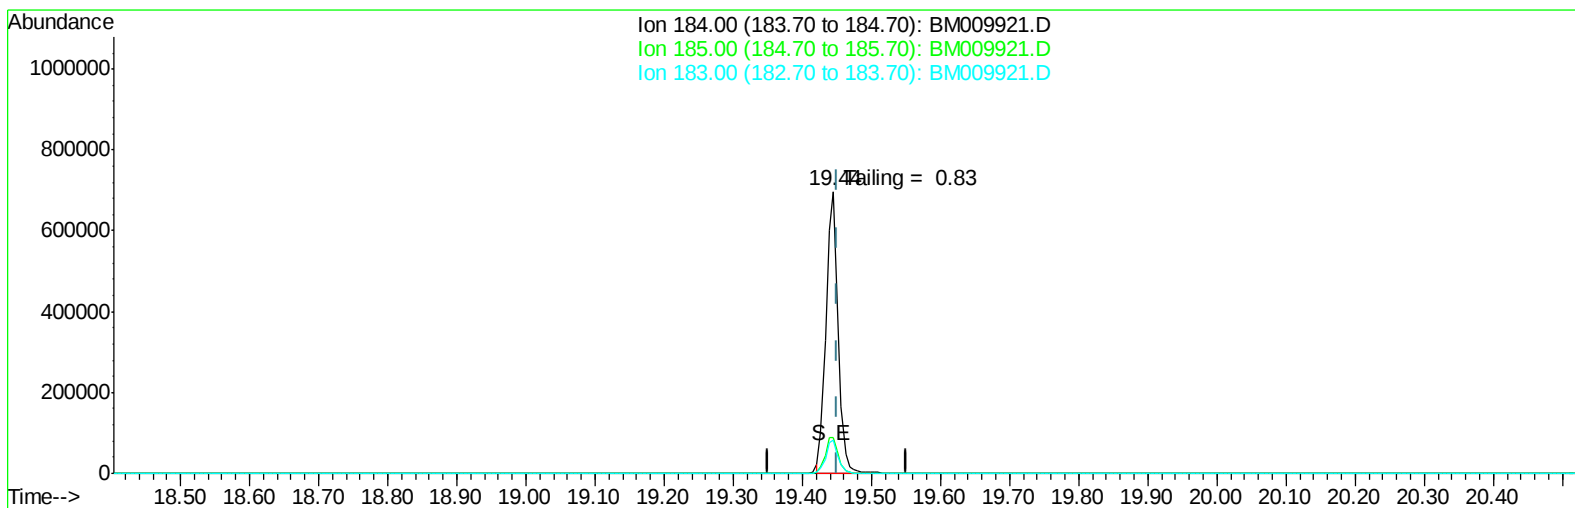

TIC: BM009921.D

(76) Benzidine



19.445min (-0.006) 5716.03ng

response 861820

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 12.93 |
| 183.00 | 11.10 | 11.64 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050517\  
Data File : BM009921.D  
Acq On : 06 May 2017 02:29  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:14:03 2017  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 05 14:52:12 2017  
Response via : Initial Calibration

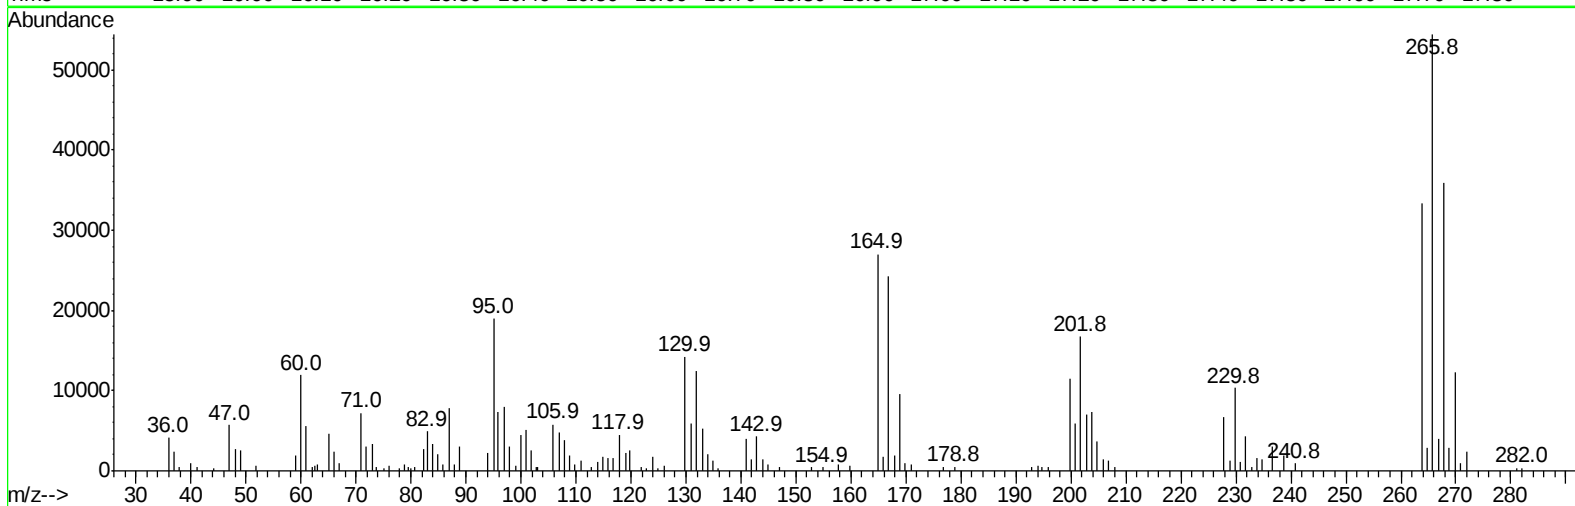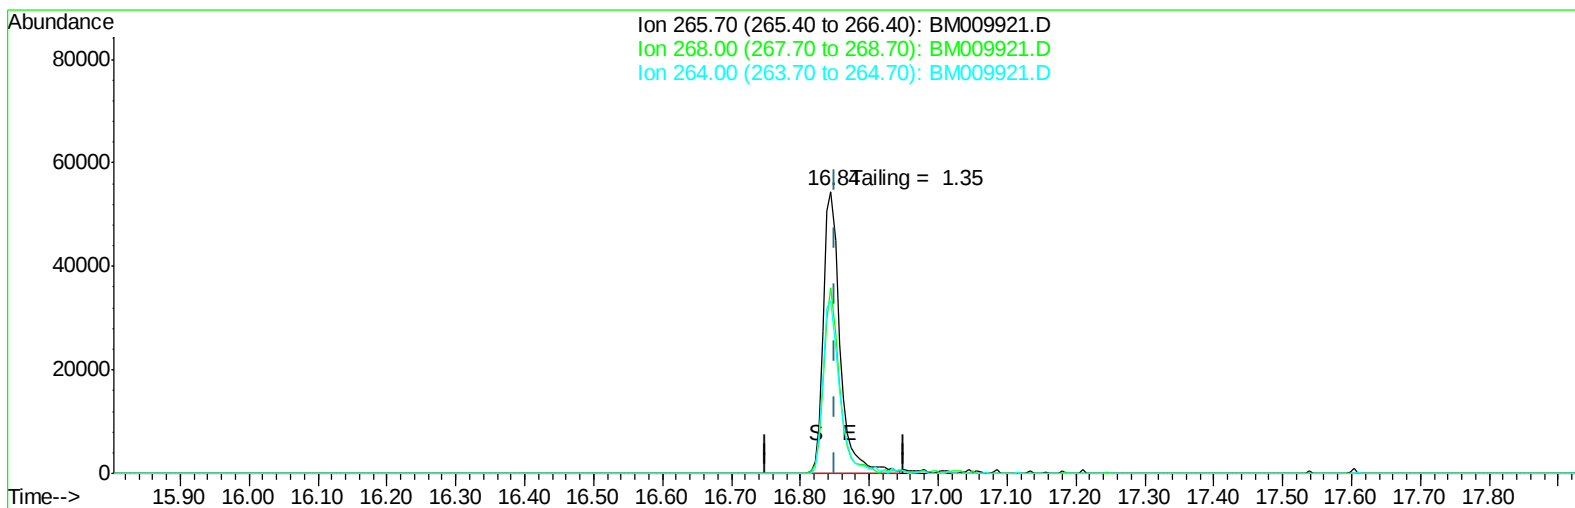

TIC: BM009921.D

(69) Pentachlorophenol (C)

16.845min (-0.005) 0.00ng

response 90946

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 66.10 |
| 264.00 | 61.20 | 61.31 |
| 0.00   | 0.00  | 0.00  |