


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050517\
 Data File : BM009894.D
 Acq On : 05 May 2017 09:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 05 14:52:12 2017

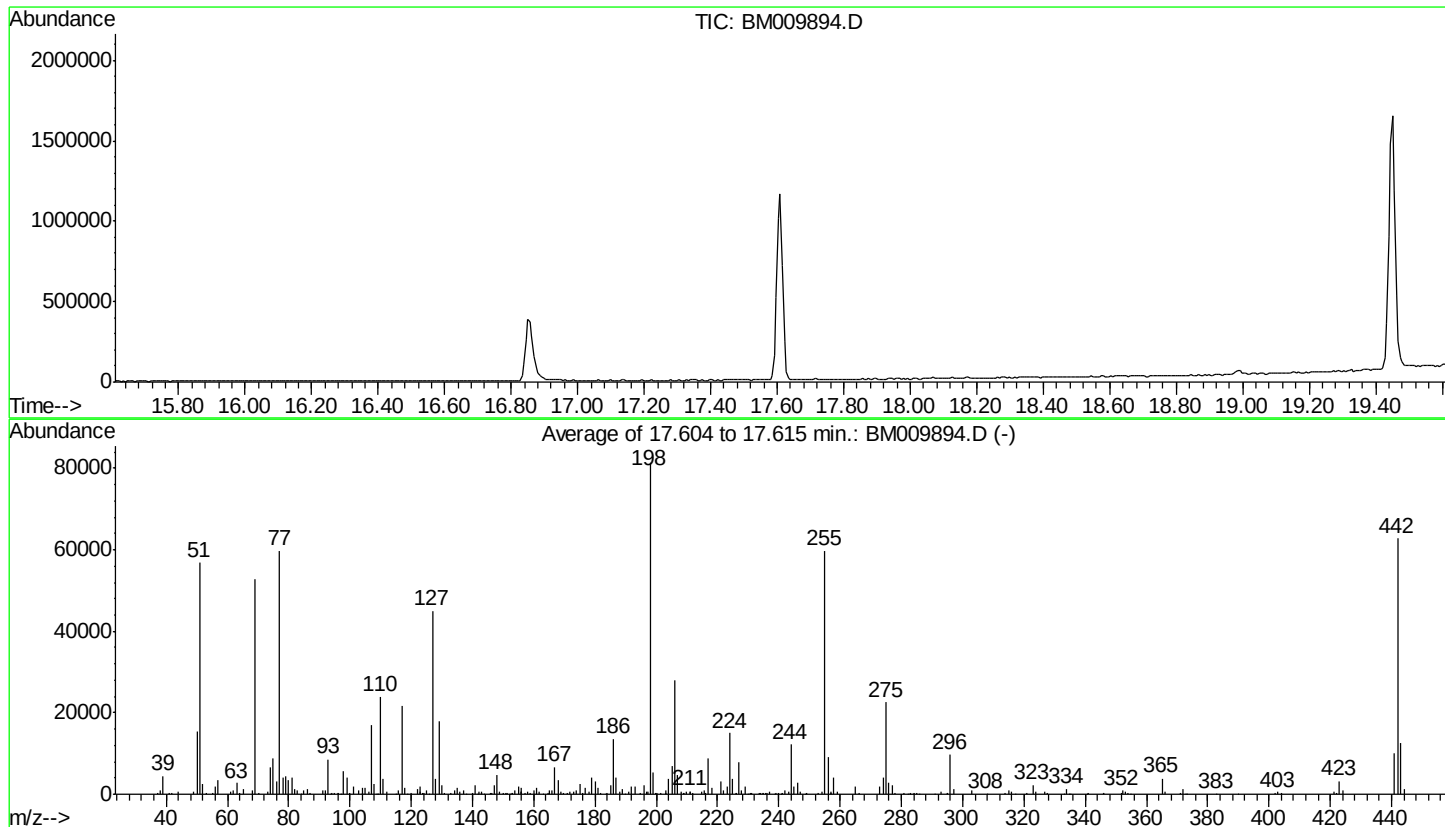

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.7	56757	PASS
68	69	0.00	2	1.9	1014	PASS
69	198	0.00	100	64.9	52790	PASS
70	69	0.00	2	0.7	351	PASS
127	198	10	80	55.3	44984	PASS
197	198	0.00	2	0.7	540	PASS
198	198	100	100	100.0	81386	PASS
199	198	5	9	6.6	5346	PASS
275	198	10	60	27.7	22509	PASS
365	198	1	100	4.7	3864	PASS
441	442	0.01	24	15.8	9918	PASS
442	198	50	100	77.2	62800	PASS
443	442	15	24	19.9	12475	PASS