


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050517\
 Data File : BM009903.D
 Acq On : 05 May 2017 15:20
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
 Title : SVOA CALIBRATION
 Last Update : Wed Nov 30 00:32:18 2016

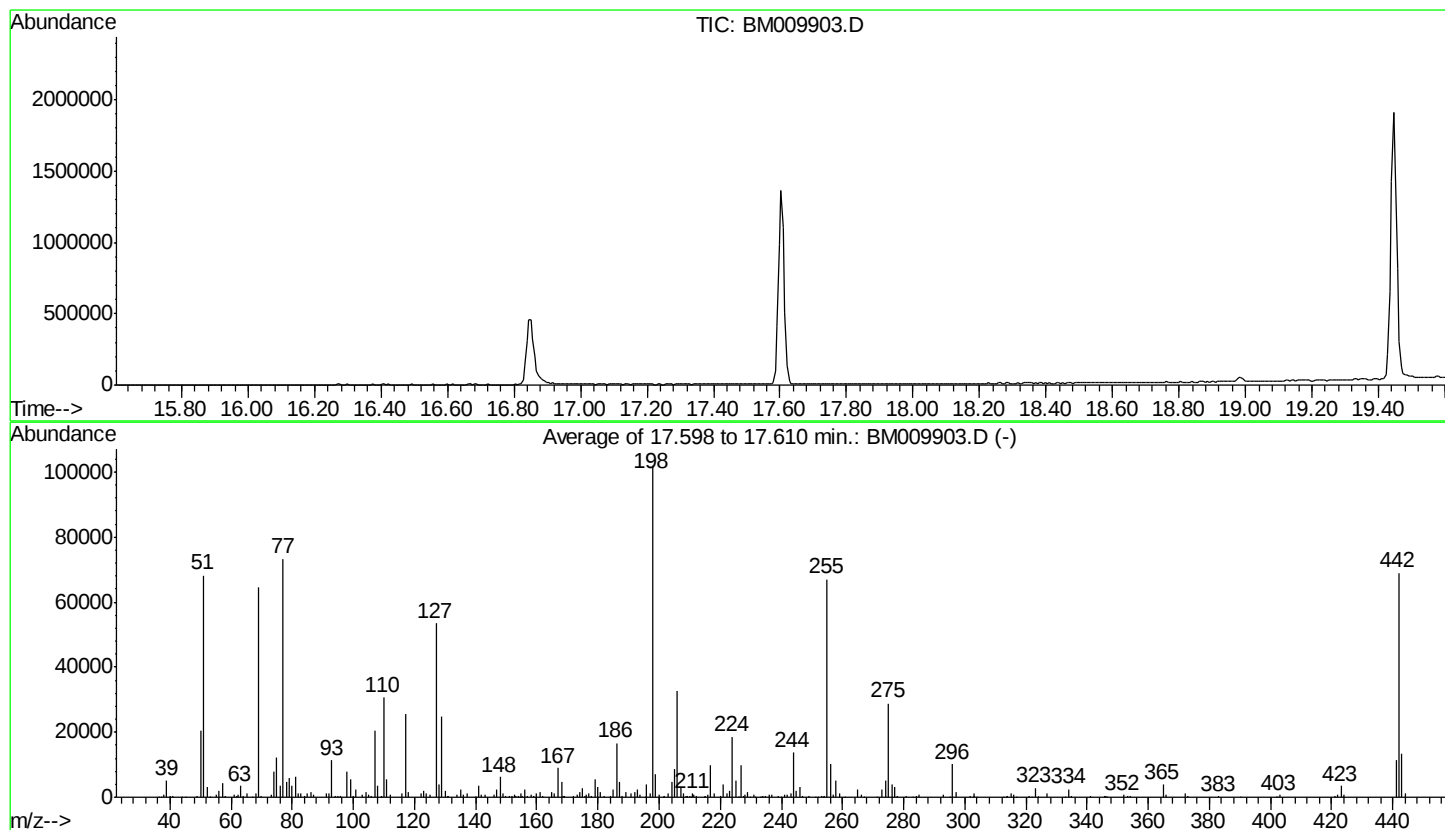

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.8	68129	PASS
68	69	0.00	2	1.8	1143	PASS
69	198	0.00	100	63.5	64709	PASS
70	69	0.00	2	0.7	447	PASS
127	198	10	80	52.4	53472	PASS
197	198	0.00	2	1.0	1057	PASS
198	198	100	100	100.0	101965	PASS
199	198	5	9	7.0	7115	PASS
275	198	10	60	28.3	28818	PASS
365	198	1	100	3.8	3867	PASS
441	443	0.01	100	86.5	11602	PASS
442	198	50	100	67.7	69005	PASS
443	442	15	24	19.4	13406	PASS