


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050517\
Data File : BM009921.D
Acq On : 06 May 2017 02:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

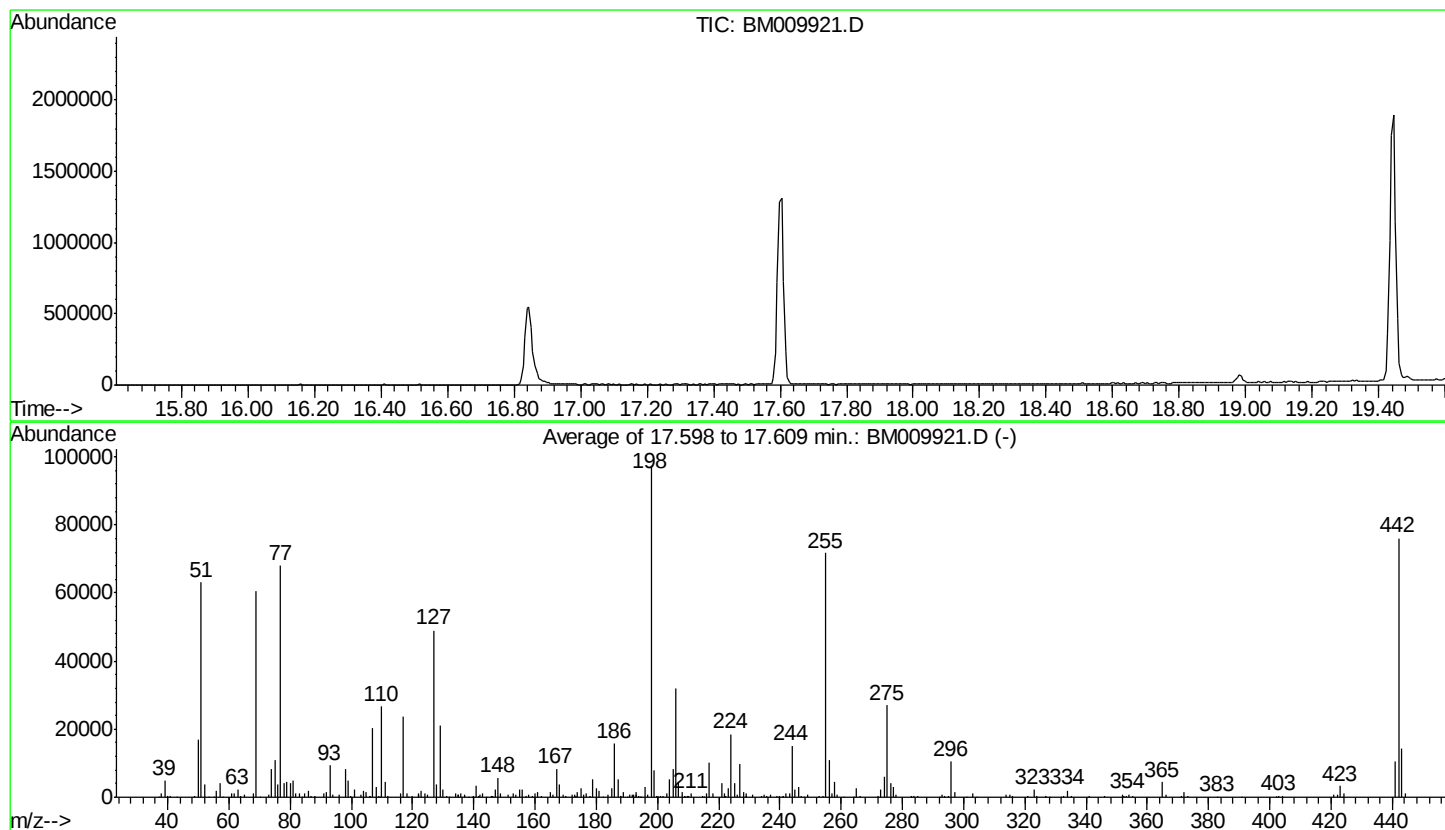

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.7	63034	PASS
68	69	0.00	2	2.0	1236	PASS
69	198	0.00	100	62.0	60384	PASS
70	69	0.00	2	0.2	104	PASS
127	198	10	80	50.3	48978	PASS
197	198	0.00	2	0.8	803	PASS
198	198	100	100	100.0	97386	PASS
199	198	5	9	8.1	7880	PASS
275	198	10	60	27.7	26968	PASS
365	198	1	100	4.5	4365	PASS
441	443	0.01	100	73.5	10387	PASS
442	198	50	100	78.1	76064	PASS
443	442	15	24	18.6	14127	PASS