

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050523\
 Data File : BM039845.D
 Acq On : 05 May 2023 15:04
 Operator : CG/JU
 Sample : PB152529BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK529

Quant Time: May 06 02:47:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 06 02:22:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	1654	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.584	136	6736	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.437	164	3918	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.191	188	9083	0.400	ng/ul	-0.02
17) Chrysene-d12	21.413	240	7488	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	9949	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.172	96	11983	4.916	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	2743	0.317	ng/ul	0.01
18) Fluoranthene-d10	19.234	212	6836	0.339	ng/ul	0.00
Target Compounds				Qvalue		
12) Fluorene	15.431	166	1015	0.077	ng/ul#	19
20) Pyrene	19.592	202	1162	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.581	252	2411	0.077	ng/ul#	44

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050523\
Data File : BM039845.D
Acq On : 05 May 2023 15:04
Operator : CG/JU
Sample : PB152529BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK529

Quant Time: May 06 02:47:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 06 02:22:07 2023
Response via : Initial Calibration

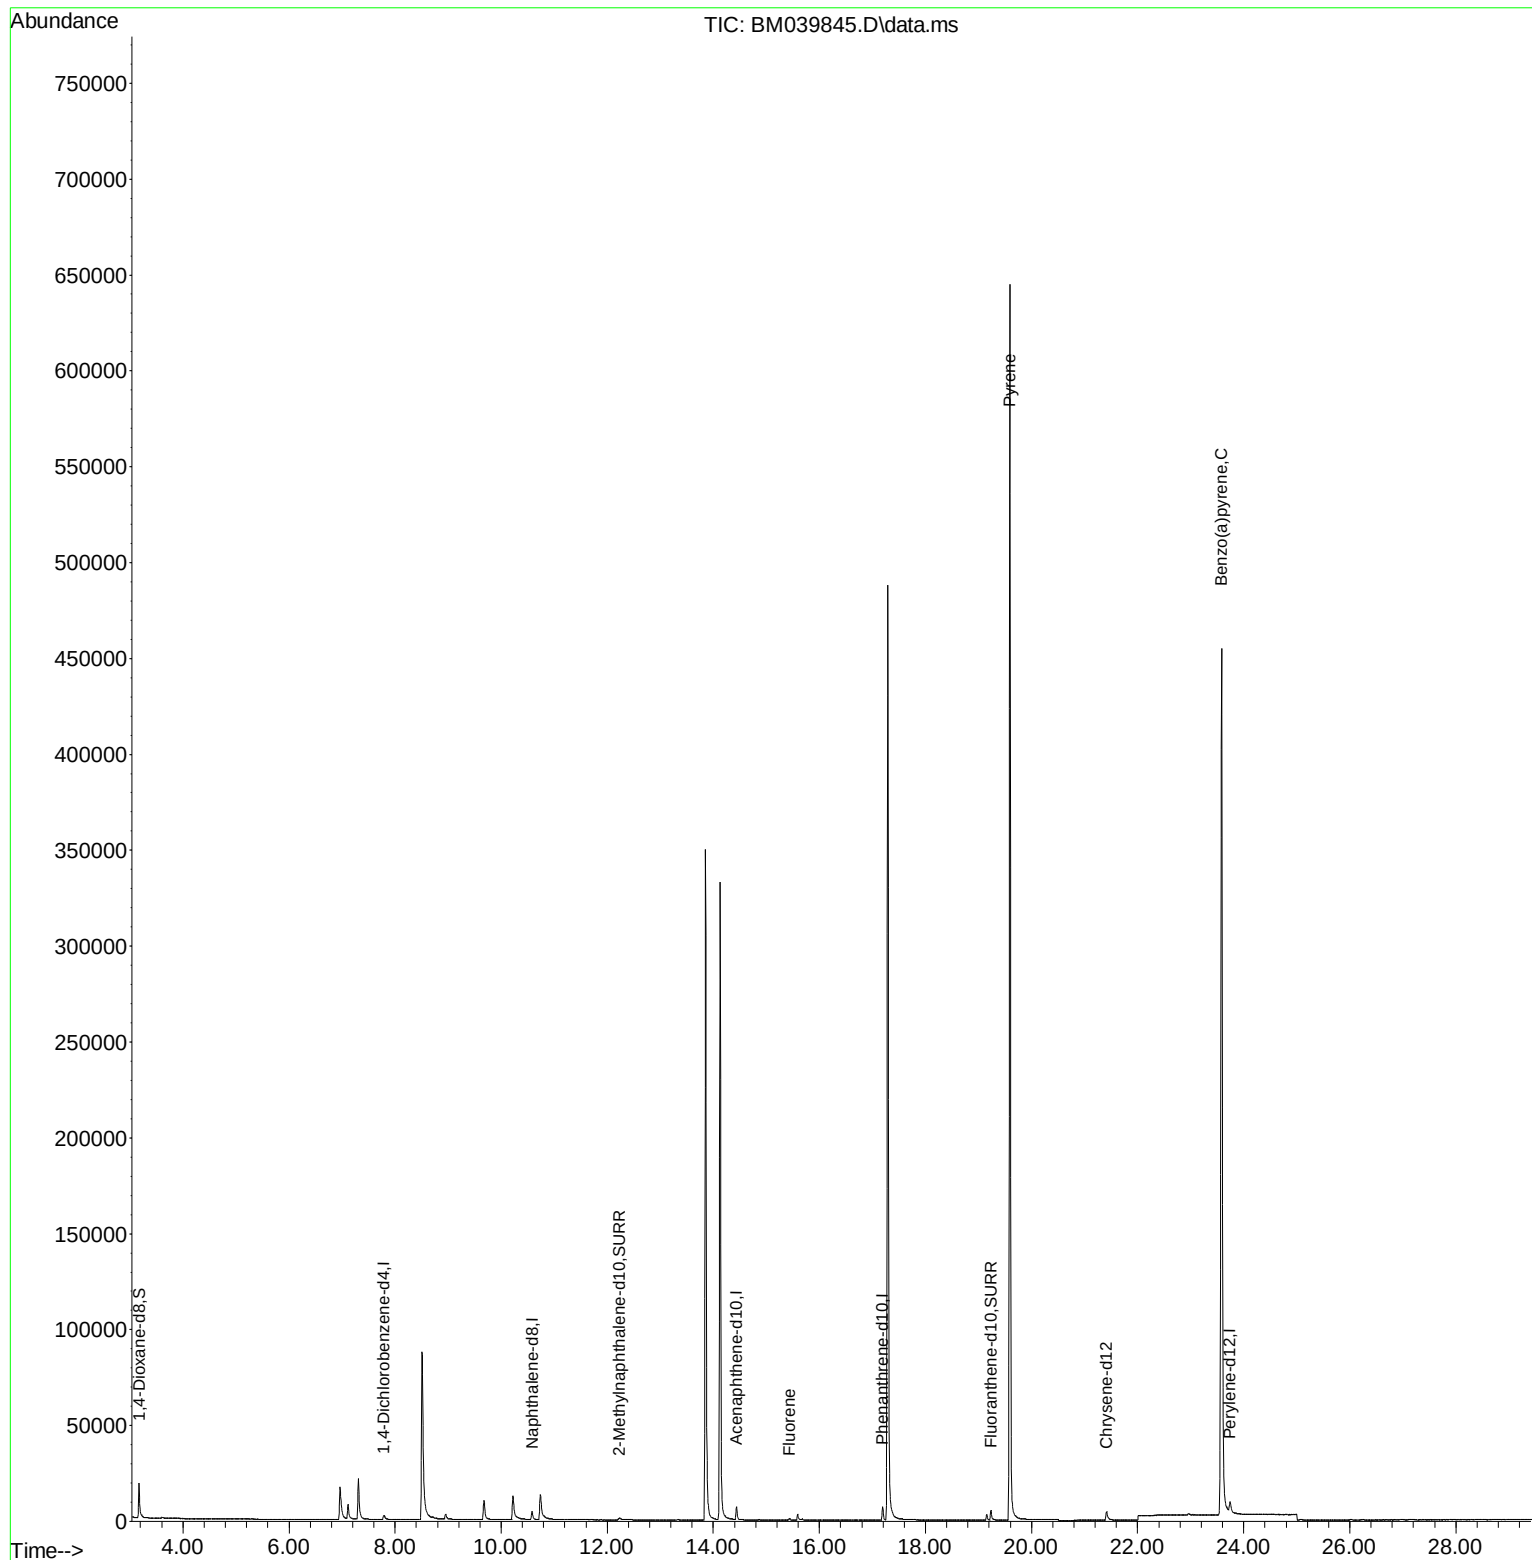



Abundance Scan 2732 (15.524 min): BM039835.D\data.ms (-2710) (-)

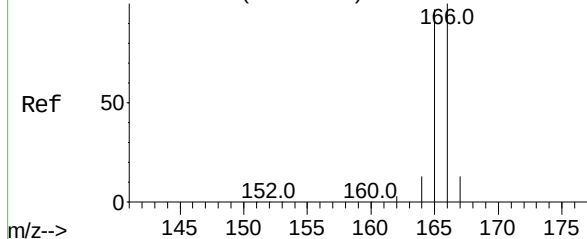


Fluorene
Concen: 0.077 ng/ul
RT: 15.431 min Scan# 2712
Delta R.T. -0.083 min
Lab File: BM039845.D
Acq: 05 May 2023 15:04

Instrument :
BNA_M
ClientSampleId :
SBLK529


Tgt Ion:	166	Resp:	1015
Ion	Ratio	Lower	Upper
166	100		
165	13.3	79.0	118.6#
167	35.1	11.8	17.6#

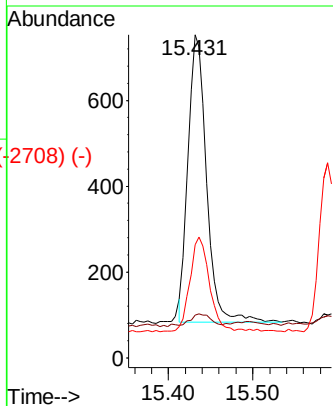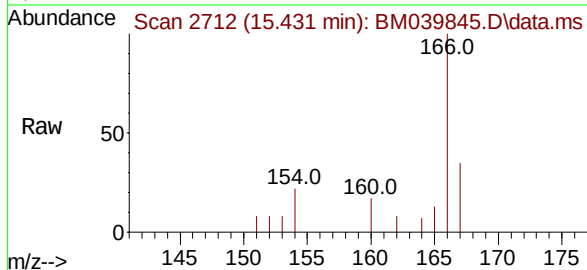

Abundance Scan 2712 (15.431 min): BM039845.D\data.ms (-2708) (-)


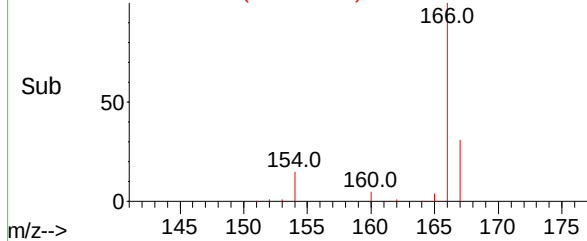


Abundance Scan 3672 (19.638 min): BM039835.D\data.ms (-3669) (-)

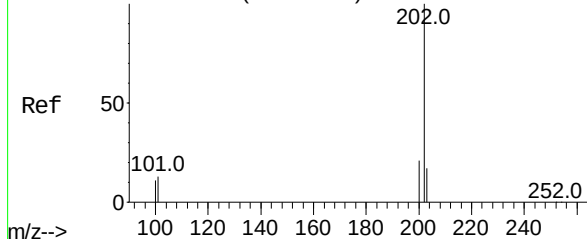


Pyrene
Concen: 0.040 ng/ul
RT: 19.592 min Scan# 3662
Delta R.T. -0.042 min
Lab File: BM039845.D
Acq: 05 May 2023 15:04


Tgt Ion:	202	Resp:	1162
Ion	Ratio	Lower	Upper
202	100		
101	161.8	10.9	16.3#
100	1167.6	8.9	13.3#

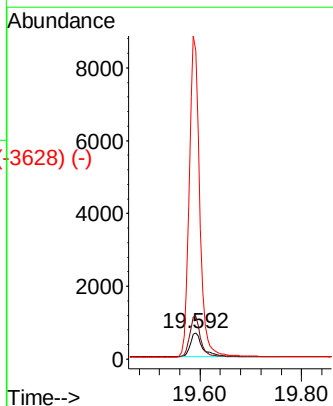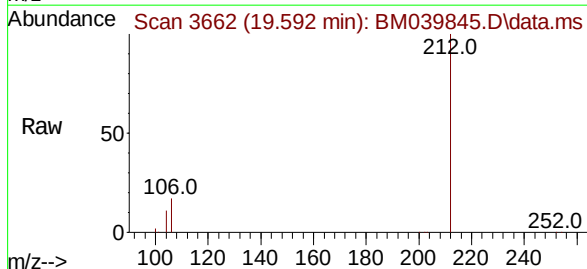

Abundance Scan 3662 (19.592 min): BM039845.D\data.ms (-3628) (-)

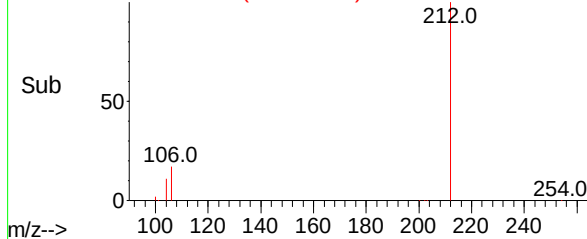

Abundance Scan 4937 (23.657 min): BM039835.D\data.ms (-4920) (-)

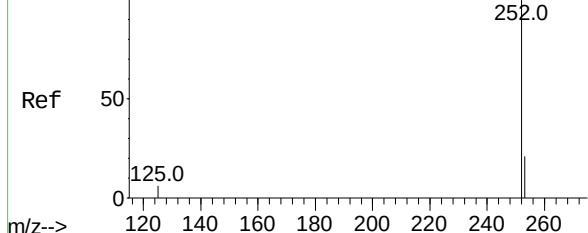

Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.581 min Scan# 4911
Delta R.T. -0.069 min
Lab File: BM039845.D
Acq: 05 May 2023 15:04

Instrument :
BNA_M
ClientSampleId :
SBLK529

Tgt Ion:	252	Resp:	2411
Ion	Ratio	Lower	Upper
252	100		
253	54.4	24.7	37.1#
125	56.1	16.5	24.7#

