


Data Path : Z:\HPCHEM1\BNA M\Data\BM050615\
 Data File : BM001224.D
 Acq On : 06 May 2015 19:29
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-ACID-BM050615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 07 07:00:24 2015

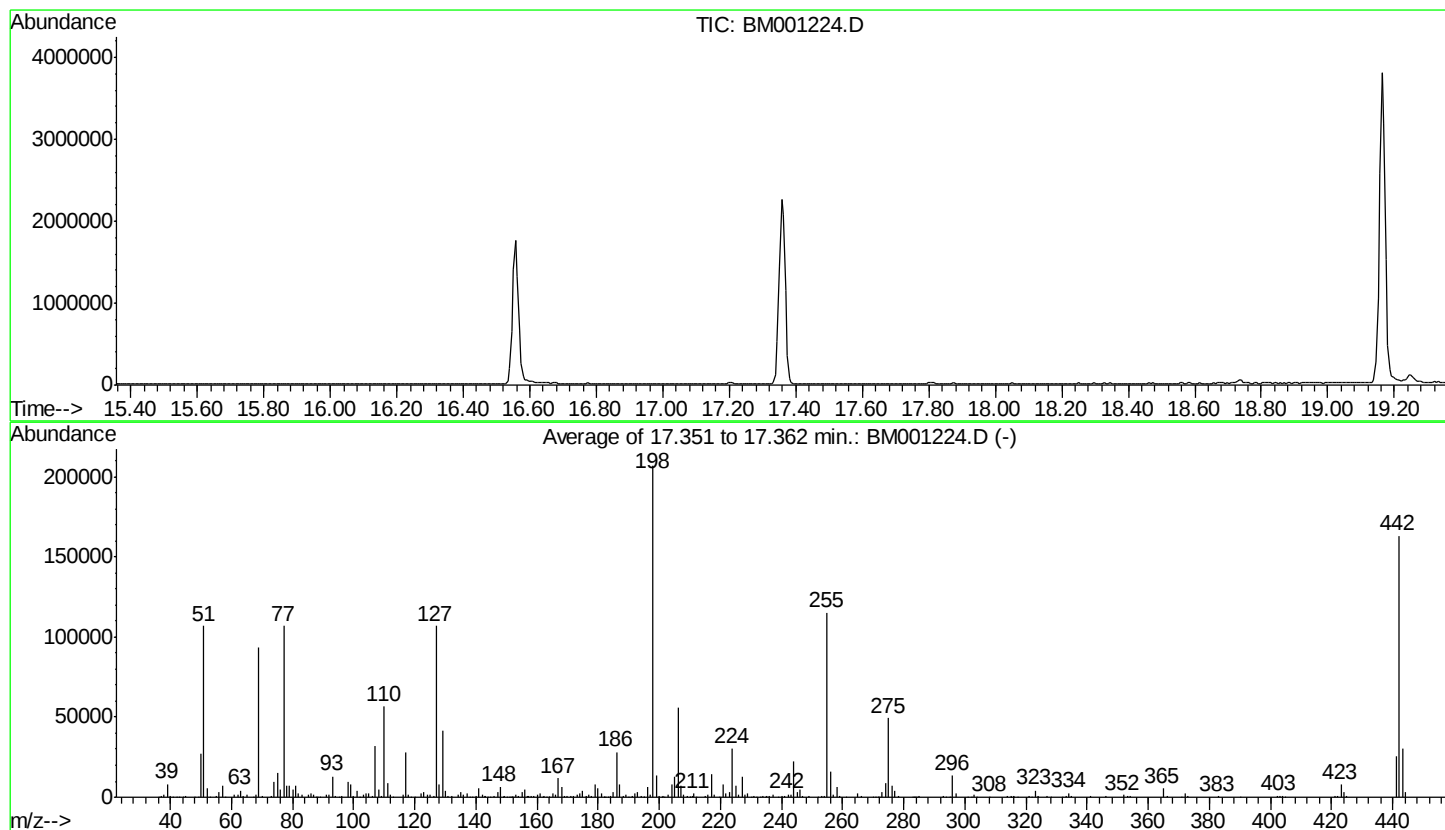

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	107009	PASS
68	69	0.00	2	1.7	1544	PASS
69	198	0.00	100	45.2	93546	PASS
70	69	0.00	2	0.6	532	PASS
127	198	10	80	51.7	107048	PASS
197	198	0.00	2	0.6	1305	PASS
198	198	100	100	100.0	206976	PASS
199	198	5	9	6.7	13853	PASS
275	198	10	60	23.8	49290	PASS
365	198	1	100	2.6	5405	PASS
441	442	0.01	24	15.6	25562	PASS
442	198	50	100	78.9	163394	PASS
443	442	15	24	18.8	30690	PASS