

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005288.D
 Acq On : 07 May 2016 02:10
 Operator : UM/SJ
 Sample : H2820-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A3

Quant Time: May 07 06:54:43 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 07 00:48:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	104140	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	500506	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	326916	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	774175	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	900238	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	842421	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	4669	2.11	ng/uL	0.00
5) Phenol-d5	6.95	99	106334	11.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	65213	12.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	83518	11.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	85479	10.95	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	42492	11.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	48850	12.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	88925	11.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	113444	12.53	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	334480	12.76	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	398236	12.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	37414	7.82	ng/ul	0.00
57) Fluorene-d10	15.40	176	301248	13.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	40070	9.20	ng/ul	0.00
70) Anthracene-d10	17.26	188	469972	13.73	ng/ul	0.00
76) Pyrene-d10	19.56	212	551196	13.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	493253	13.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.87	163	88213	3.37	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005288.D
Acq On : 07 May 2016 02:10
Operator : UM/SJ
Sample : H2820-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A3

Quant Time: May 07 06:54:43 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 07 00:48:43 2016
Response via : Initial Calibration

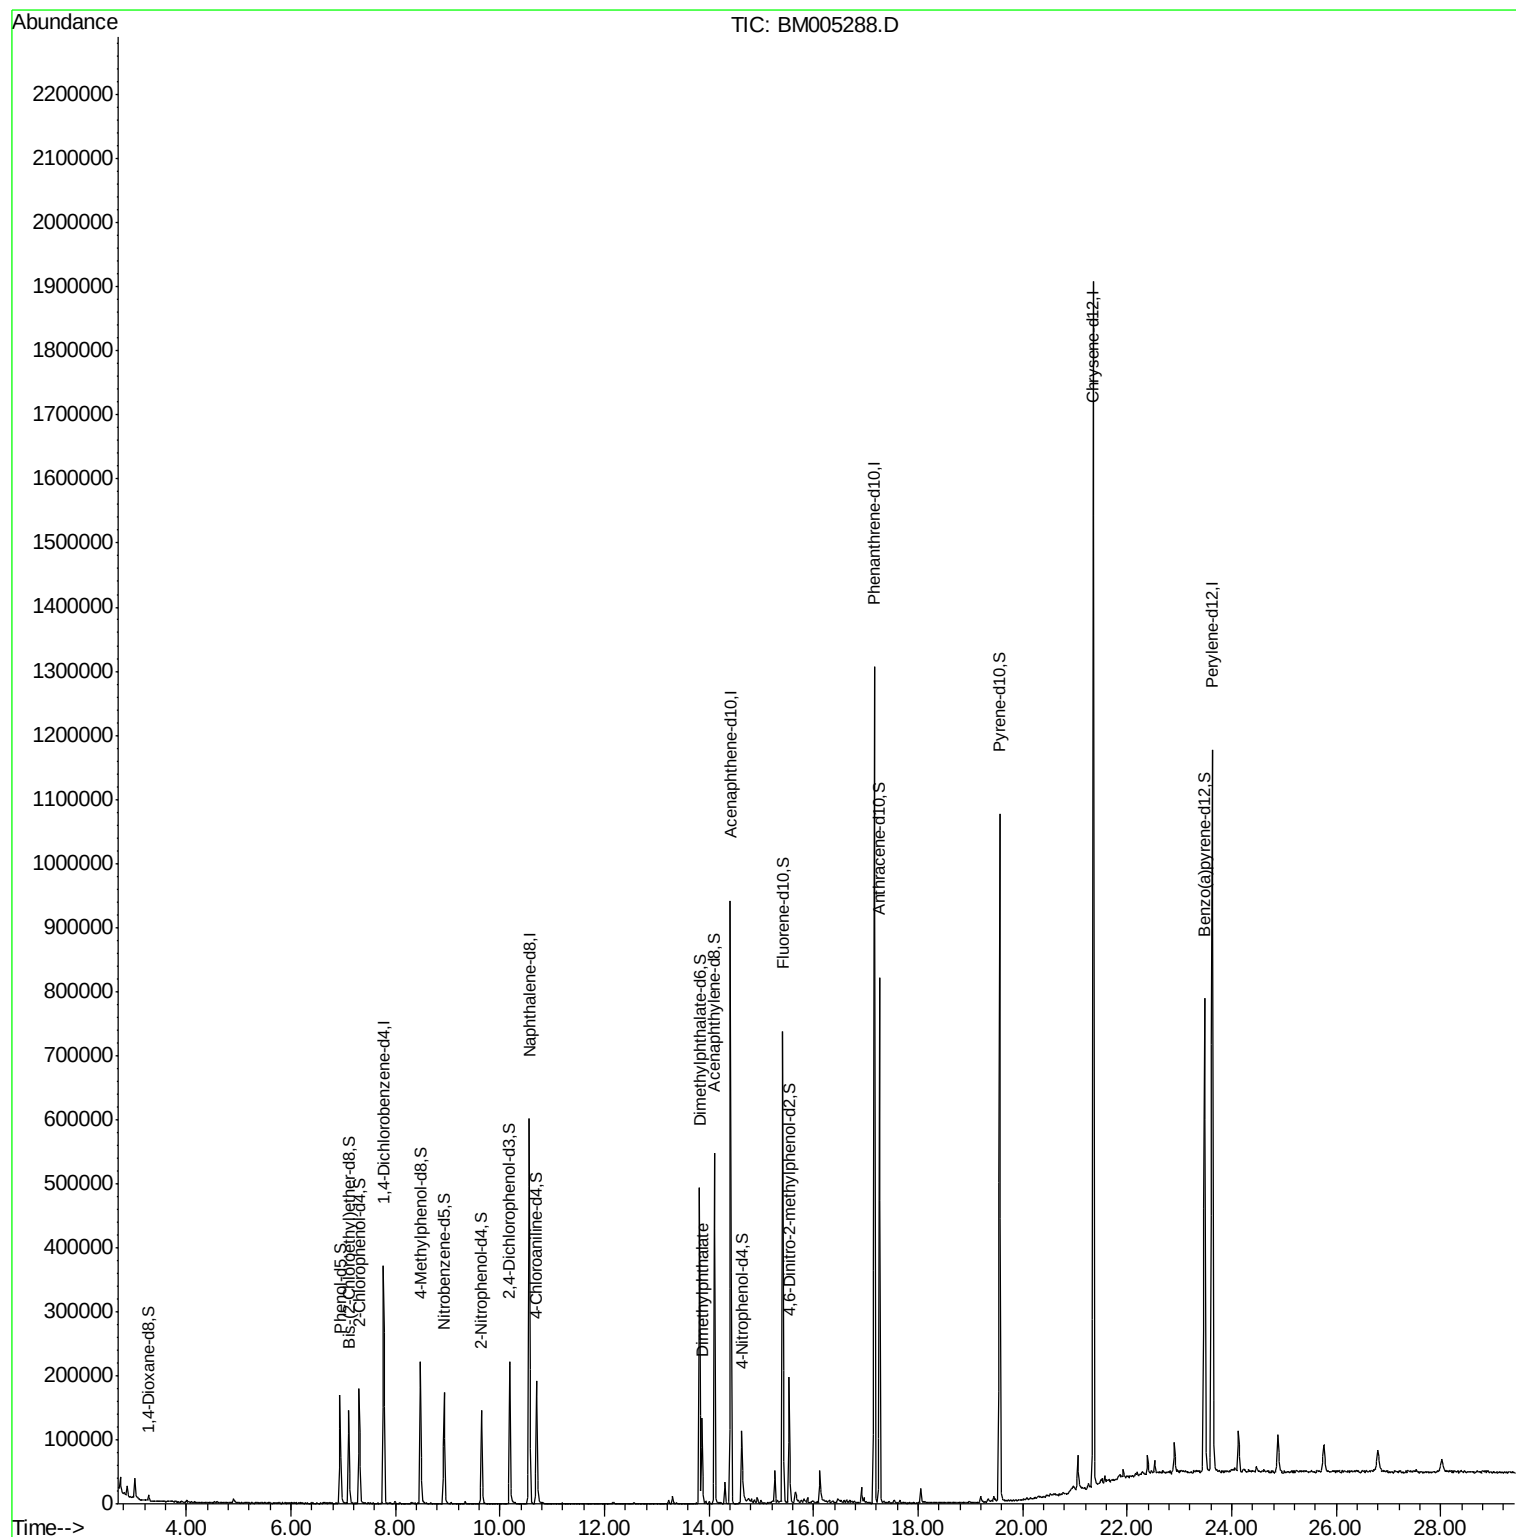

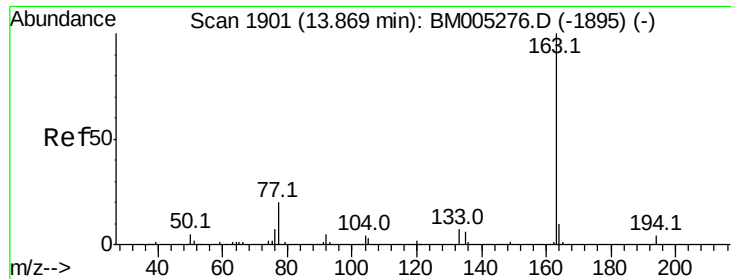

#44

Dimethylphthalate

Concen: 3.37 ng/ul

RT: 13.87 min Scan# 1901

Delta R.T. 0.00 min

Lab File: BM005288.D

Acq: 07 May 2016 02:10

Instrument :

BNA_M

ClientSampleId :

BD3A3


Tot Ion:163 Resp: 88213

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.5 7.9 11.9

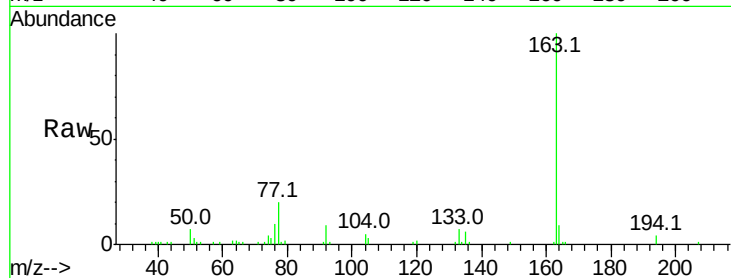

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

