

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005277.D
 Acq On : 06 May 2016 19:31
 Operator : UM/SJ
 Sample : PB90282BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.939	718	723	733	rBV	328664	542846	18.61%	1.999%
2	7.104	745	751	761	rBV	287126	449946	15.42%	1.657%
3	7.304	779	785	796	rBV	353244	562876	19.30%	2.073%
4	7.775	858	865	875	rBV	266391	447240	15.33%	1.647%
5	8.475	978	984	997	rBV	466256	749517	25.69%	2.761%
6	8.928	1054	1061	1077	rBV	369991	595512	20.41%	2.193%
7	9.645	1178	1183	1197	rBV	306645	509890	17.48%	1.878%
8	10.180	1268	1274	1290	rBV	437095	766700	26.28%	2.824%
9	10.557	1331	1338	1352	rBV	432531	757297	25.96%	2.789%
10	10.698	1356	1362	1381	rBV	457227	809193	27.74%	2.980%
11	13.821	1887	1893	1901	rBV	1028440	1435744	49.22%	5.288%
12	14.104	1933	1941	1953	rBV	1101609	1644087	56.36%	6.055%
13	14.415	1987	1994	2002	rBV2	736554	1137978	39.01%	4.191%
14	14.621	2023	2029	2053	rBV	378635	634626	21.76%	2.337%
15	15.410	2156	2163	2173	rBV	1469696	2145517	73.55%	7.902%
16	15.533	2178	2184	2200	rBV	480851	670186	22.97%	2.468%
17	17.162	2454	2461	2471	rBV2	990315	1456772	49.94%	5.366%
18	17.262	2471	2478	2495	rVV2	1604509	2398793	82.23%	8.835%
19	19.562	2862	2869	2882	rBV	2027724	2917094	100.00%	10.744%
20	21.356	3168	3174	3184	rBV	1398152	1873722	64.23%	6.901%
21	23.485	3528	3536	3552	rBV2	1422519	2793472	95.76%	10.289%
22	23.633	3553	3561	3577	rVB2	873707	1736855	59.54%	6.397%
23	24.138	3642	3647	3656	rVB2	32016	59598	2.04%	0.220%
24	24.891	3770	3775	3782	rVB2	27593	54999	1.89%	0.203%


Sum of corrected areas: 27150460

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005277.D
Acq On : 06 May 2016 19:31
Operator : UM/SJ
Sample : PB90282BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

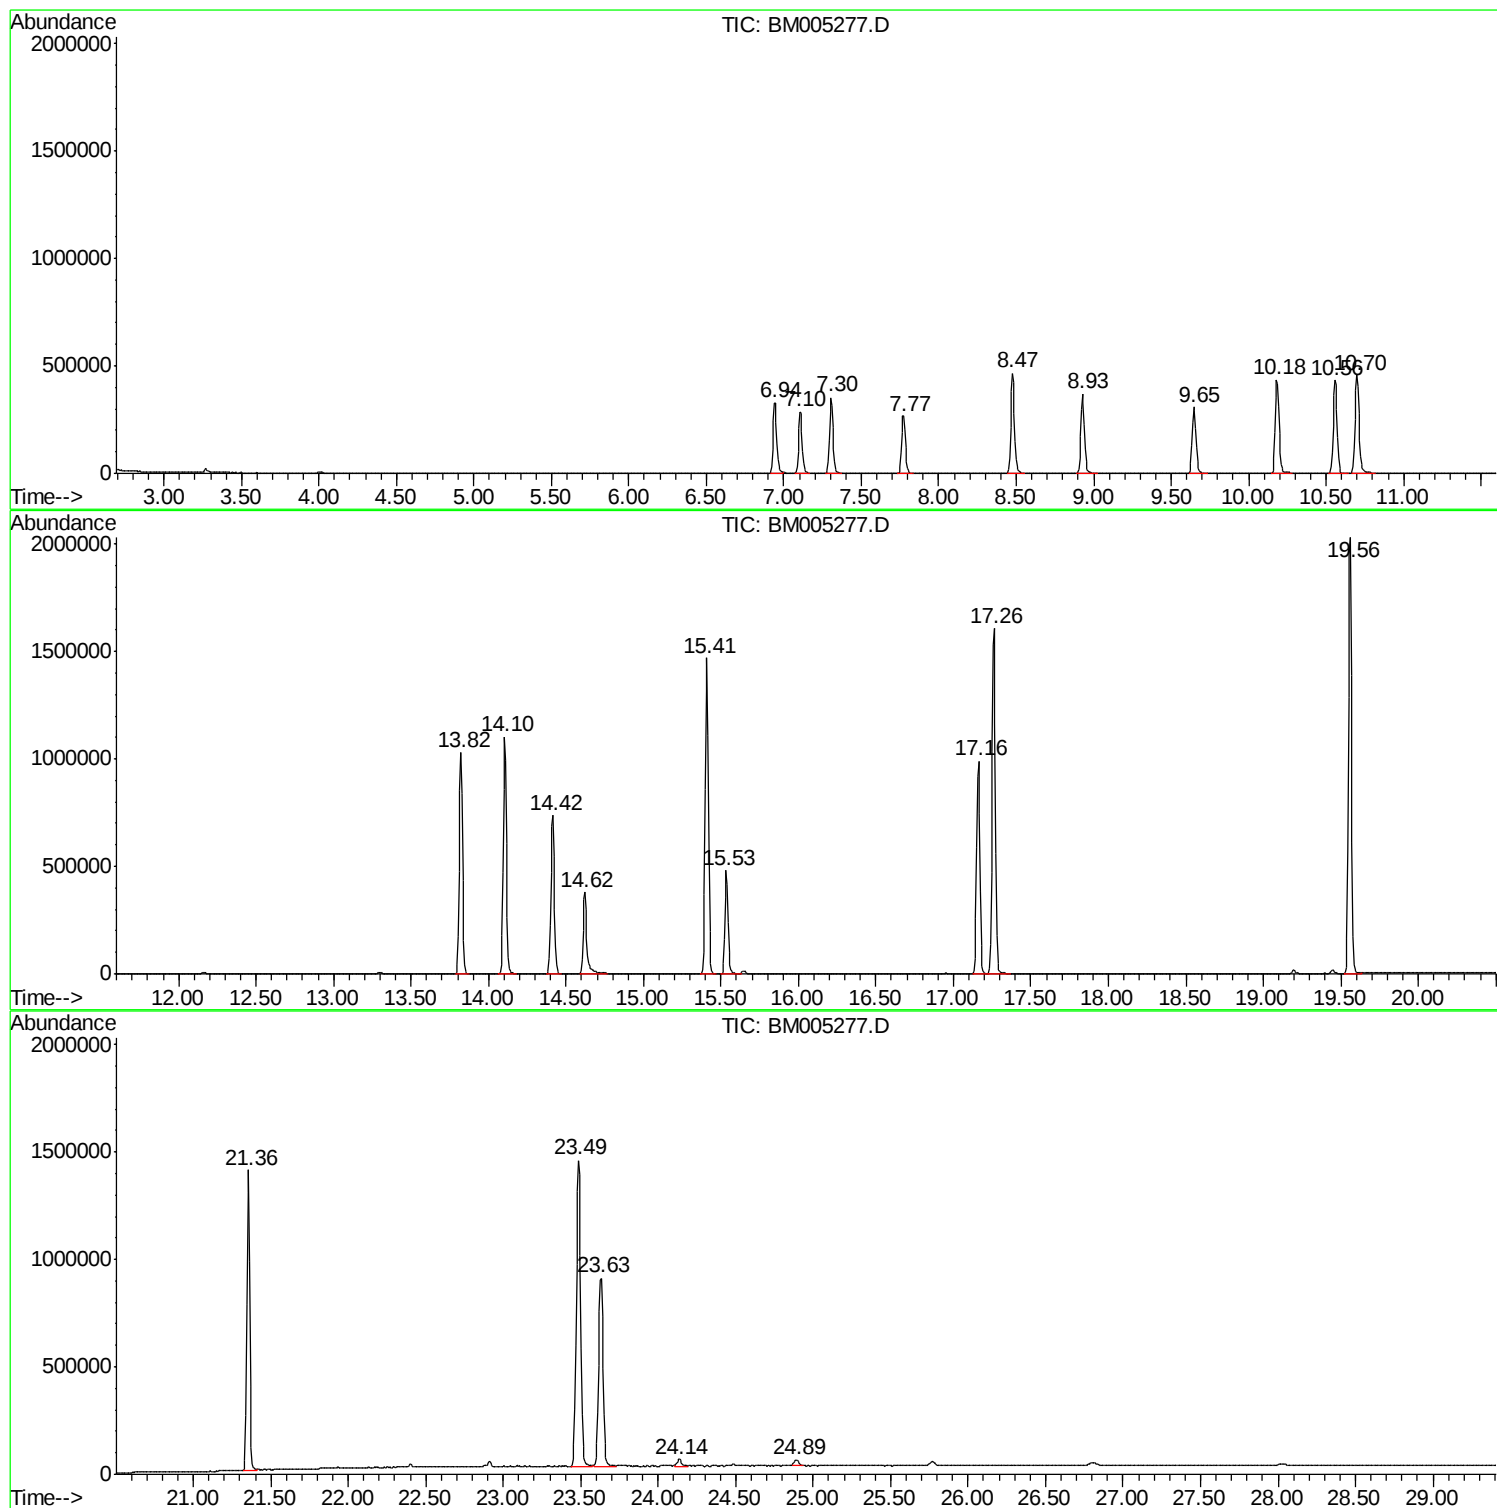

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005277.D
Acq On : 06 May 2016 19:31
Operator : UM/SJ
Sample : PB90282BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005277.D
Acq On : 06 May 2016 19:31
Operator : UM/SJ
Sample : PB90282BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc