

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005278.D
 Acq On : 06 May 2016 20:07
 Operator : UM/SJ
 Sample : H2820-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD388

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.734	4	8	17	rVB	21971	34852	1.93%	0.207%
2	2.863	27	30	37	rVB	16106	20377	1.13%	0.121%
3	3.010	52	55	61	rVB	29147	36971	2.05%	0.220%
4	6.946	719	724	733	rBV	123028	203951	11.31%	1.211%
5	7.104	745	751	767	rVB	106758	171306	9.50%	1.018%
6	7.304	779	785	797	rBV	129239	207854	11.52%	1.235%
7	7.775	856	865	873	rBV	219074	370022	20.52%	2.198%
8	8.475	979	984	994	rBV	133862	223677	12.40%	1.329%
9	8.928	1054	1061	1074	rBV	124125	207630	11.51%	1.233%
10	9.645	1176	1183	1194	rBV	100396	166834	9.25%	0.991%
11	10.187	1268	1275	1290	rBV	157936	280564	15.56%	1.666%
12	10.557	1331	1338	1349	rBV	365129	621974	34.48%	3.694%
13	10.698	1357	1362	1381	rBV	121600	233379	12.94%	1.386%
14	13.822	1887	1893	1897	rBV	397974	568727	31.53%	3.378%
15	13.869	1897	1901	1910	rVB	182655	252928	14.02%	1.502%
16	14.104	1935	1941	1951	rBV	424185	636446	35.29%	3.780%
17	14.416	1987	1994	2002	rVB2	608103	957319	53.08%	5.686%
18	14.627	2025	2030	2046	rBV	85848	176562	9.79%	1.049%
19	15.257	2132	2137	2142	rVB	26262	32645	1.81%	0.194%
20	15.404	2156	2162	2171	rBV	609780	902196	50.02%	5.359%
21	15.533	2179	2184	2198	rBV	154312	213214	11.82%	1.266%
22	15.651	2198	2204	2211	rBV3	10286	22377	1.24%	0.133%
23	16.121	2278	2284	2292	rBV	35302	62144	3.45%	0.369%
24	16.910	2414	2418	2422	rBV	28693	36180	2.01%	0.215%
25	16.963	2422	2427	2434	rVB4	10302	19021	1.05%	0.113%
26	17.163	2454	2461	2466	rBV2	839632	1246074	69.09%	7.401%
27	17.204	2466	2468	2472	rVV	40859	47339	2.62%	0.281%
28	17.257	2472	2477	2488	rVB2	707676	1038938	57.60%	6.171%
29	17.539	2519	2525	2538	rBV3	16939	38468	2.13%	0.228%
30	17.651	2540	2544	2548	rVV	17444	21621	1.20%	0.128%
31	18.051	2606	2612	2616	rBV2	40693	58607	3.25%	0.348%
32	18.915	2755	2759	2766	rBV3	15534	32427	1.80%	0.193%
33	19.221	2801	2811	2820	rBV	191968	267374	14.82%	1.588%
34	19.333	2826	2830	2833	rBV2	14134	18407	1.02%	0.109%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005278.D
Acq On : 06 May 2016 20:07
Operator : UM/SJ
Sample : H2820-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD388

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Title : SVOA CALIBRATION

35	19.556	2862	2868	2879	rBV3	996042	1576997	87.43%	9.367%
36	20.086	2948	2958	2964	rVB3	19421	39777	2.21%	0.236%
37	21.056	3117	3123	3132	rBV5	34972	94591	5.24%	0.562%
38	21.356	3166	3174	3178	rBV	1245621	1803654	100.00%	10.713%
39	21.392	3178	3180	3189	rVB	106090	118705	6.58%	0.705%
40	21.509	3196	3200	3206	rVB4	20219	31025	1.72%	0.184%
41	22.397	3348	3351	3356	rBV4	19643	28384	1.57%	0.169%
42	22.633	3387	3391	3396	rBV	48107	66524	3.69%	0.395%
43	22.915	3435	3439	3440	rBV	39287	50469	2.80%	0.300%
44	22.956	3440	3446	3459	rVB2	121264	391676	21.72%	2.326%
45	23.433	3521	3527	3529	rBV	51840	89397	4.96%	0.531%
46	23.480	3529	3535	3541	rVV2	629285	1179869	65.42%	7.008%
47	23.627	3552	3560	3575	rBV2	779819	1564261	86.73%	9.291%
48	24.139	3641	3647	3655	rVB	66987	129886	7.20%	0.771%
49	24.891	3770	3775	3786	rVB3	28749	74849	4.15%	0.445%
50	25.768	3919	3924	3931	rVB3	30864	67762	3.76%	0.402%
51	25.921	3945	3950	3960	rVB2	37493	99381	5.51%	0.590%


Sum of corrected areas: 16835612

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005278.D
Acq On : 06 May 2016 20:07
Operator : UM/SJ
Sample : H2820-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD388

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

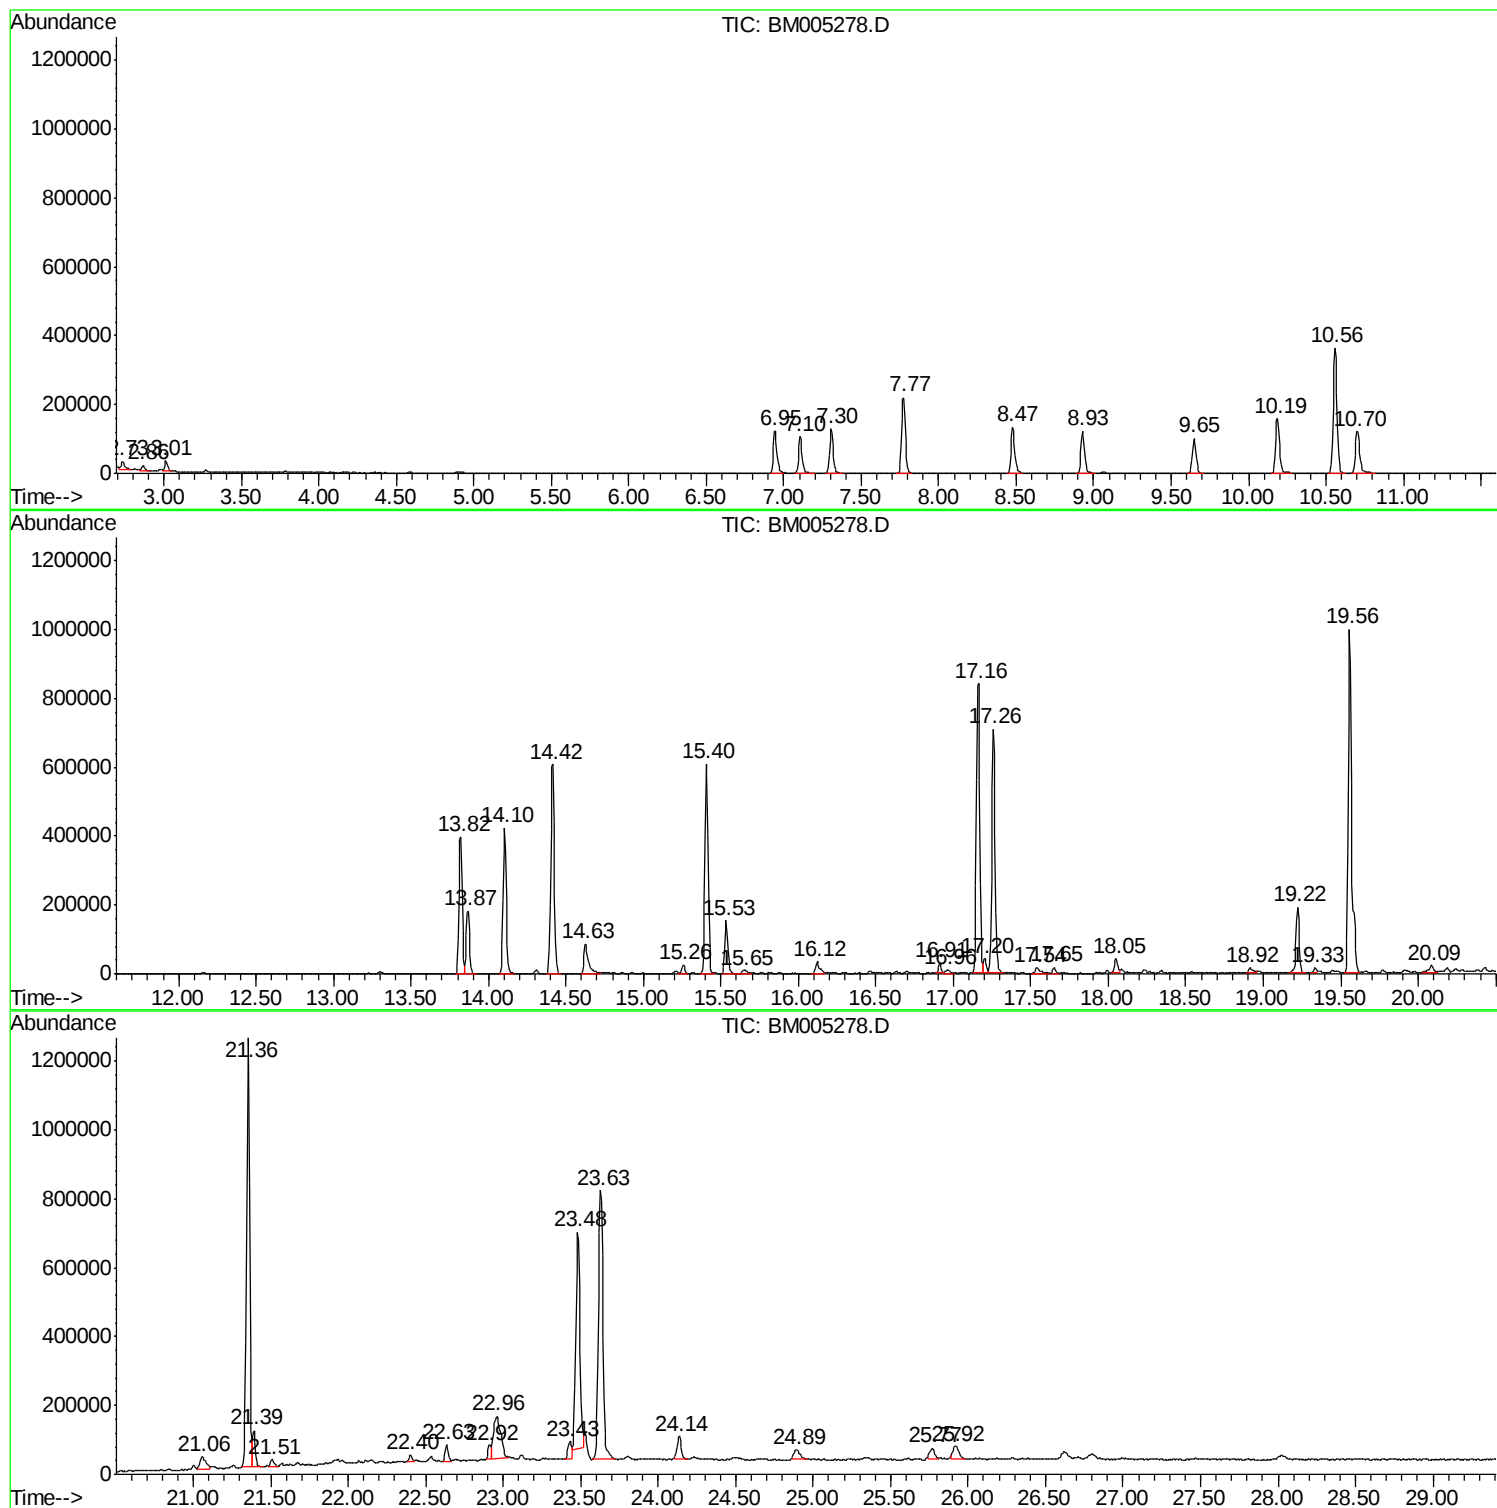

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005278.D
Acq On : 06 May 2016 20:07
Operator : UM/SJ
Sample : H2820-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD388

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005278.D
Acq On : 06 May 2016 20:07
Operator : UM/SJ
Sample : H2820-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD388

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc