

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005298.D
 Acq On : 07 May 2016 08:13
 Operator : UM/SJ
 Sample : H2743-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H4014

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.945	719	724	735	rBV	39561	65648	2.65%	0.331%
2	7.104	746	751	763	rBV	189375	296650	11.97%	1.496%
3	7.304	778	785	799	rBV	185414	300713	12.13%	1.516%
4	7.769	859	864	877	rVB	216578	363355	14.66%	1.832%
5	8.475	979	984	1001	rVB	142170	230775	9.31%	1.164%
6	8.928	1055	1061	1073	rBV	238737	398776	16.09%	2.011%
7	9.645	1177	1183	1196	rVB	206220	332976	13.43%	1.679%
8	10.181	1269	1274	1293	rBV	271033	487348	19.66%	2.457%
9	10.557	1331	1338	1347	rBV	370703	629329	25.39%	3.173%
10	13.821	1887	1893	1903	rBV	708458	997189	40.23%	5.028%
11	14.104	1934	1941	1952	rBV	773337	1139936	45.99%	5.747%
12	14.410	1987	1993	2002	rBV2	619196	969261	39.10%	4.887%
13	14.633	2026	2031	2042	rBV	19422	44598	1.80%	0.225%
14	15.410	2156	2163	2179	rVB	1090157	1647247	66.45%	8.305%
15	15.533	2179	2184	2196	rBV	395297	537797	21.70%	2.711%
16	17.162	2454	2461	2471	rBV2	815431	1216732	49.09%	6.135%
17	17.257	2471	2477	2490	rVV2	1337378	2017292	81.38%	10.171%
18	19.556	2862	2868	2878	rBV2	1714426	2478788	100.00%	12.498%
19	21.350	3168	3173	3186	rBV	1201322	1589656	64.13%	8.015%
20	22.909	3434	3438	3443	rVB	26208	38466	1.55%	0.194%
21	23.480	3527	3535	3547	rBV2	1231764	2385446	96.23%	12.027%
22	23.621	3552	3559	3572	rVB2	735891	1461691	58.97%	7.370%
23	24.133	3641	3646	3654	rVB	43414	76069	3.07%	0.384%
24	24.885	3769	3774	3782	rVB	39422	76873	3.10%	0.388%
25	25.768	3919	3924	3931	rVB2	22772	51453	2.08%	0.259%


Sum of corrected areas: 19834064

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005298.D
Acq On : 07 May 2016 08:13
Operator : UM/SJ
Sample : H2743-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4014

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

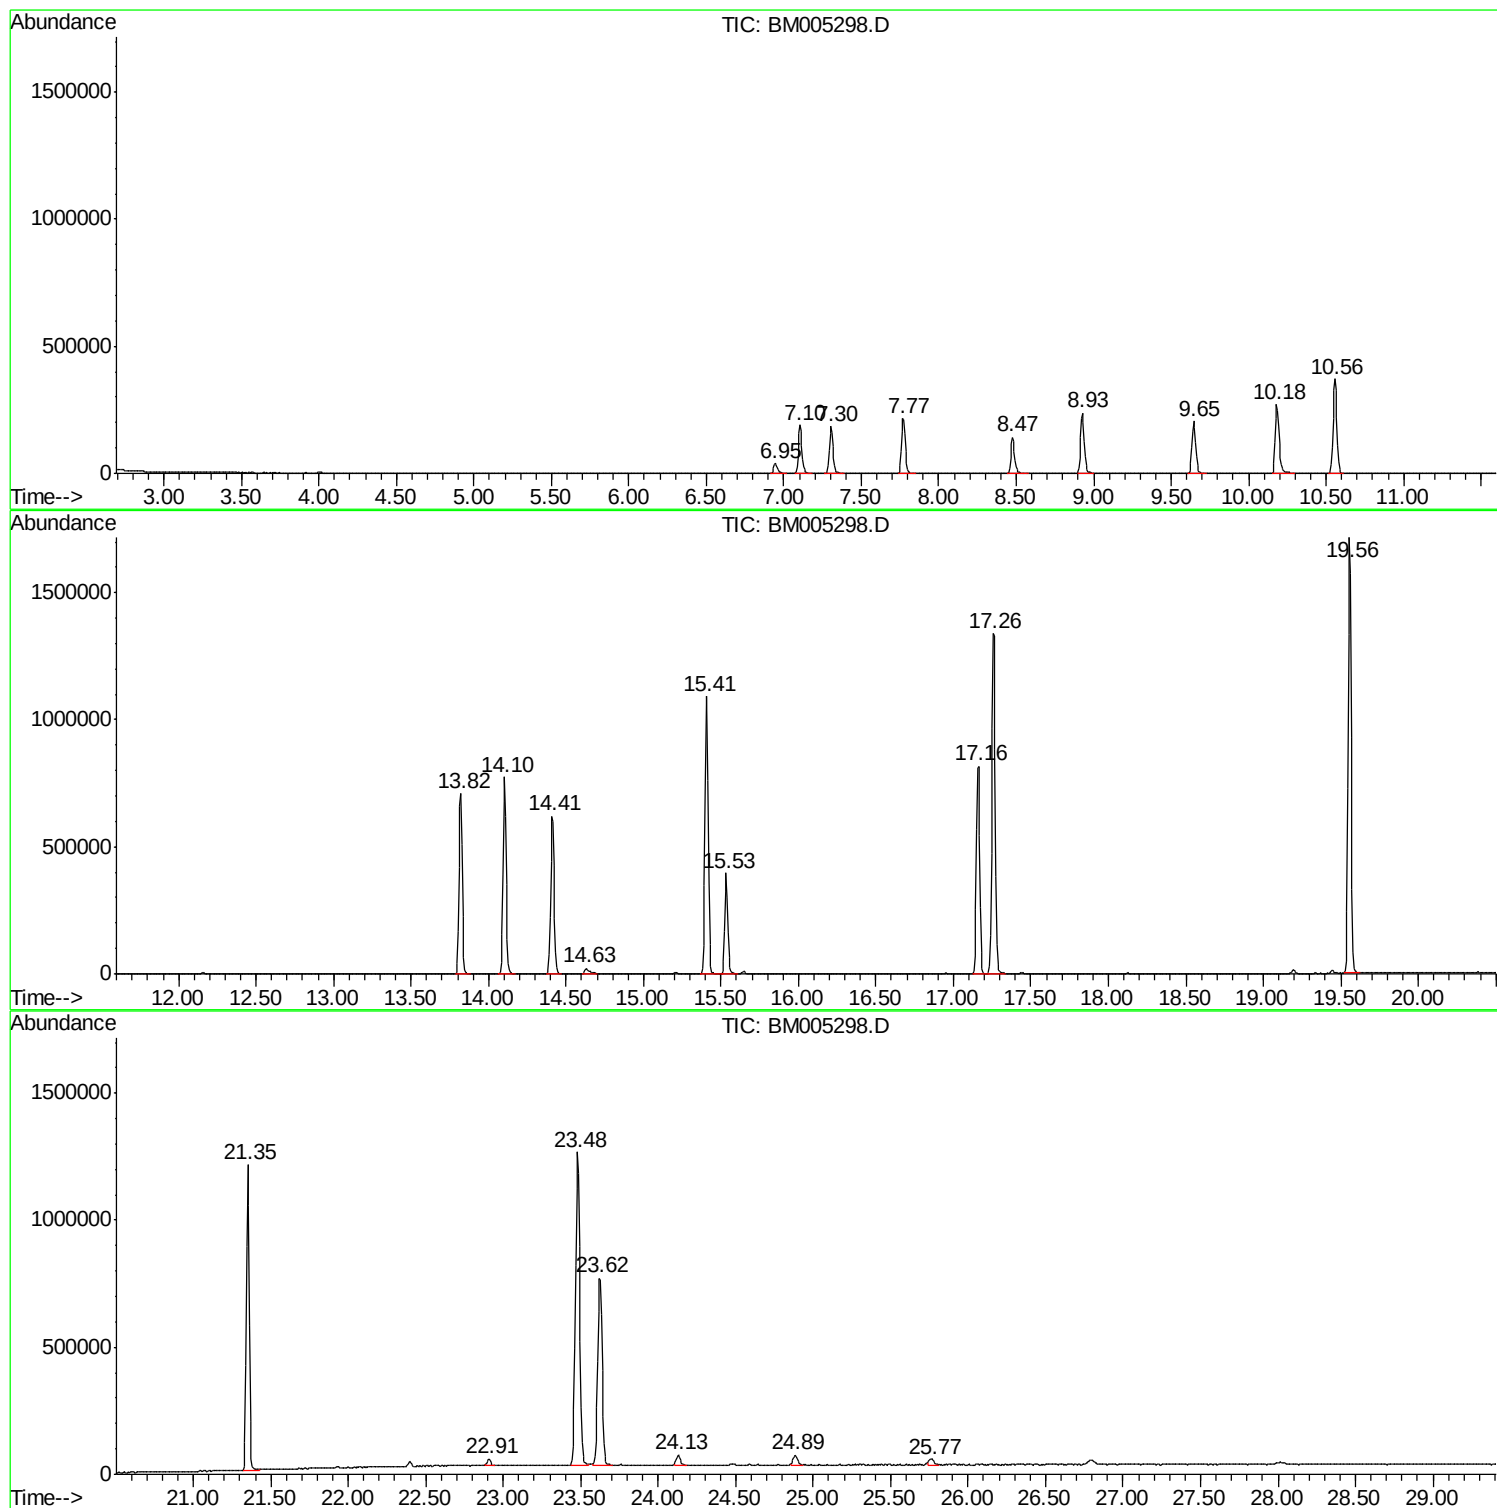

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005298.D
Acq On : 07 May 2016 08:13
Operator : UM/SJ
Sample : H2743-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4014

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005298.D
Acq On : 07 May 2016 08:13
Operator : UM/SJ
Sample : H2743-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4014

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc