

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005301.D
 Acq On : 07 May 2016 10:01
 Operator : UM/SJ
 Sample : H2743-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H4011

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.516	304	311	322	rBV	197583	318004	12.45%	1.489%
2	6.946	719	724	733	rBV	45587	75556	2.96%	0.354%
3	7.105	746	751	767	rVB	209397	329994	12.92%	1.545%
4	7.305	779	785	796	rVB	208418	332485	13.02%	1.556%
5	7.769	859	864	877	rBV	232794	385206	15.08%	1.803%
6	8.475	978	984	993	rBV	167510	269202	10.54%	1.260%
7	8.928	1055	1061	1071	rBV	269029	440579	17.25%	2.062%
8	9.646	1177	1183	1193	rBV	227572	370484	14.50%	1.734%
9	10.181	1268	1274	1293	rBV	310616	552740	21.64%	2.587%
10	10.557	1330	1338	1346	rBV	386967	651431	25.50%	3.049%
11	13.822	1886	1893	1901	rBV	792412	1128333	44.17%	5.282%
12	14.104	1934	1941	1953	rBV	865031	1313788	51.43%	6.150%
13	14.410	1987	1993	2002	rVB2	643277	989711	38.74%	4.633%
14	14.628	2026	2030	2042	rBV2	22671	49662	1.94%	0.232%
15	15.404	2156	2162	2173	rBV	1205796	1802954	70.58%	8.440%
16	15.533	2179	2184	2198	rVB	412771	558577	21.87%	2.615%
17	17.157	2454	2460	2471	rBV2	882896	1281057	50.15%	5.997%
18	17.257	2471	2477	2493	rVV	1441239	2106156	82.45%	9.859%
19	19.557	2862	2868	2881	rBV2	1794713	2554598	100.00%	11.959%
20	21.351	3168	3173	3183	rBV	1271589	1641848	64.27%	7.686%
21	22.398	3347	3351	3356	rBV	21593	27536	1.08%	0.129%
22	22.909	3434	3438	3442	rVB	27282	38703	1.52%	0.181%
23	23.480	3527	3535	3551	rBV2	1292712	2444062	95.67%	11.441%
24	23.627	3552	3560	3571	rVB2	759525	1496600	58.58%	7.006%
25	24.133	3641	3646	3654	rVB	40249	73327	2.87%	0.343%
26	24.886	3768	3774	3782	rVB	37148	77352	3.03%	0.362%
27	25.756	3918	3922	3932	rVB3	22456	52172	2.04%	0.244%


Sum of corrected areas: 21362117

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005301.D
Acq On : 07 May 2016 10:01
Operator : UM/SJ
Sample : H2743-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4011

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

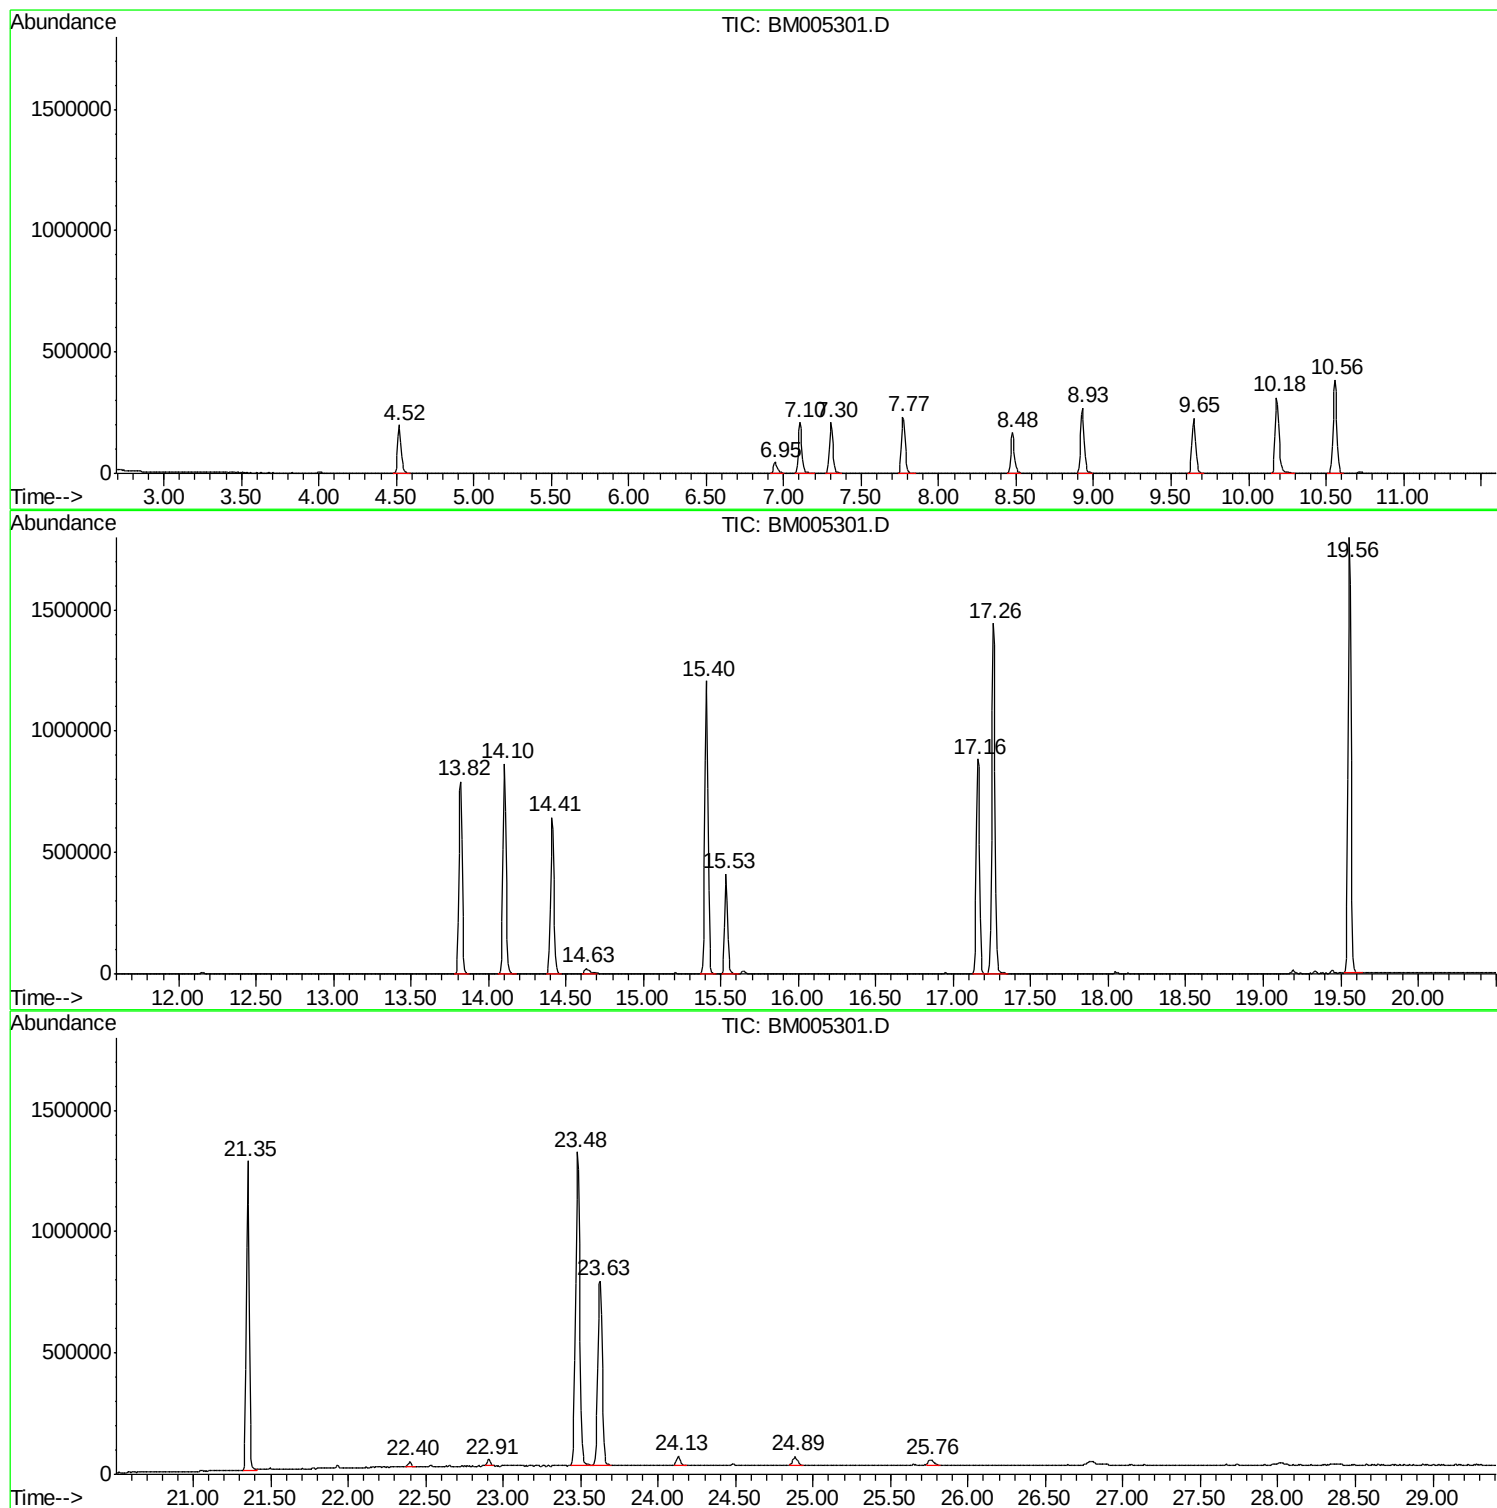

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005301.D
Acq On : 07 May 2016 10:01
Operator : UM/SJ
Sample : H2743-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4011

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005301.D
Acq On : 07 May 2016 10:01
Operator : UM/SJ
Sample : H2743-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4011

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc