

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005303.D
 Acq On : 07 May 2016 11:14
 Operator : UM/SJ
 Sample : H2743-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H4007

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.516	305	311	323	rVB	261514	415832	16.41%	2.044%
2	6.946	717	724	735	rBV	34313	61885	2.44%	0.304%
3	7.104	746	751	761	rBV	171453	268136	10.58%	1.318%
4	7.304	779	785	795	rBV	169202	270998	10.69%	1.332%
5	7.769	858	864	874	rBV	249415	405688	16.01%	1.994%
6	8.475	979	984	993	rBV	130080	210979	8.33%	1.037%
7	8.928	1055	1061	1072	rBV	216124	359237	14.18%	1.766%
8	9.645	1177	1183	1196	rVB	183424	299132	11.80%	1.471%
9	10.181	1269	1274	1288	rBV	245972	439426	17.34%	2.160%
10	10.557	1331	1338	1347	rBV	403952	682073	26.92%	3.353%
11	13.822	1886	1893	1900	rBV	661681	949564	37.47%	4.668%
12	14.104	1934	1941	1955	rBV	713158	1065302	42.04%	5.237%
13	14.410	1987	1993	2002	rVB2	666207	1034651	40.83%	5.086%
14	14.633	2027	2031	2043	rBV2	19551	47980	1.89%	0.236%
15	15.404	2156	2162	2170	rBV	1037857	1529346	60.35%	7.518%
16	15.533	2178	2184	2197	rBV	400509	550335	21.72%	2.705%
17	17.157	2454	2460	2468	rBV2	926464	1344839	53.07%	6.611%
18	17.257	2471	2477	2494	rVB2	1323795	1997478	78.82%	9.819%
19	19.556	2862	2868	2881	rBV2	1749606	2534107	100.00%	12.457%
20	21.350	3168	3173	3184	rBV	1338106	1735442	68.48%	8.531%
21	22.909	3435	3438	3442	rVB2	20732	27708	1.09%	0.136%
22	23.480	3527	3535	3547	rBV2	1237990	2419405	95.47%	11.894%
23	23.627	3552	3560	3574	rVB2	825330	1604426	63.31%	7.887%
24	24.133	3641	3646	3652	rVB	24388	44013	1.74%	0.216%
25	24.886	3770	3774	3780	rVB2	22511	44060	1.74%	0.217%


Sum of corrected areas: 20342042

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005303.D
Acq On : 07 May 2016 11:14
Operator : UM/SJ
Sample : H2743-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4007

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

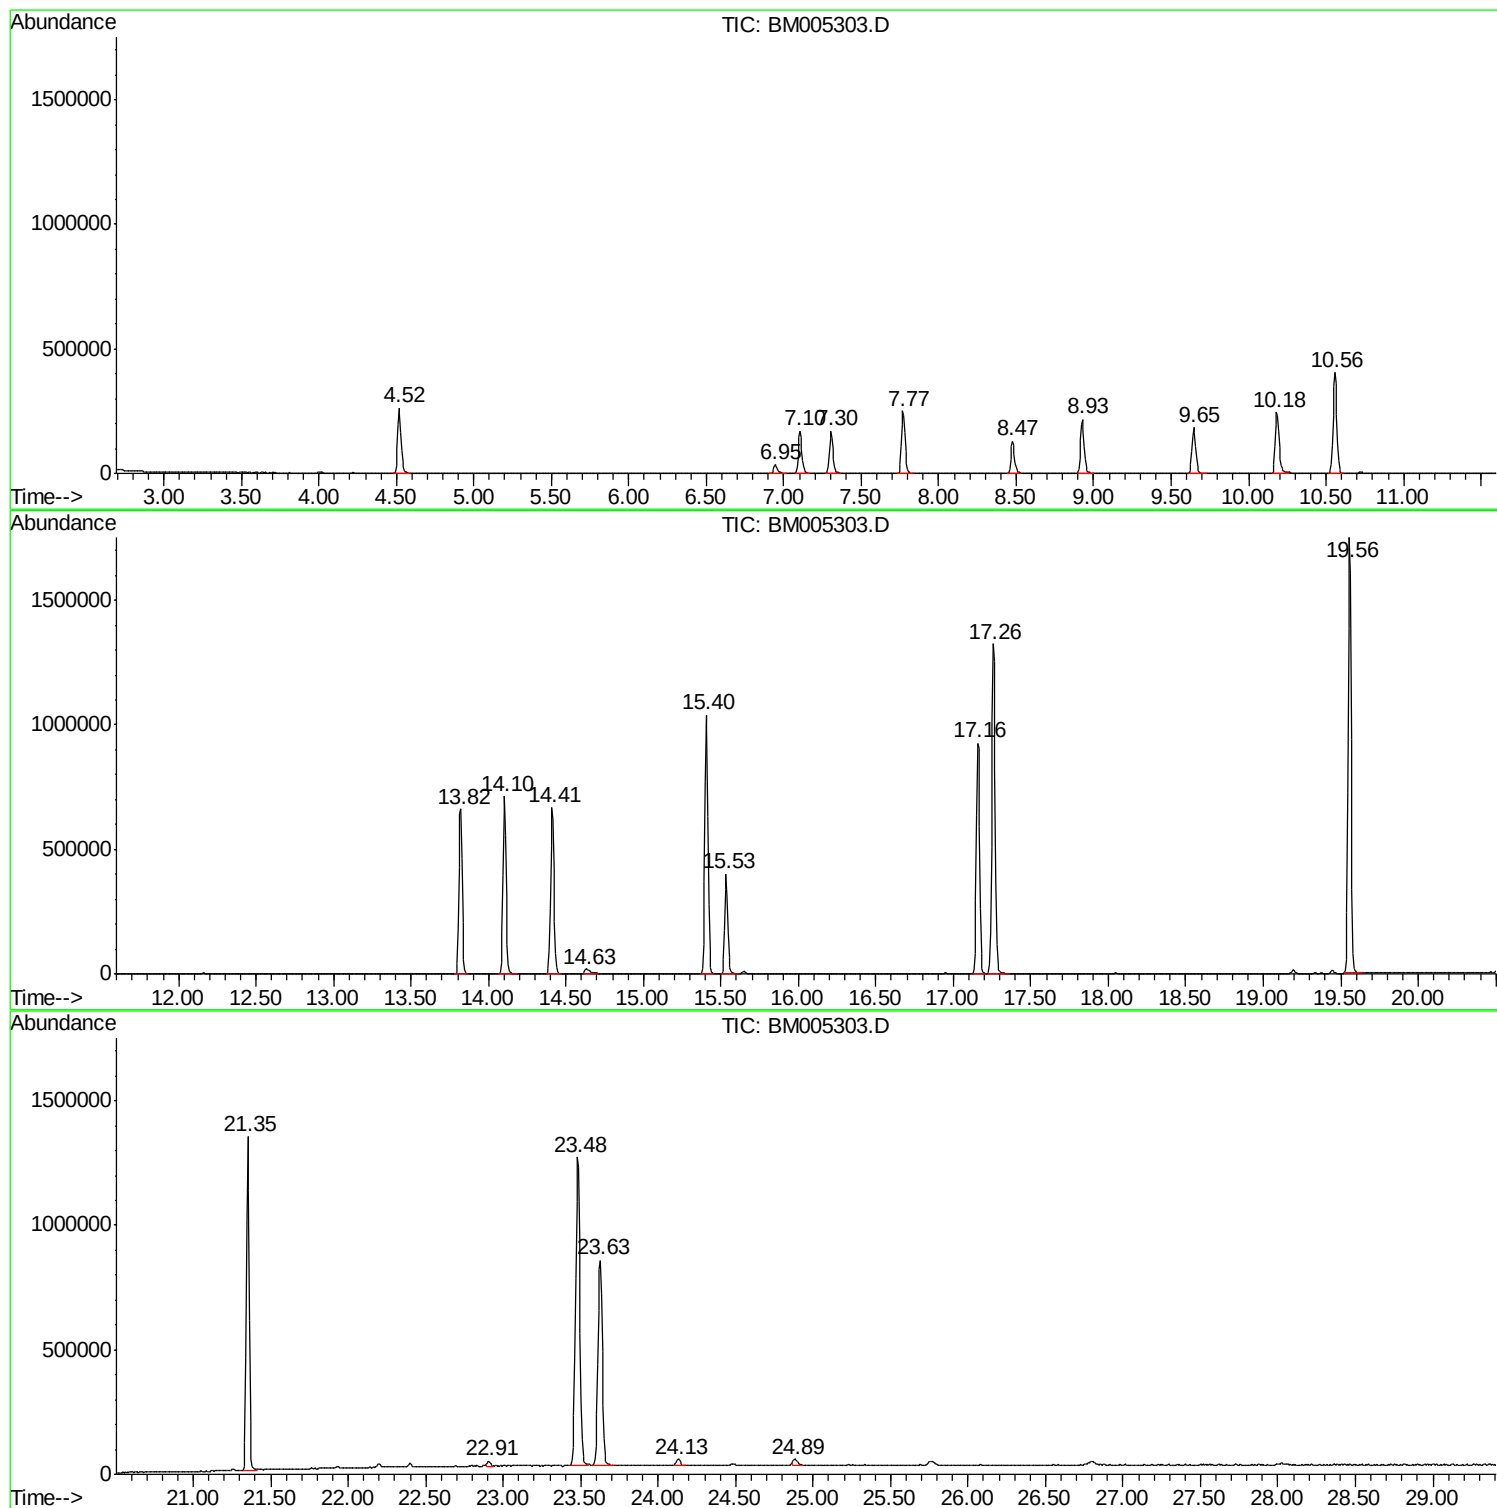

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005303.D
Acq On : 07 May 2016 11:14
Operator : UM/SJ
Sample : H2743-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4007

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005303.D
Acq On : 07 May 2016 11:14
Operator : UM/SJ
Sample : H2743-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4007

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc