

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
 Data File : BM005304.D
 Acq On : 07 May 2016 11:50
 Operator : UM/SJ
 Sample : H2743-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H4015

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	719	724	733	rBV	47092	77607	2.85%	0.363%
2	7.104	745	751	764	rVB	215489	332981	12.24%	1.556%
3	7.304	779	785	799	rBV	207985	342860	12.60%	1.602%
4	7.769	859	864	875	rVB	227640	368664	13.55%	1.723%
5	8.475	979	984	994	rBV	171564	274783	10.10%	1.284%
6	8.928	1055	1061	1075	rBV	270106	454836	16.72%	2.125%
7	9.645	1177	1183	1195	rBV	232187	382482	14.06%	1.787%
8	10.181	1268	1274	1288	rBV	317853	572555	21.04%	2.675%
9	10.557	1331	1338	1346	rBV	377130	627950	23.08%	2.934%
10	13.822	1886	1893	1908	rBV	797916	1131334	41.58%	5.287%
11	14.104	1934	1941	1955	rBV	886182	1319329	48.49%	6.165%
12	14.410	1987	1993	2003	rVB2	618494	960246	35.29%	4.487%
13	14.628	2026	2030	2038	rBV	25339	51720	1.90%	0.242%
14	15.404	2156	2162	2171	rBV	1223004	1813255	66.64%	8.473%
15	15.533	2178	2184	2196	rBV	445968	608427	22.36%	2.843%
16	17.157	2454	2460	2467	rBV2	846246	1244857	45.75%	5.817%
17	17.257	2471	2477	2488	rBV2	1465932	2202060	80.93%	10.290%
18	19.557	2862	2868	2881	rBV2	1880191	2720909	100.00%	12.715%
19	21.351	3168	3173	3181	rBV	1258221	1625036	59.72%	7.594%
20	22.198	3313	3317	3321	rVB	39268	48157	1.77%	0.225%
21	22.909	3435	3438	3442	rVB	21131	27703	1.02%	0.129%
22	23.480	3527	3535	3548	rBV2	1328570	2623692	96.43%	12.260%
23	23.627	3552	3560	3570	rVB2	765353	1491138	54.80%	6.968%
24	24.133	3640	3646	3651	rBV	25408	50041	1.84%	0.234%
25	24.886	3769	3774	3780	rVB2	24621	47395	1.74%	0.221%


Sum of corrected areas: 21400017

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050616\
Data File : BM005304.D
Acq On : 07 May 2016 11:50
Operator : UM/SJ
Sample : H2743-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4015

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

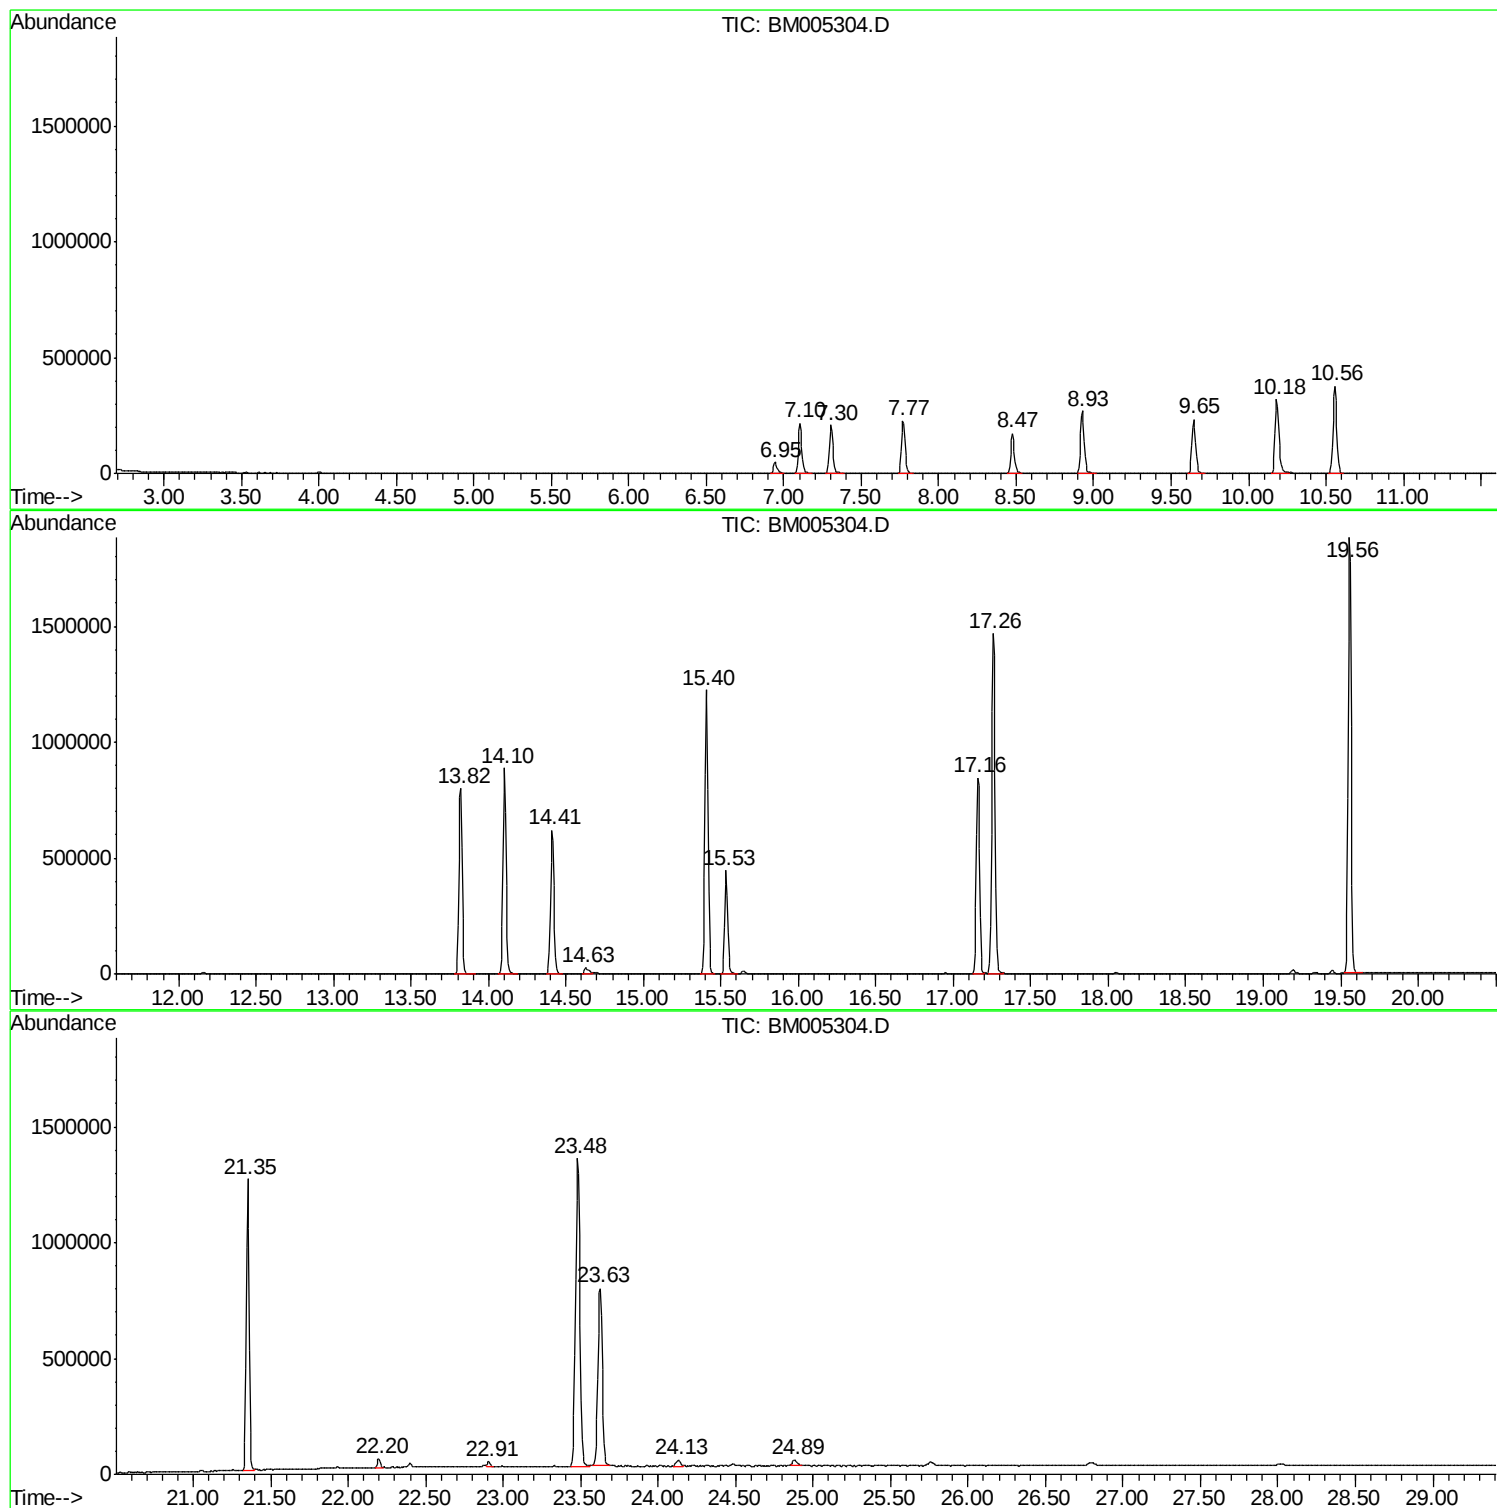

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005304.D
Acq On : 07 May 2016 11:50
Operator : UM/SJ
Sample : H2743-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4015

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050616\
Data File : BM005304.D
Acq On : 07 May 2016 11:50
Operator : UM/SJ
Sample : H2743-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4015

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc