
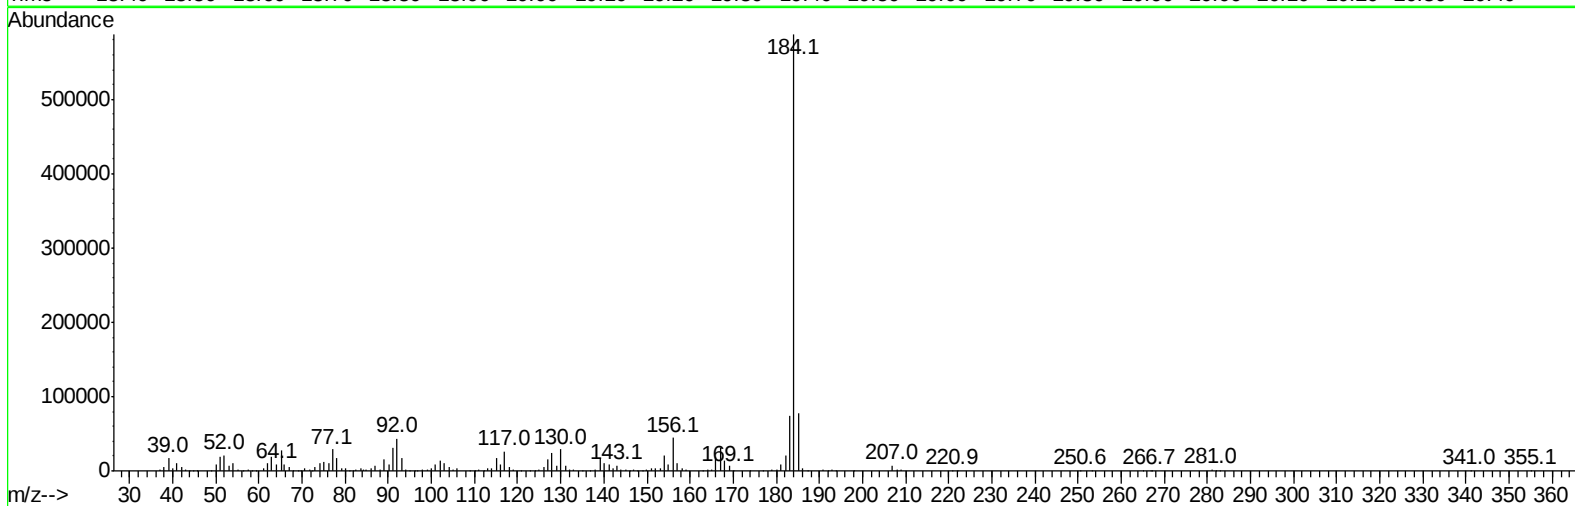


Data Path : Z:\HPCHEM1\BNA M\Data\BM050617\
Data File : BM009931.D
Acq On : 06 May 2017 08:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 01:24:09 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:52:12 2017
Response via : Initial Calibration

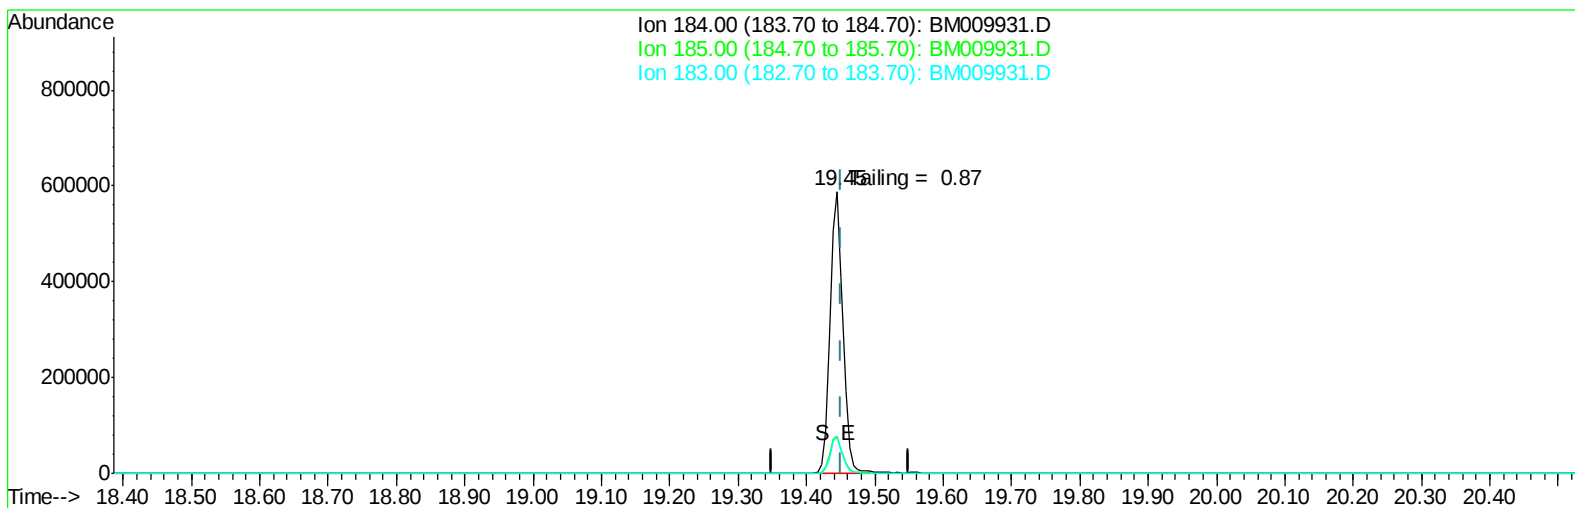

TIC: BM009931.D

(76) Benzidine



19.445min (-0.006) 8000.29ng

response 766500

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.10
183.00	11.10	12.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM050617\
Data File : BM009931.D
Acq On : 06 May 2017 08:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 01:24:09 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:52:12 2017
Response via : Initial Calibration

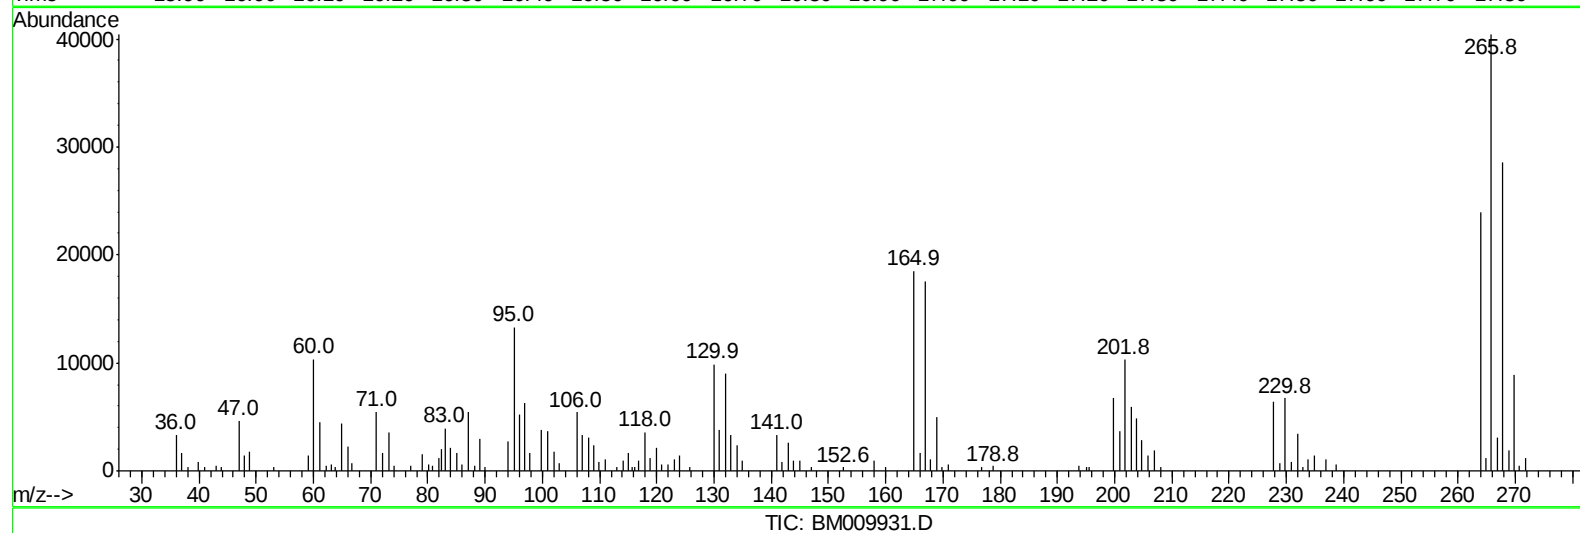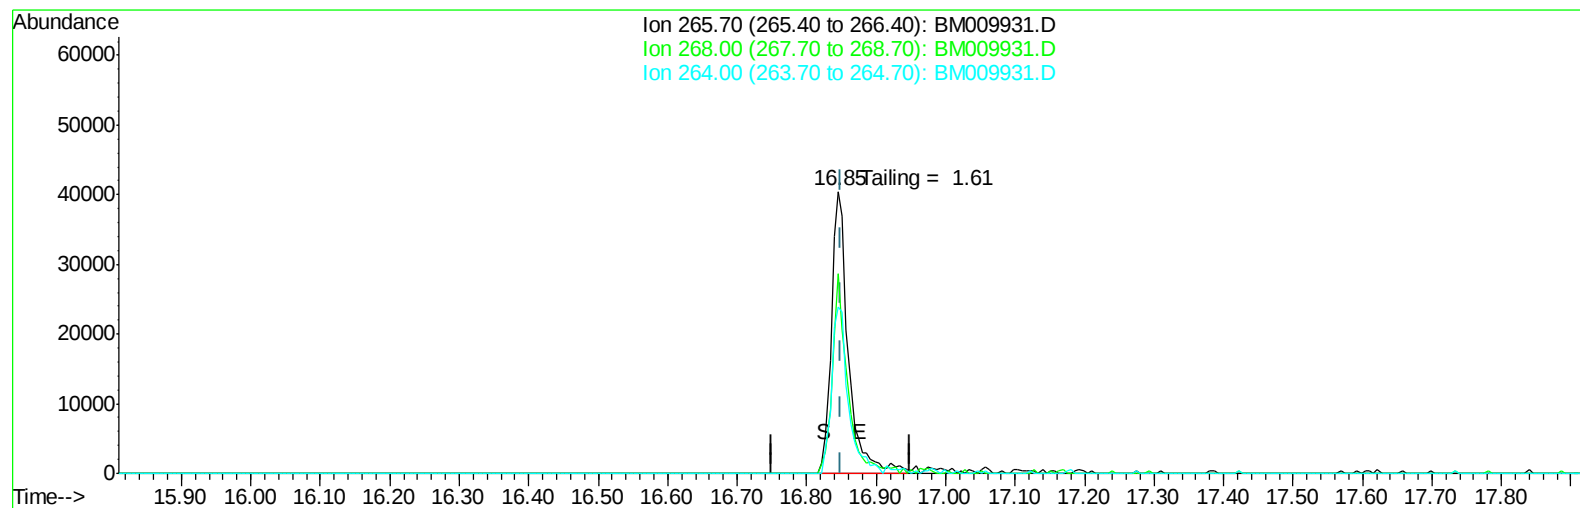

(69) Pentachlorophenol (C)

16.845min (-0.005) 0.00ng m

response 69299

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	70.82
264.00	61.20	59.30
0.00	0.00	0.00