

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050617\
 Data File : BM009958.D
 Acq On : 07 May 2017 01:39
 Operator : SJ/MA
 Sample : I2995-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-AOC17-003

Quant Time: May 08 05:45:28 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 14:52:12 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	76206	20.00	ng	0.00
21) Naphthalene-d8	10.57	136	308042	20.00	ng	-0.01
38) Acenaphthene-d10	14.43	164	187098	20.00	ng	-0.01
63) Phenanthrene-d10	17.18	188	463890	20.00	ng	-0.02
75) Chrysene-d12	21.37	240	507913	20.00	ng	-0.02
86) Perylene-d12	23.67	264	388583	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	752604	157.23	ng	0.00
7) Phenol-d6	6.96	99	1039103	141.62	ng	-0.01
23) Nitrobenzene-d5	8.95	82	865049	101.62	ng	-0.01
41) 2,4,6-Tribromophenol	15.93	330	415801	162.72	ng	-0.01
44) 2-Fluorobiphenyl	13.04	172	1400054	97.50	ng	-0.01
78) Terphenyl-d14	19.80	244	2668632	107.78	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050617\
Data File : BM009958.D
Acq On : 07 May 2017 01:39
Operator : SJ/MA
Sample : I2995-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-AOC17-003

Quant Time: May 08 05:45:28 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:52:12 2017
Response via : Initial Calibration

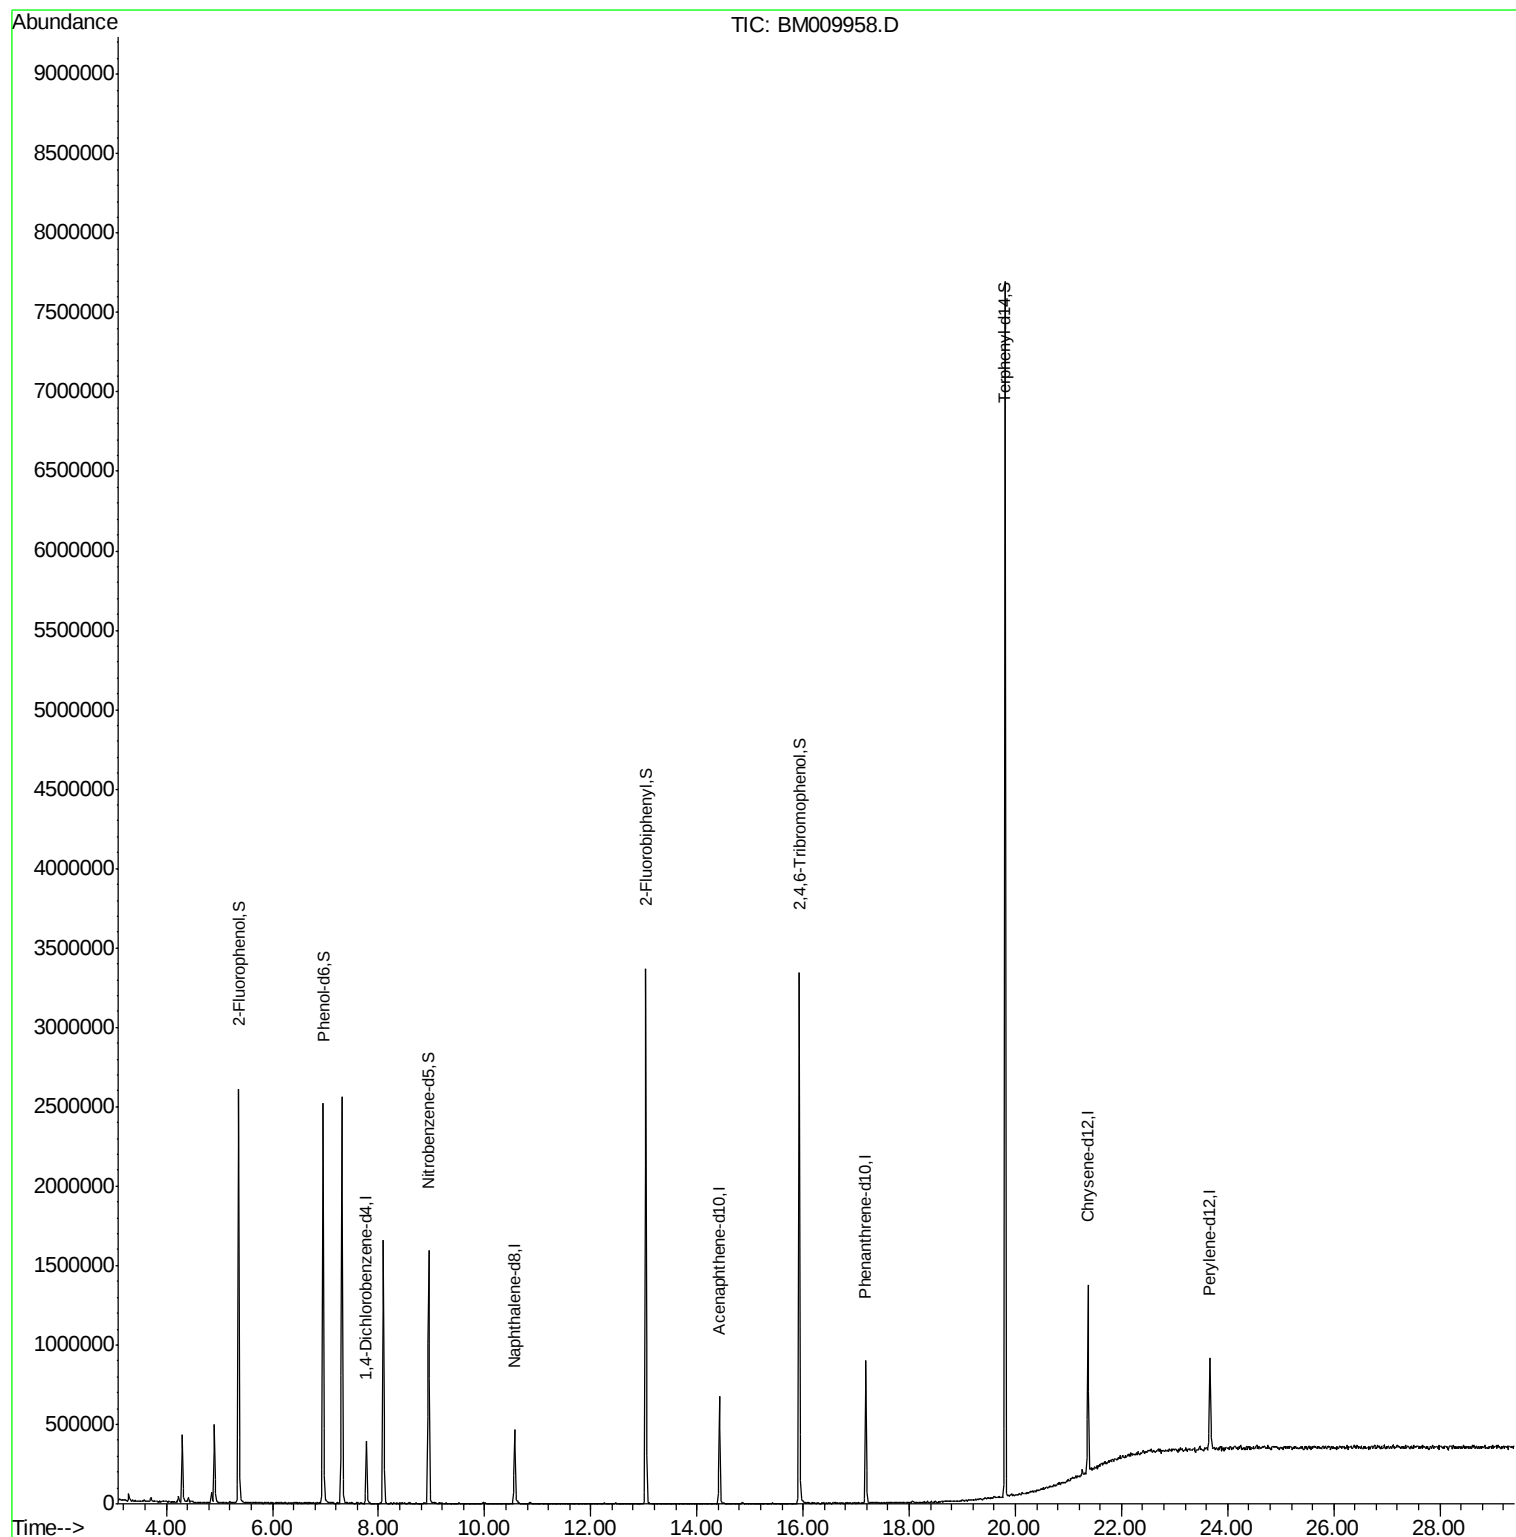

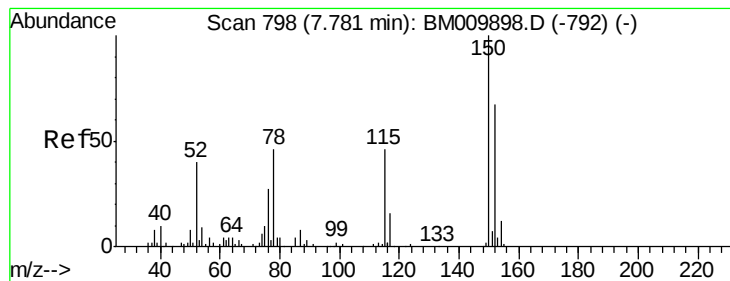


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.77 min Scan# 797
Delta R.T. -0.01 min
Lab File: BM009958.D
Acq: 07 May 2017 01:39

Instrument :
BNA_M
ClientSampleId :
WC-AOC17-003

Tgt Ion:152 Resp: 76206
Ion Ratio Lower Upper
152 100
150 141.6 119.5 179.3
115 61.4 43.0 64.4

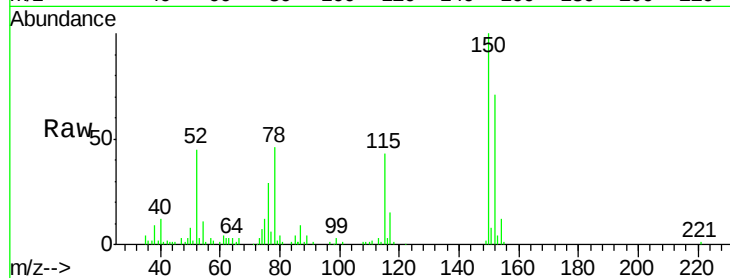


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

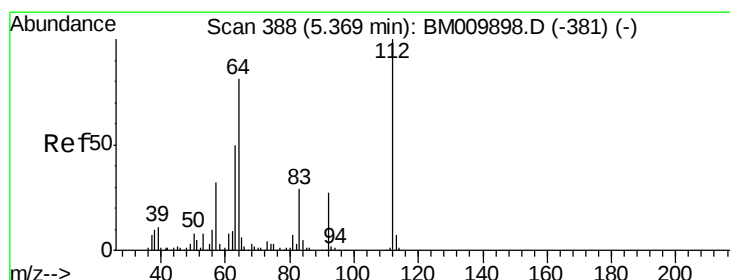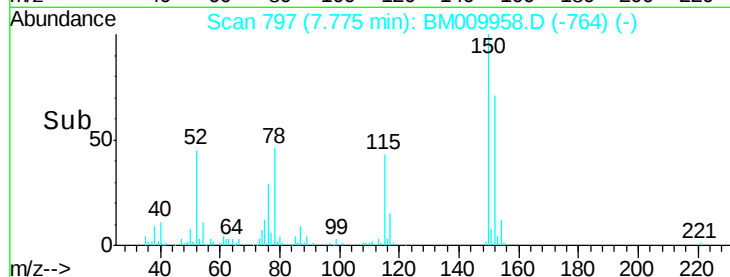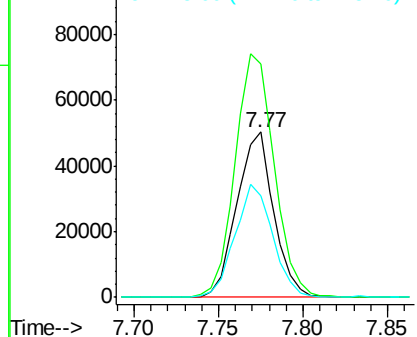



#5


2-Fluorophenol
Concen: 157.23 ng
RT: 5.36 min Scan# 387
Delta R.T. -0.01 min
Lab File: BM009958.D
Acq: 07 May 2017 01:39

Tgt Ion:112 Resp: 752604
Ion Ratio Lower Upper
112 100
64 82.2 38.6 57.8#
63 50.6 19.3 28.9#

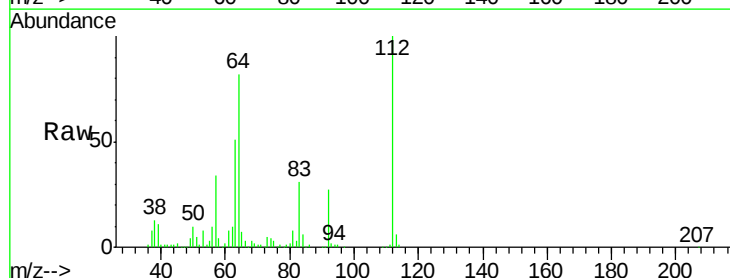

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

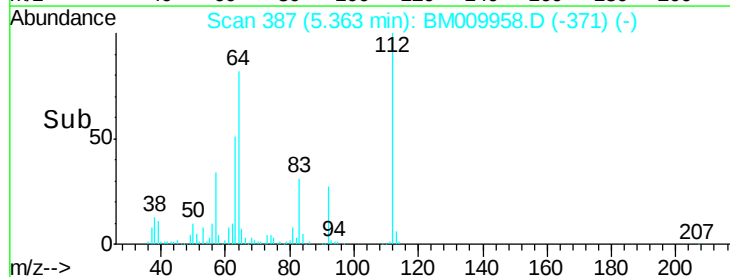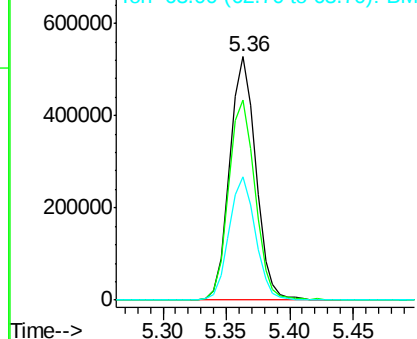

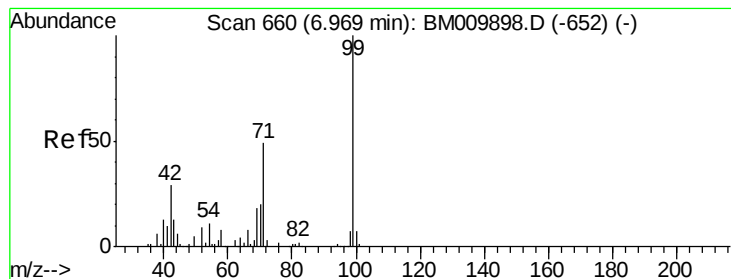

#7

Phenol-d6

Concen: 141.62 ng

RT: 6.96 min Scan# 658

Delta R.T. -0.01 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39

Instrument :

BNA_M

ClientSampleId :

WC-AOC17-003


Tgt Ion: 99 Resp: 1039103

Ion Ratio Lower Upper

99 100

42 31.9 11.0 16.4#




71 49.8 23.4 35.2#

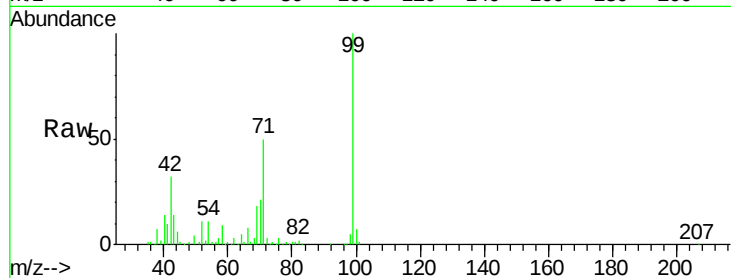

Abundance Ion 99.00 (98.70 to 99.70): BM009958.D (-652) (-)

Ion 42.00 (41.70 to 42.70): BM009958.D (-652) (-)

Ion 71.00 (70.70 to 71.70): BM009958.D (-652) (-)

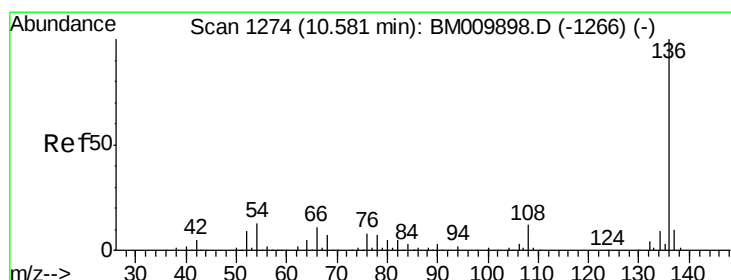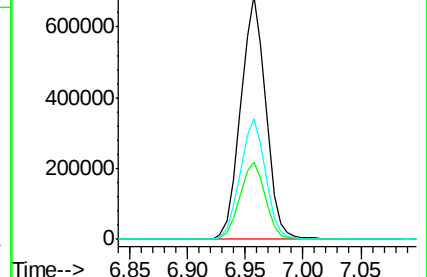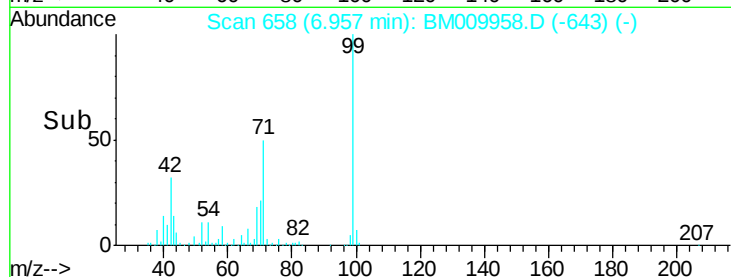

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.57 min Scan# 1272

Delta R.T. -0.01 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39

Tgt Ion: 136 Resp: 308042


Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 13.3 4.6 6.8#

68 7.6 3.7 5.5#


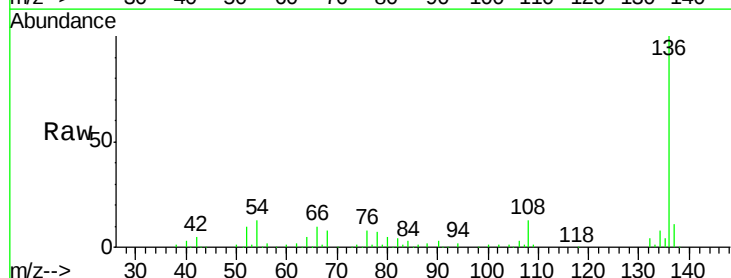



Abundance Ion 136.00 (135.70 to 136.70): BM009958.D (-1266) (-)

Ion 137.00 (136.70 to 137.70): BM009958.D (-1266) (-)

Ion 54.00 (53.70 to 54.70): BM009958.D (-1266) (-)

Ion 68.00 (67.70 to 68.70): BM009958.D (-1266) (-)



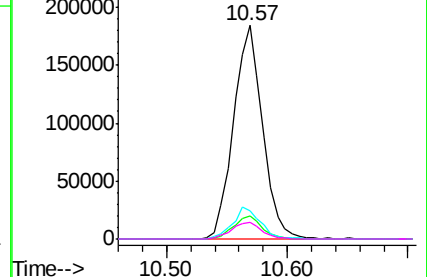
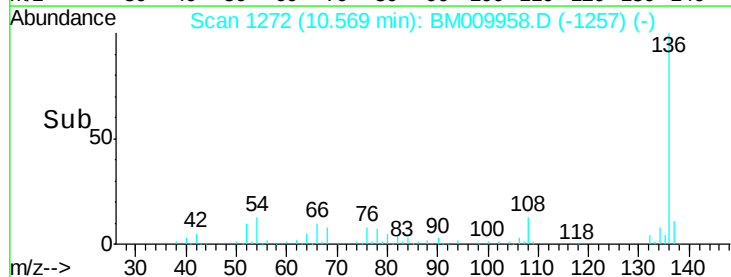


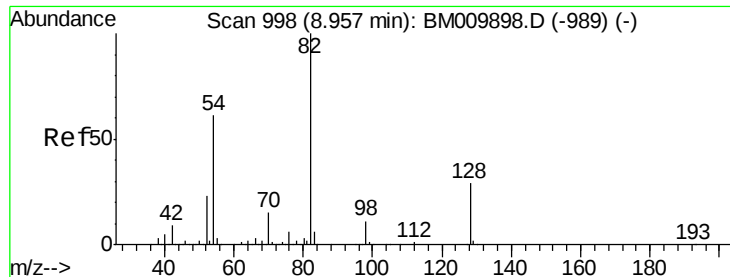

#23
 Nitrobenzene-d5
 Concen: 101.62 ng
 RT: 8.95 min Scan# 996
 Delta R.T. -0.01 min
 Lab File: BM009958.D
 Acq: 07 May 2017 01:39




Instrument :
 BNA_M
 ClientSampleId :
 WC-AOC17-003


Tgt Ion: 82 Resp: 865049
 Ion Ratio Lower Upper
 82 100
 128 26.6 32.8 49.2#
 54 61.3 40.6 60.8#

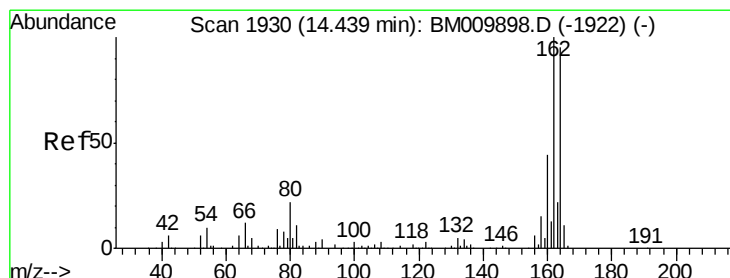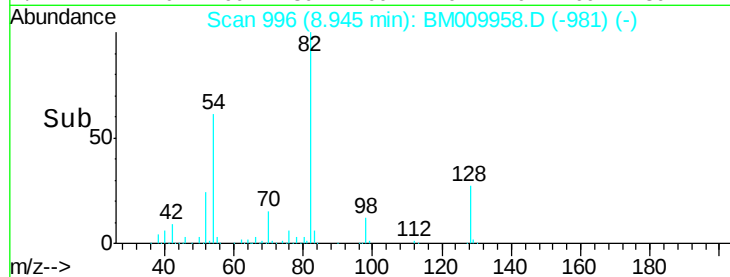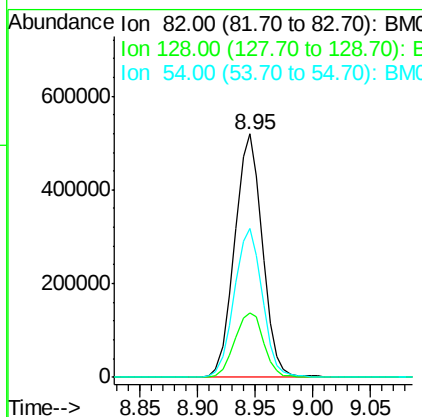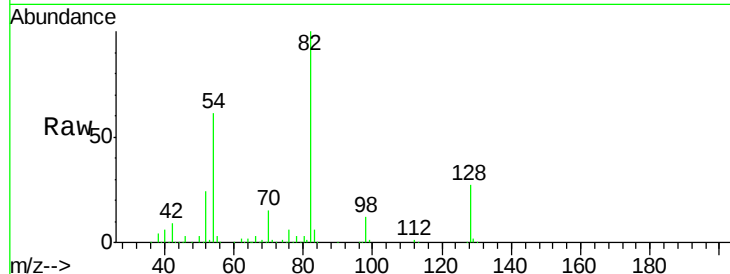

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1928
 Delta R.T. -0.01 min
 Lab File: BM009958.D
 Acq: 07 May 2017 01:39

Tgt Ion: 164 Resp: 187098
 Ion Ratio Lower Upper
 164 100
 162 107.5 82.4 123.6
 160 48.9 35.8 53.6

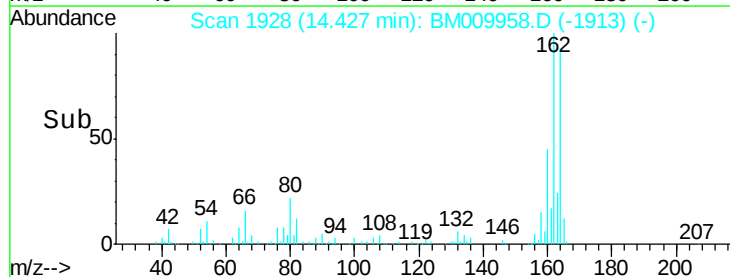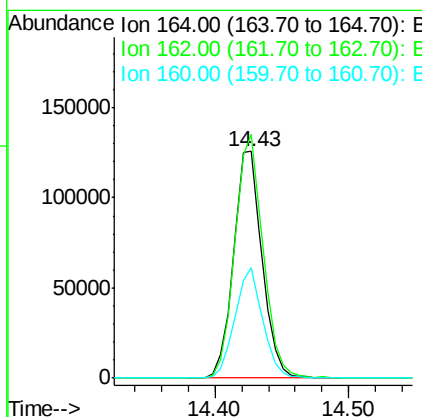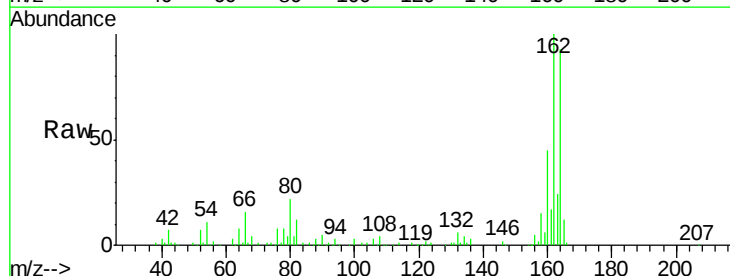

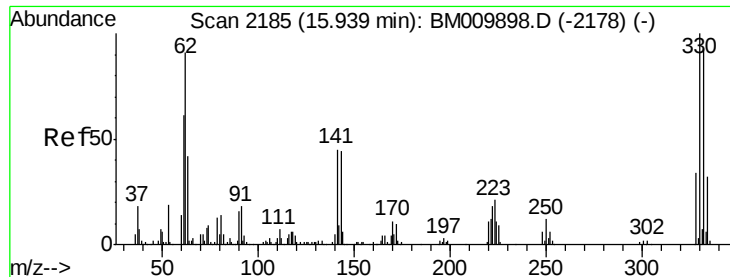

#41

2,4,6-Tribromophenol

Concen: 162.72 ng

RT: 15.93 min Scan# 2183

Delta R.T. -0.01 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39

Instrument :

BNA_M

ClientSampleId :

WC-AOC17-003


Tgt Ion:330 Resp: 415801

Ion Ratio Lower Upper

330 100

332 96.4 0.0 0.0#




141 48.6 0.0 0.0#

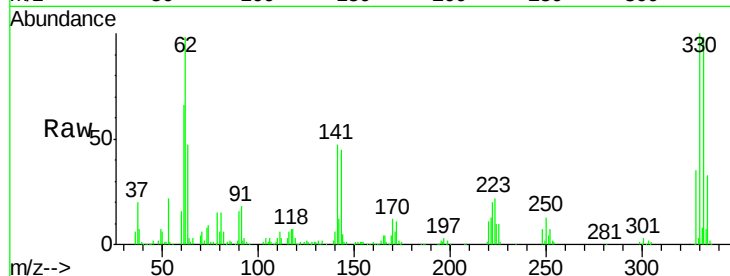

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

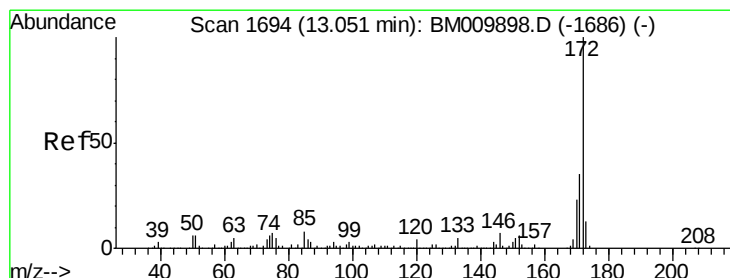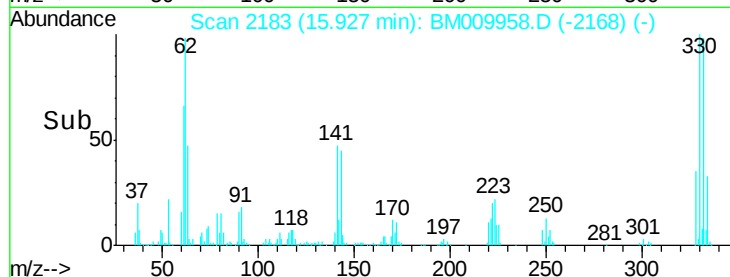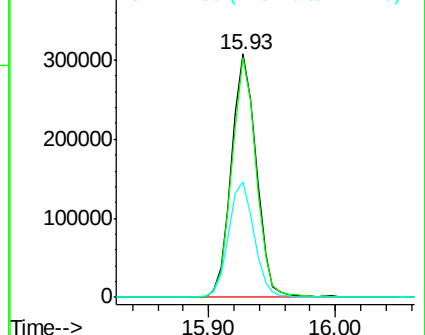

#44

2-Fluorobiphenyl

Concen: 97.50 ng

RT: 13.04 min Scan# 1692

Delta R.T. -0.01 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39


Tgt Ion:172 Resp: 1400054

Ion Ratio Lower Upper

172 100

171 35.7 28.5 42.7



170 23.9 18.8 28.2

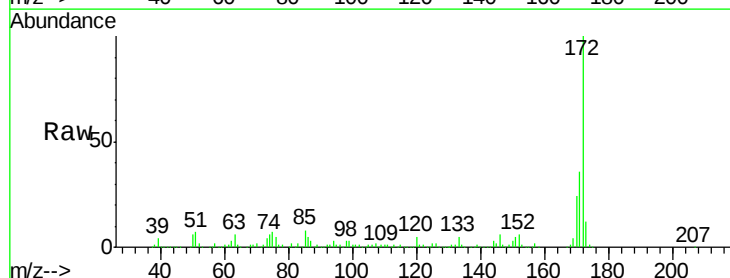


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



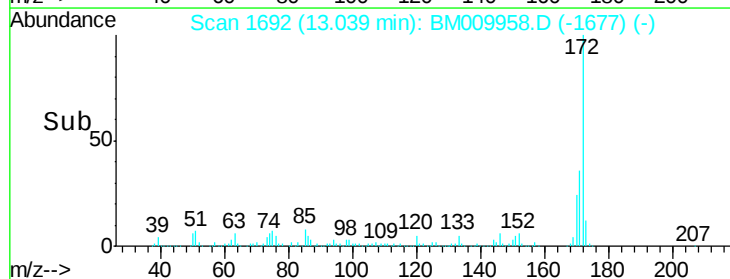
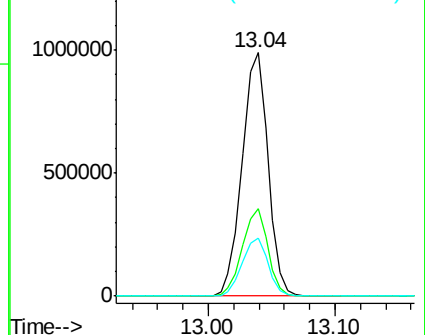


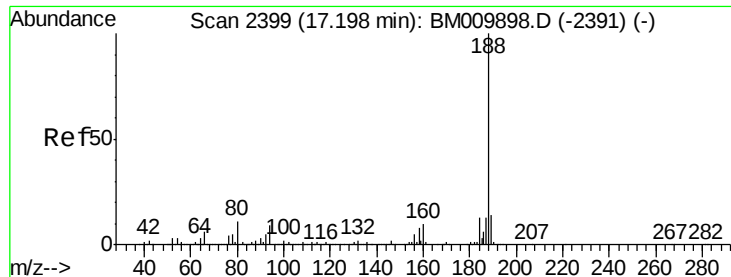

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.18 min Scan# 2396
Delta R.T. -0.02 min
Lab File: BM009958.D
Acq: 07 May 2017 01:39




Instrument :
BNA_M
ClientSampleId :
WC-AOC17-003


Tgt Ion:188 Resp: 463890
Ion Ratio Lower Upper
188 100
94 9.5 8.7 13.1
80 11.1 9.3 13.9

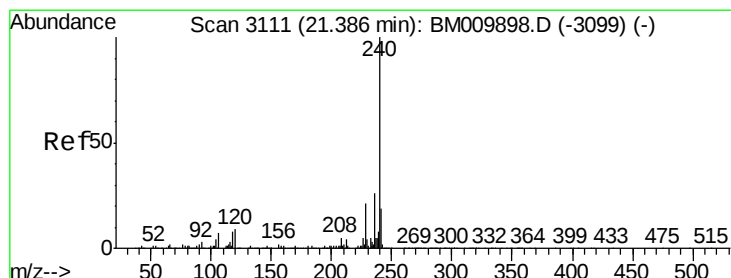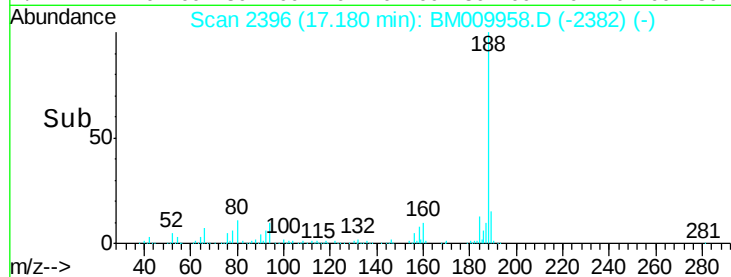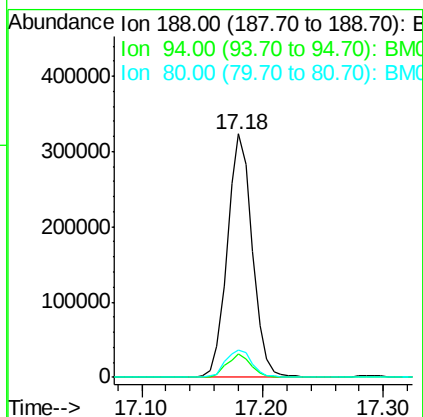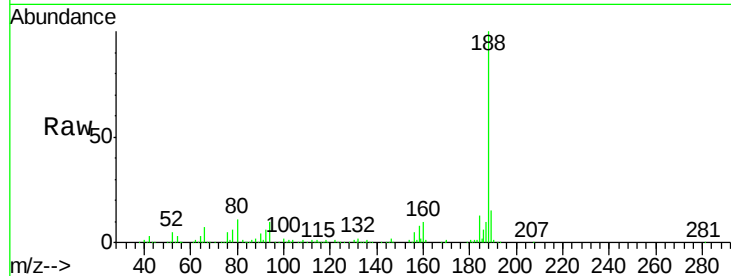

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.37 min Scan# 3108
Delta R.T. -0.02 min
Lab File: BM009958.D
Acq: 07 May 2017 01:39

Tgt Ion:240 Resp: 507913
Ion Ratio Lower Upper
240 100
120 8.2 8.2 12.2
236 25.6 20.0 30.0

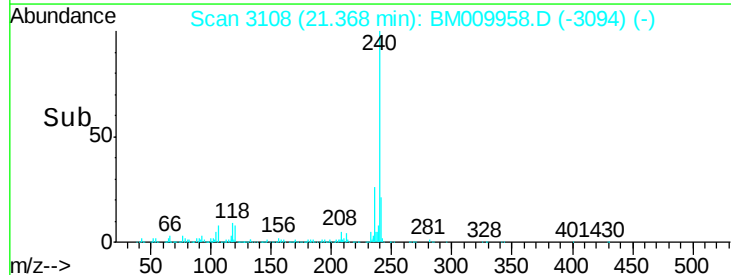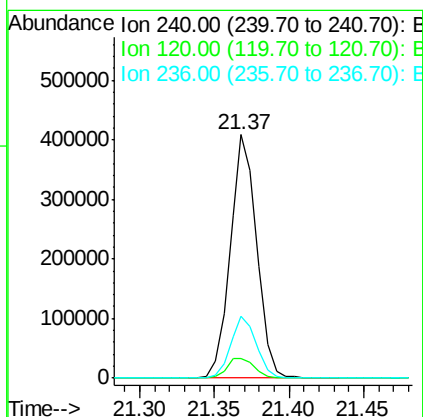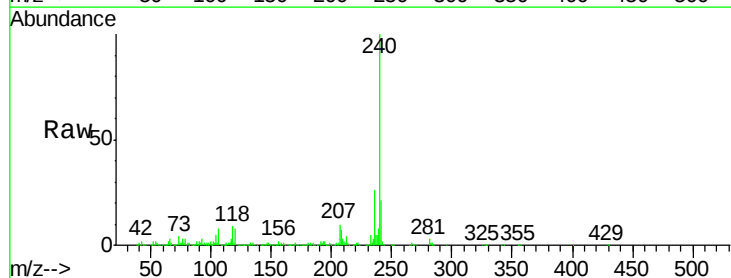

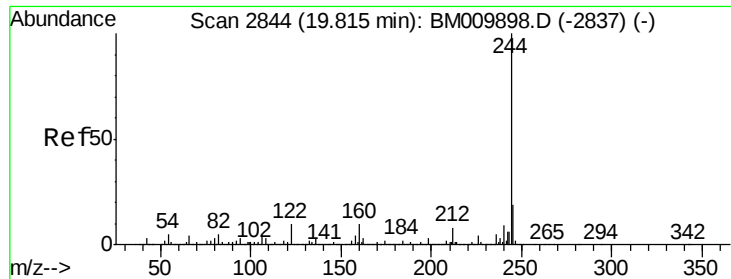

#78

Terphenyl-d14

Concen: 107.78 ng

RT: 19.80 min Scan# 2842

Delta R.T. -0.01 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39

Instrument :

BNA_M

ClientSampleId :

WC-AOC17-003


Tgt Ion:244 Resp: 2668632

Ion Ratio Lower Upper

244 100

212 8.2 4.9 7.3#




122 10.0 6.2 9.4#

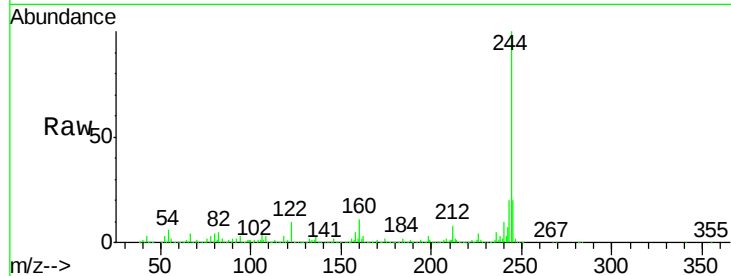

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

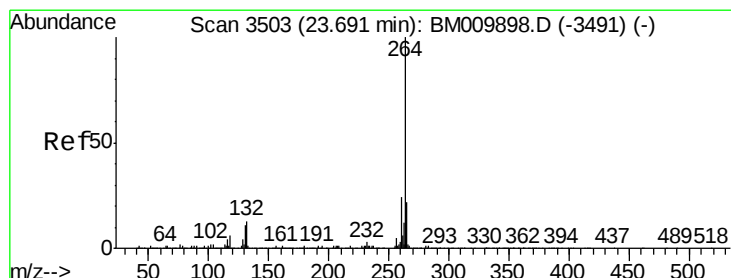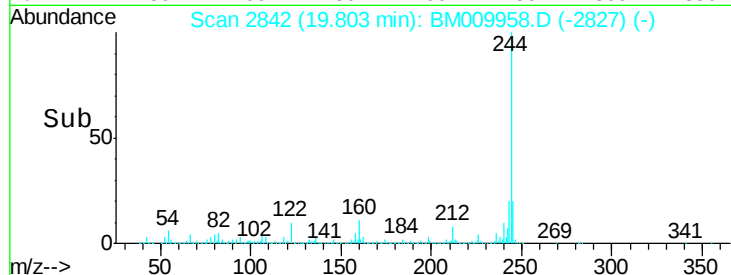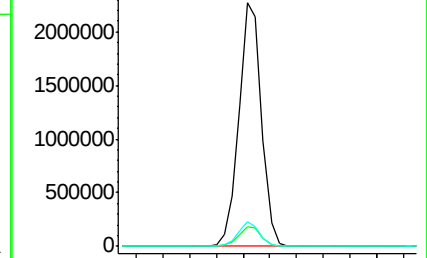

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.67 min Scan# 3499

Delta R.T. -0.02 min

Lab File: BM009958.D

Acq: 07 May 2017 01:39


Tgt Ion:264 Resp: 388583

Ion Ratio Lower Upper

264 100

260 23.1 18.6 27.8

265 20.3 17.3 25.9

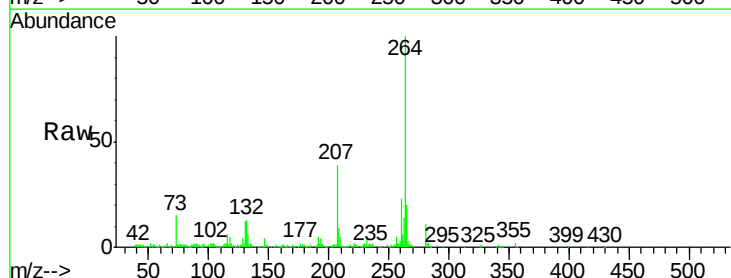

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

