


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050617\
 Data File : BM009931.D
 Acq On : 06 May 2017 08:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 05 14:52:12 2017

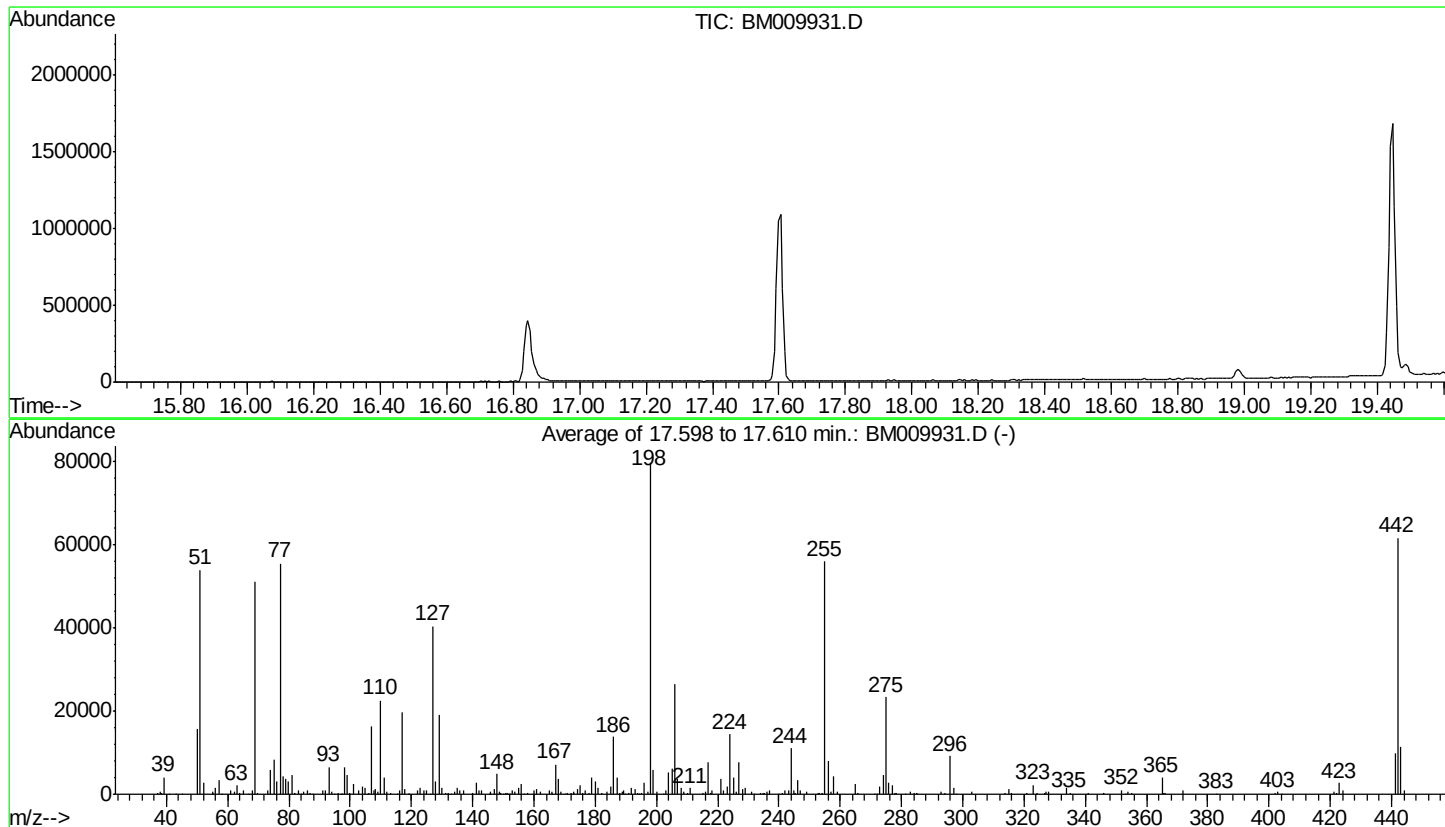

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.7	53906	PASS
68	69	0.00	2	1.8	932	PASS
69	198	0.00	100	64.2	51154	PASS
70	69	0.00	2	0.4	186	PASS
127	198	10	80	50.7	40402	PASS
197	198	0.00	2	1.0	772	PASS
198	198	100	100	100.0	79645	PASS
199	198	5	9	7.4	5876	PASS
275	198	10	60	29.3	23354	PASS
365	198	1	100	4.9	3921	PASS
441	442	0.01	24	16.1	9897	PASS
442	198	50	100	77.3	61605	PASS
443	442	15	24	18.5	11385	PASS