


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050617\
 Data File : BM009949.D
 Acq On : 06 May 2017 20:15
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
 Title : SVOA CALIBRATION
 Last Update : Wed Nov 30 00:32:18 2016

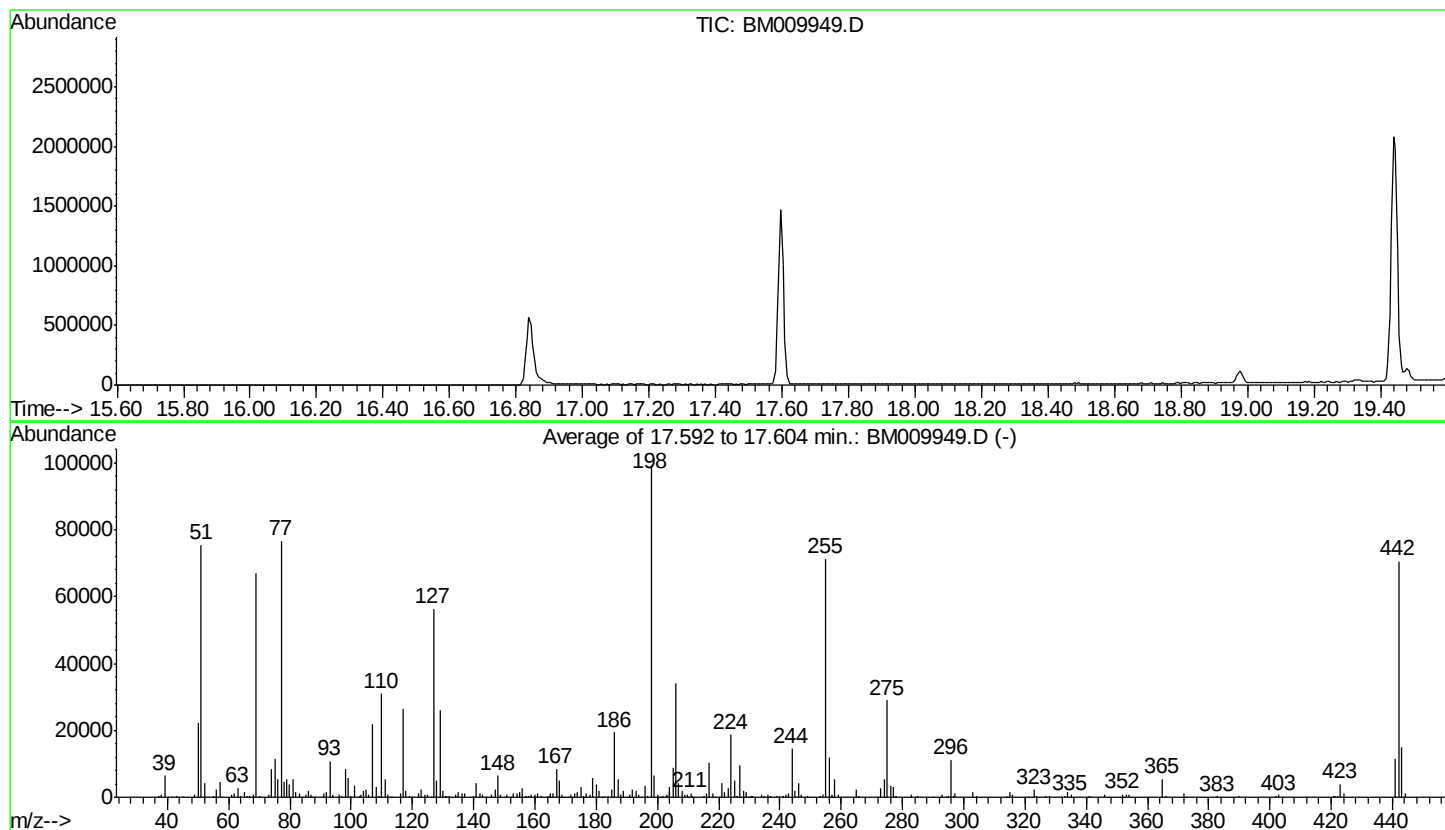

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	76.1	75485	PASS
68	69	0.00	2	1.2	782	PASS
69	198	0.00	100	67.7	67093	PASS
70	69	0.00	2	0.6	407	PASS
127	198	10	80	56.8	56325	PASS
197	198	0.00	2	0.5	499	PASS
198	198	100	100	100.0	99160	PASS
199	198	5	9	6.5	6471	PASS
275	198	10	60	29.3	29034	PASS
365	198	1	100	5.5	5459	PASS
441	443	0.01	100	77.5	11630	PASS
442	198	50	100	71.0	70453	PASS
443	442	15	24	21.3	15016	PASS