

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
 Data File : BM050122.D
 Acq On : 06 May 2025 16:38
 Operator : RC/JU
 Sample : Q1951-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MH-KK

Quant Time: May 06 18:27:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	296732	20.000	ng	-0.02
21) Naphthalene-d8	10.539	136	1055049	20.000	ng	-0.02
39) Acenaphthene-d10	14.392	164	701841	20.000	ng	-0.02
64) Phenanthrene-d10	17.145	188	1365037	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	1229890	20.000	ng	-0.01
86) Perylene-d12	24.380	264	1257507	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	1917626	113.163	ng	-0.02
7) Phenol-d6	6.934	99	2202724	103.421	ng	-0.02
23) Nitrobenzene-d5	8.904	82	1629890	76.125	ng	-0.02
42) 2,4,6-Tribromophenol	15.892	330	1435211	138.298	ng	-0.01
45) 2-Fluorobiphenyl	13.010	172	4373565	73.718	ng	-0.02
79) Terphenyl-d14	19.768	244	7439318	89.506	ng	-0.01
Target Compounds						Qvalue
50) Dimethylphthalate	13.863	163	108174	2.109	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050122.D
Acq On : 06 May 2025 16:38
Operator : RC/JU
Sample : Q1951-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MH-KK

Quant Time: May 06 18:27:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

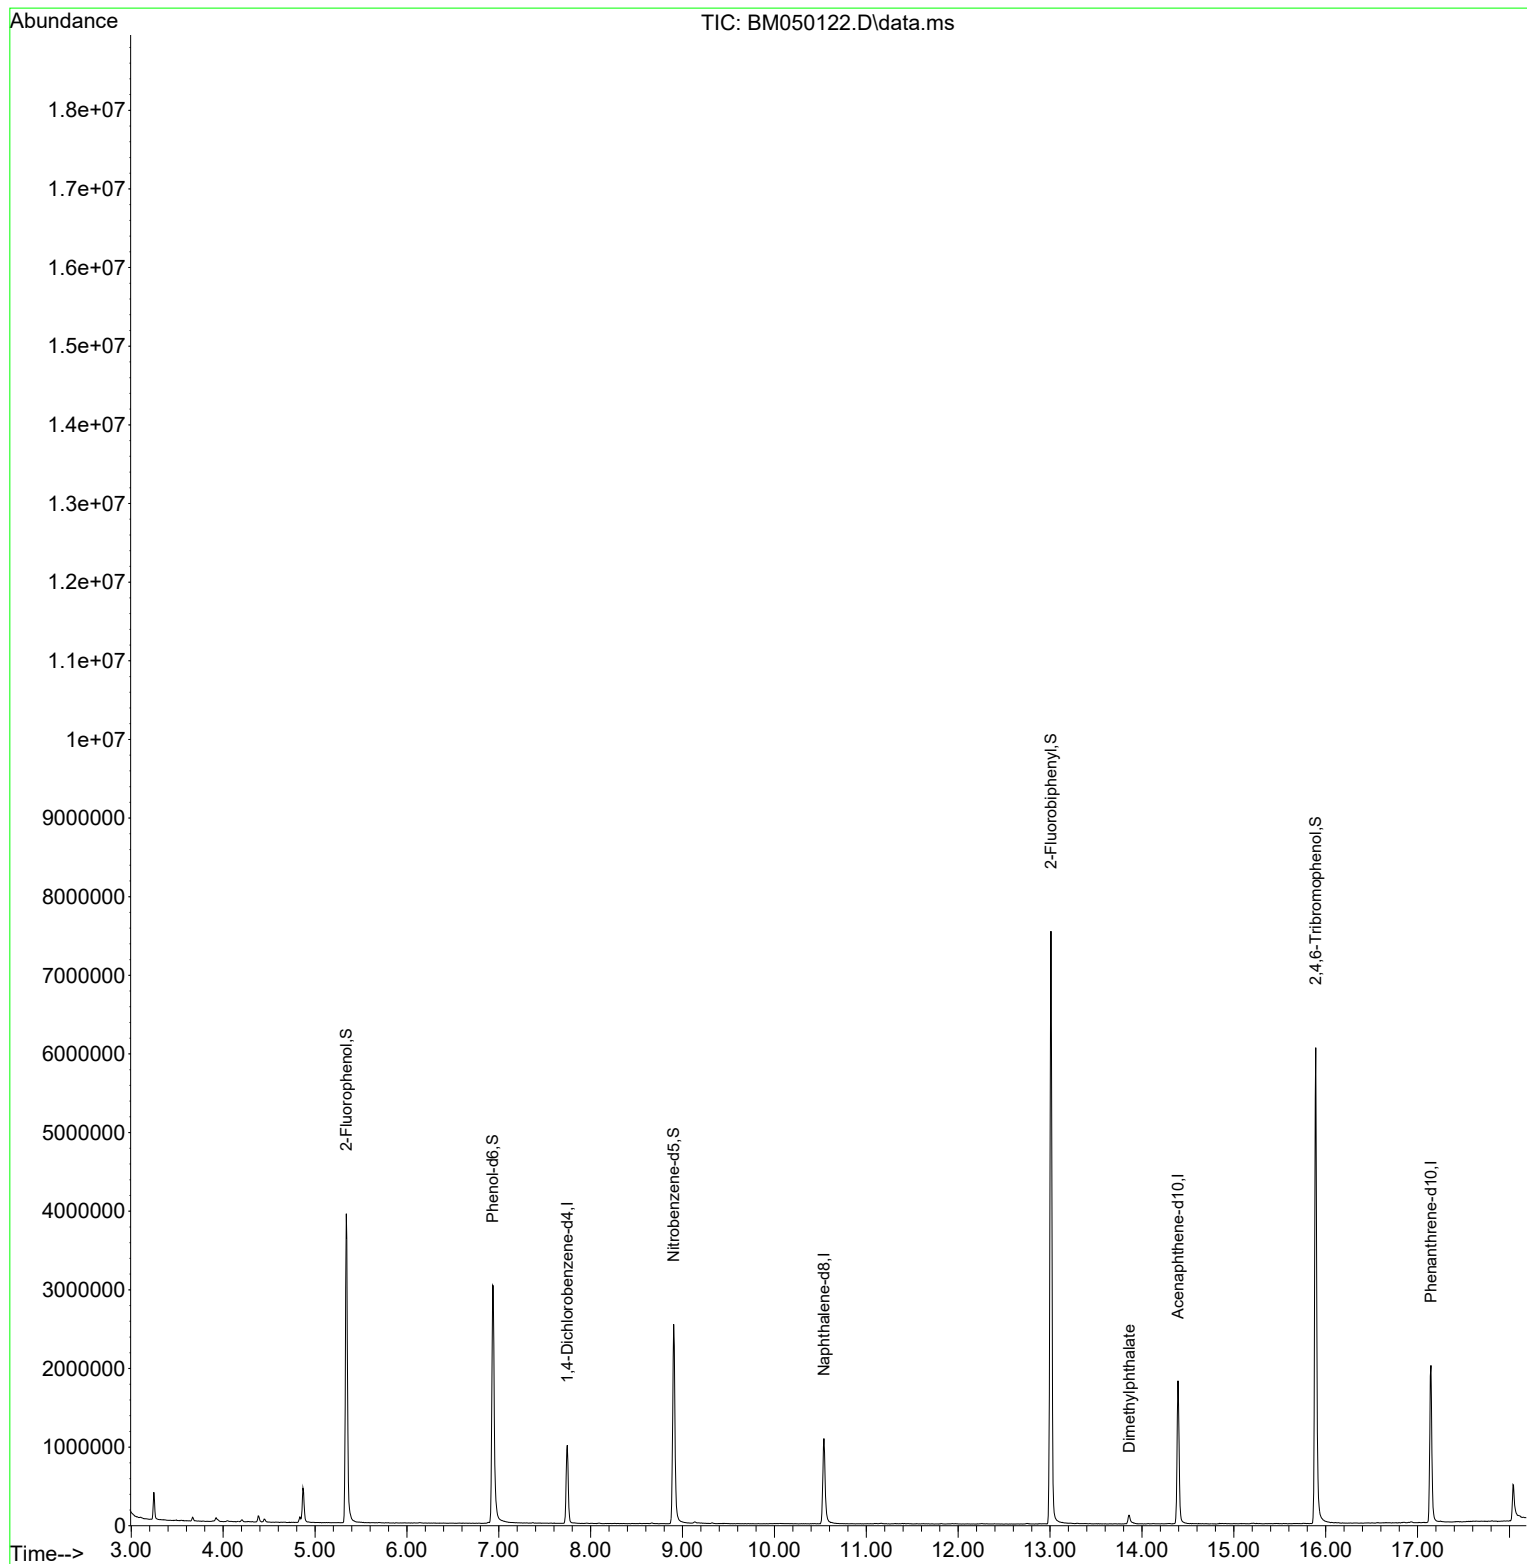

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050122.D
Acq On : 06 May 2025 16:38
Operator : RC/JU
Sample : Q1951-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MH-KK

Quant Time: May 06 18:27:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

