

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
 Data File : BM050119.D
 Acq On : 06 May 2025 14:41
 Operator : RC/JU
 Sample : Q1937-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 LARGE-PILE-E

Quant Time: May 06 15:20:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	305398	20.000	ng	-0.02
21) Naphthalene-d8	10.539	136	1098426	20.000	ng	-0.02
39) Acenaphthene-d10	14.392	164	735430	20.000	ng	-0.02
64) Phenanthrene-d10	17.139	188	1445019	20.000	ng	-0.02
76) Chrysene-d12	21.386	240	1331447	20.000	ng	-0.01
86) Perylene-d12	24.374	264	1358259	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	1576364	90.385	ng	-0.02
7) Phenol-d6	6.934	99	1956475	89.253	ng	-0.02
23) Nitrobenzene-d5	8.904	82	1181880	53.020	ng	-0.02
42) 2,4,6-Tribromophenol	15.892	330	1023324	94.105	ng	-0.01
45) 2-Fluorobiphenyl	13.010	172	3226992	51.908	ng	-0.02
79) Terphenyl-d14	19.768	244	5314478	59.064	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050119.D
Acq On : 06 May 2025 14:41
Operator : RC/JU
Sample : Q1937-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Quant Time: May 06 15:20:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

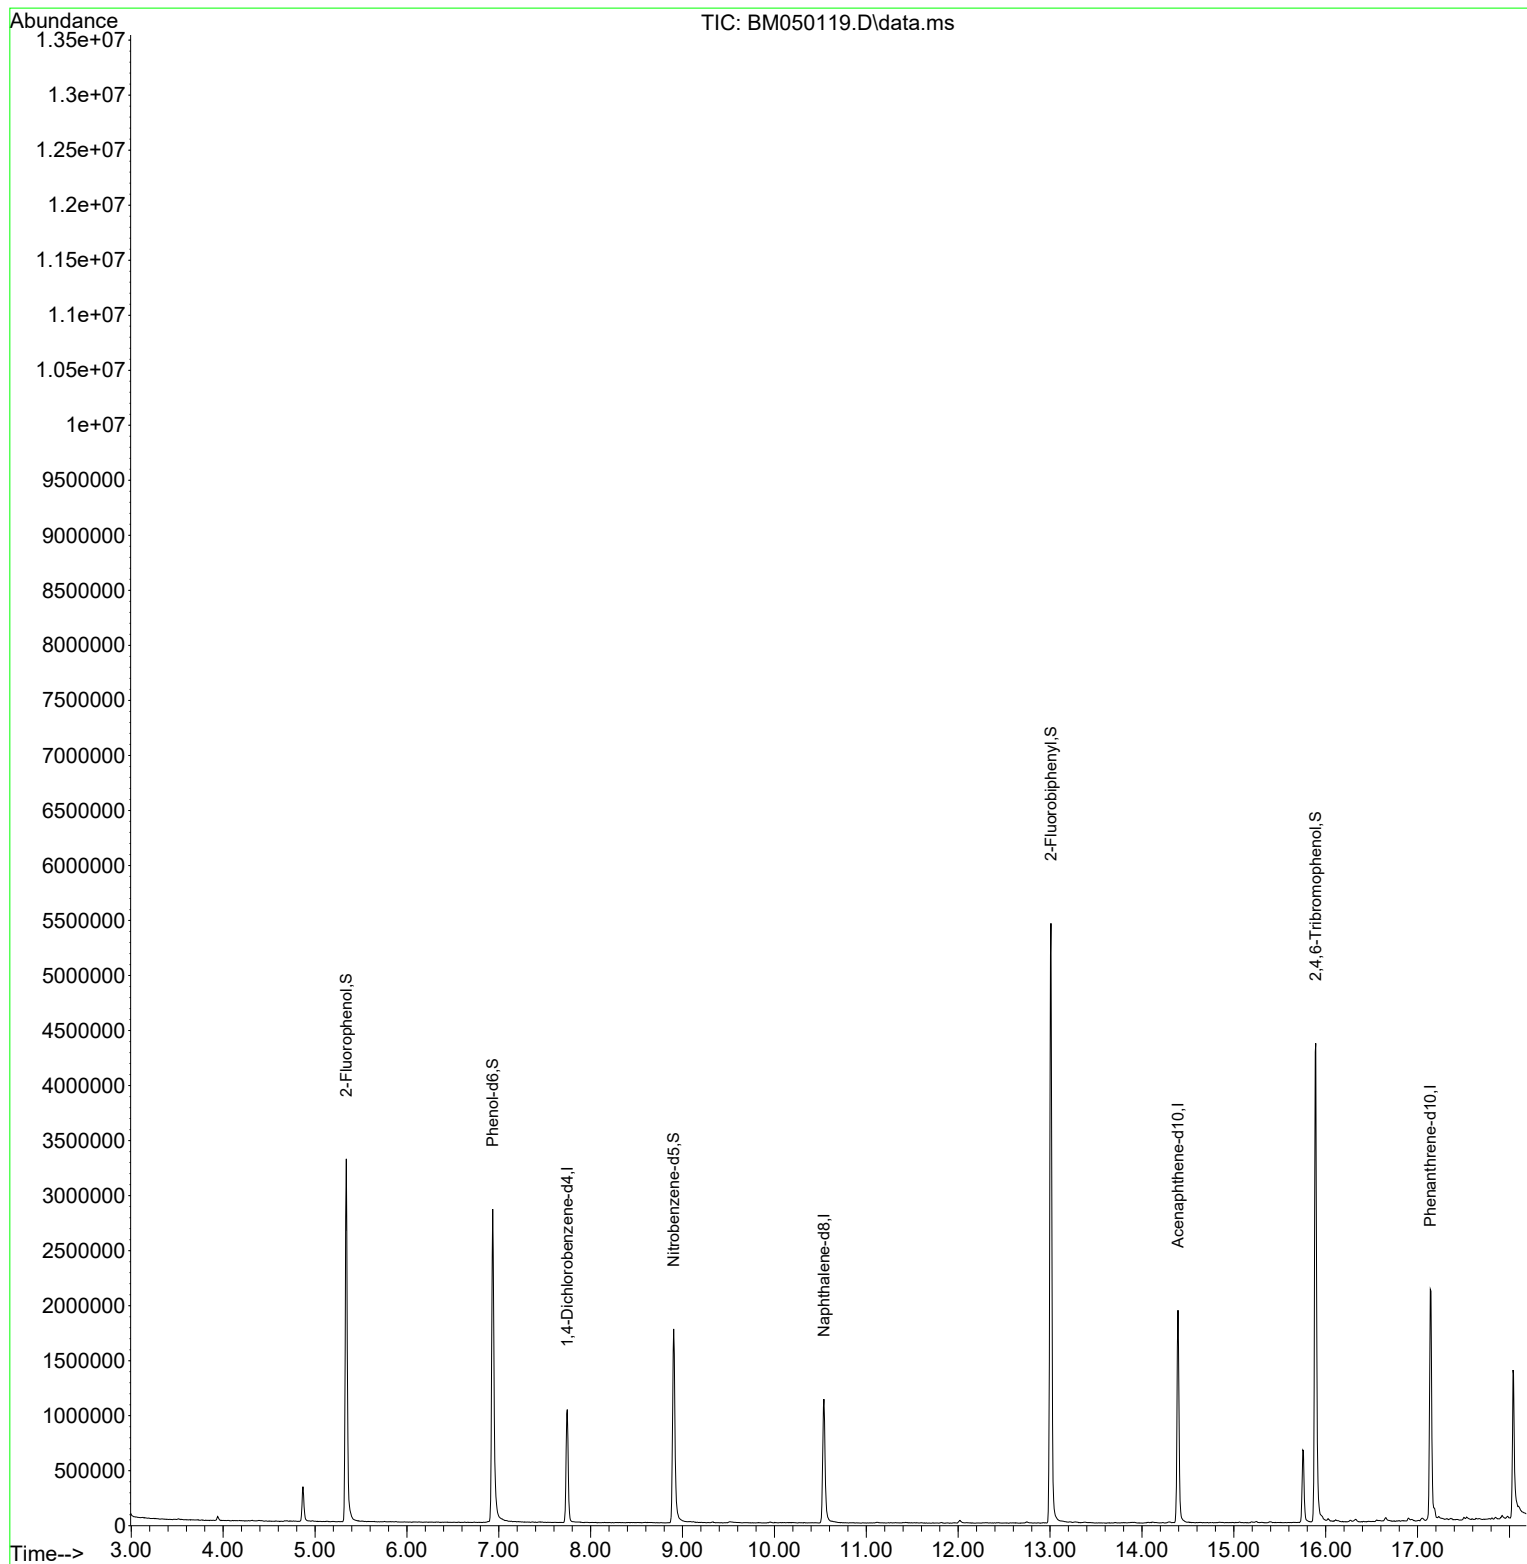


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050119.D
Acq On : 06 May 2025 14:41
Operator : RC/JU
Sample : Q1937-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E

Quant Time: May 06 15:20:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration




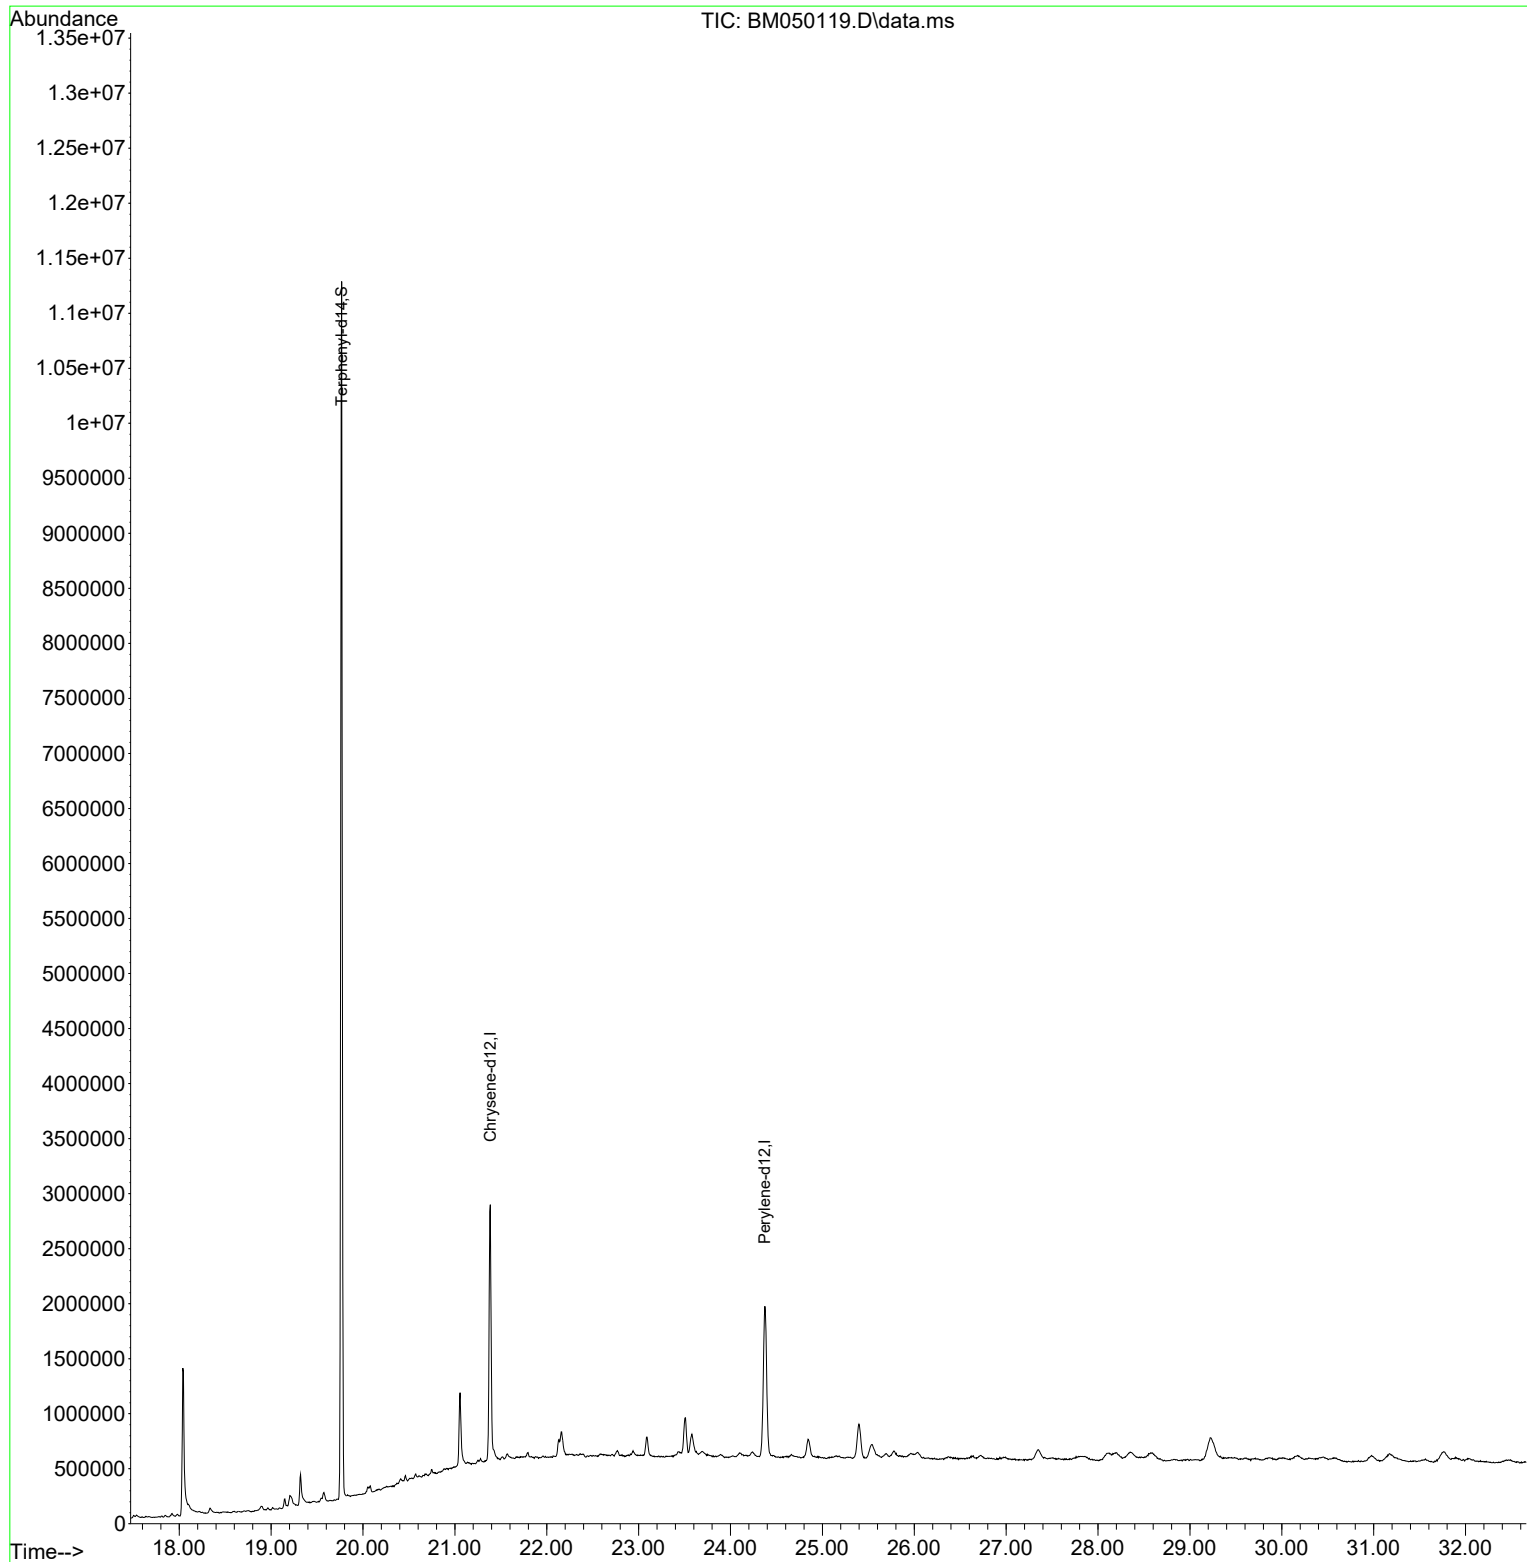


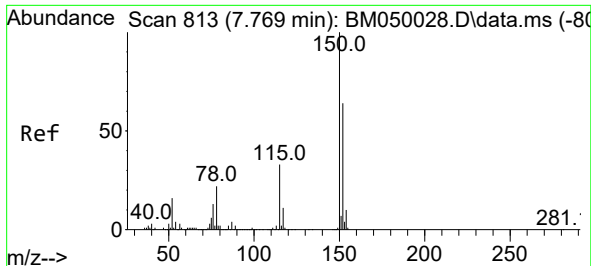

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.745 min Scan# 809
Delta R.T. -0.024 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41




Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Tgt Ion:152 Resp: 305398
Ion Ratio Lower Upper
152 100
150 157.9 124.1 186.1
115 53.9 41.2 61.8

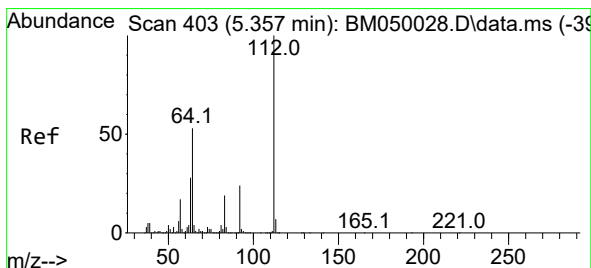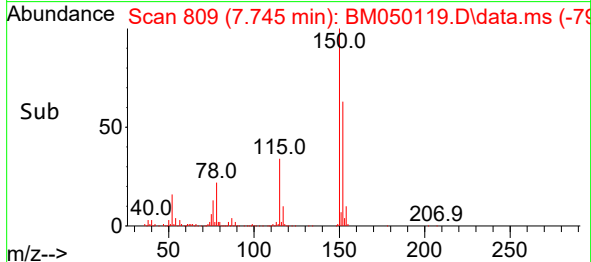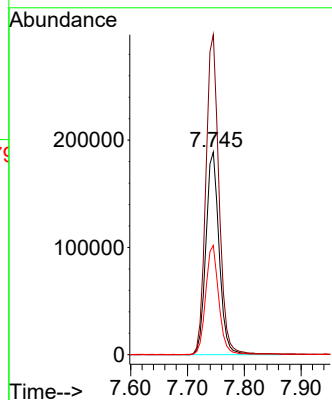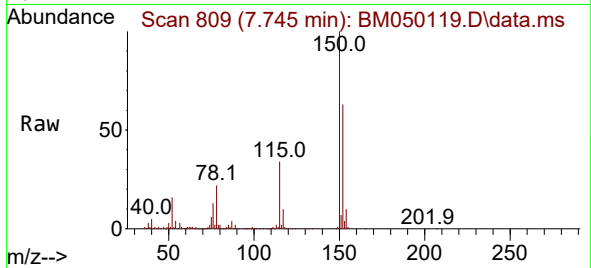

#5
2-Fluorophenol
Concen: 90.385 ng
RT: 5.340 min Scan# 400
Delta R.T. -0.018 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41

Tgt Ion:112 Resp: 1576364
Ion Ratio Lower Upper
112 100
64 52.6 42.6 64.0
63 27.2 22.2 33.4


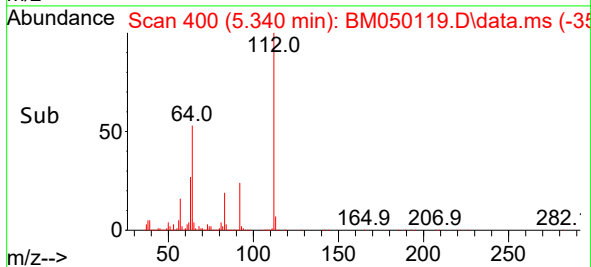
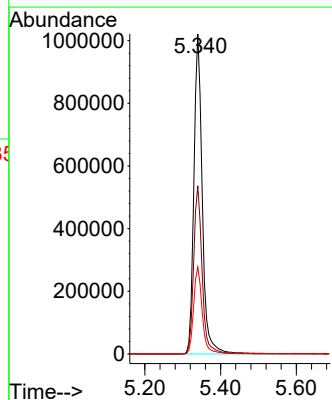
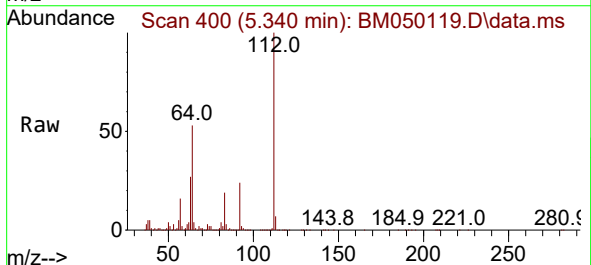


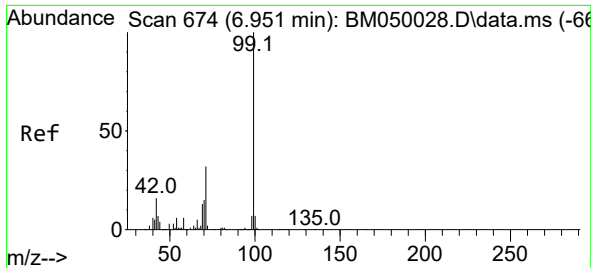

#7
Phenol-d6
Concen: 89.253 ng
RT: 6.934 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41




Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Tgt Ion: 99 Resp: 1956475
Ion Ratio Lower Upper
99 100
42 15.5 13.0 19.4
71 31.6 25.6 38.4

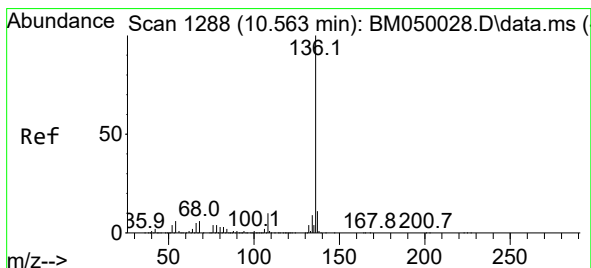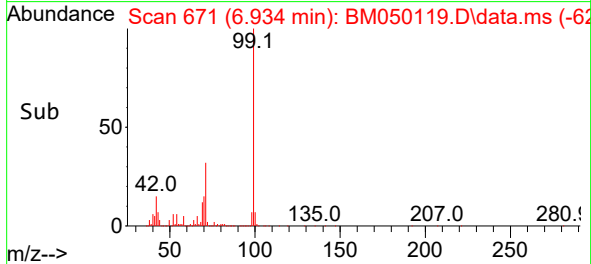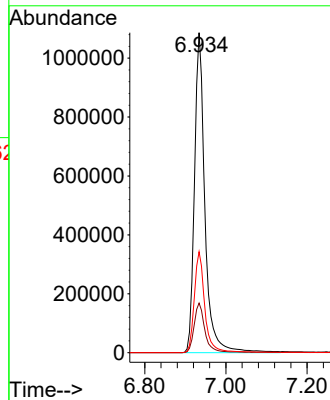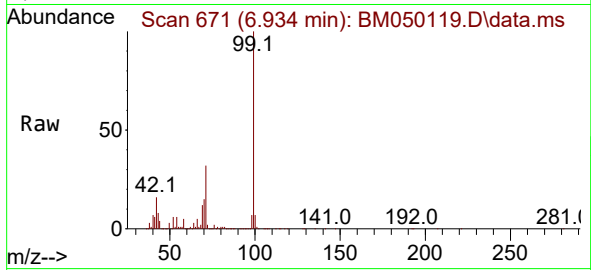

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.539 min Scan# 1284
Delta R.T. -0.024 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41

Tgt Ion: 136 Resp: 1098426
Ion Ratio Lower Upper
136 100
137 11.1 8.9 13.3
54 6.6 5.1 7.7
68 5.6 4.4 6.6


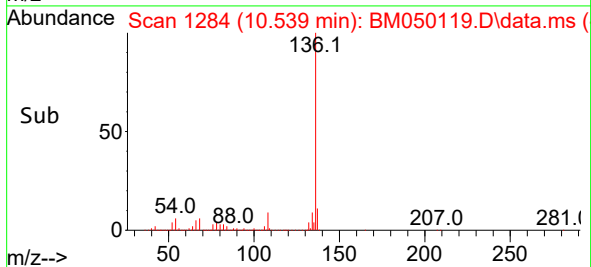
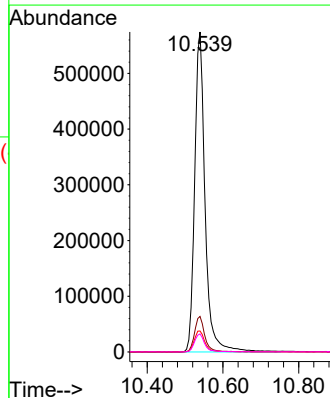
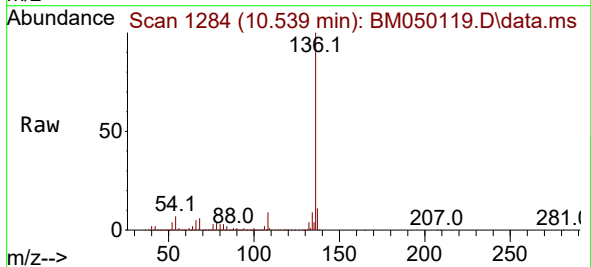


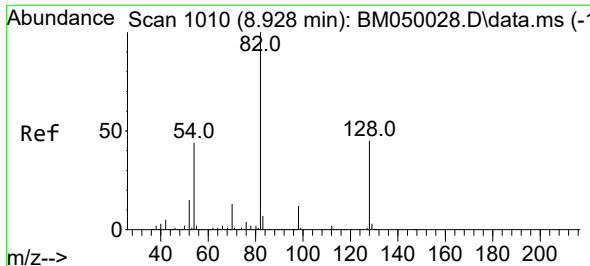

#23
Nitrobenzene-d5
Concen: 53.020 ng
RT: 8.904 min Scan# 1006
Delta R.T. -0.024 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41




Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Tgt Ion: 82 Resp: 1181880
Ion Ratio Lower Upper
82 100
128 45.5 35.7 53.5
54 44.6 35.4 53.2

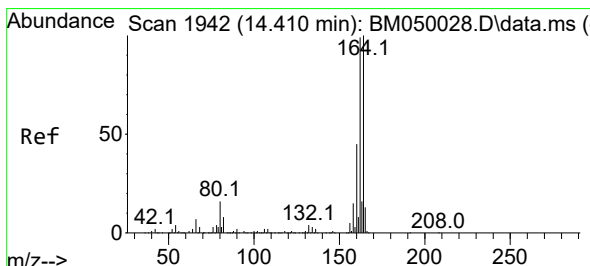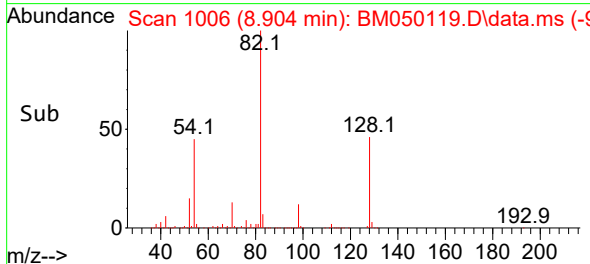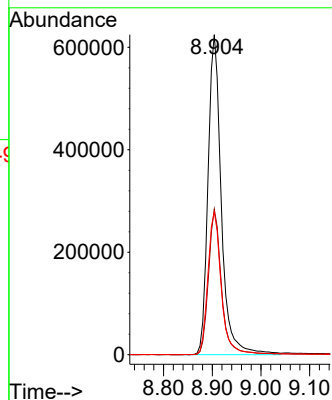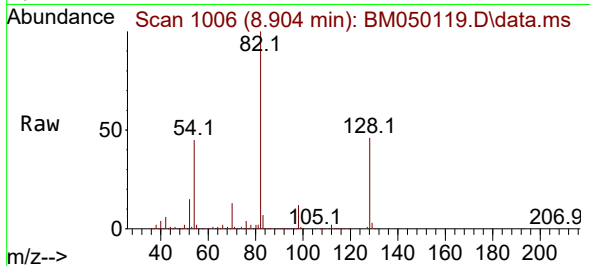

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.392 min Scan# 1939
Delta R.T. -0.018 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41

Tgt Ion: 164 Resp: 735430
Ion Ratio Lower Upper
164 100
162 100.0 79.4 119.0
160 44.2 36.2 54.4


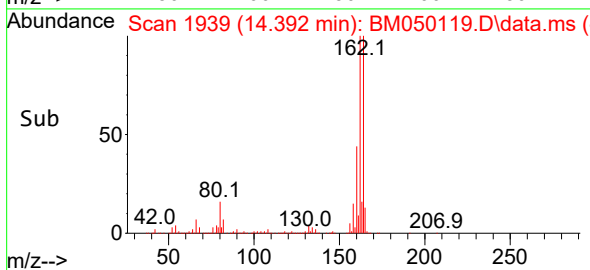
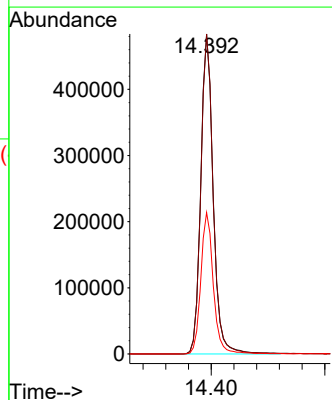
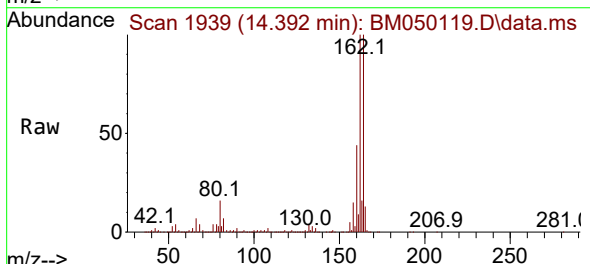


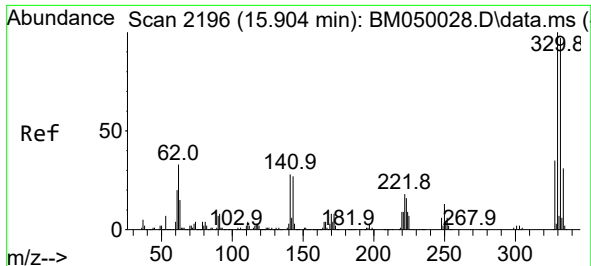

#42
2,4,6-Tribromophenol
Concen: 94.105 ng
RT: 15.892 min Scan# 2194
Delta R.T. -0.012 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41




Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Tgt Ion:330 Resp: 1023324
Ion Ratio Lower Upper
330 100
332 96.5 77.3 115.9
141 27.2 22.5 33.7

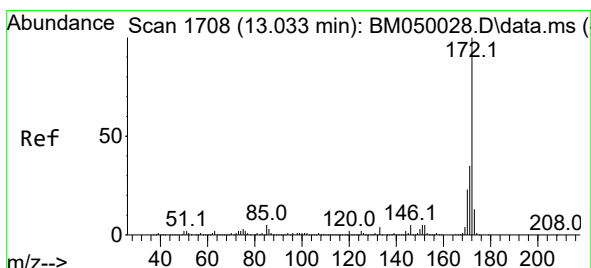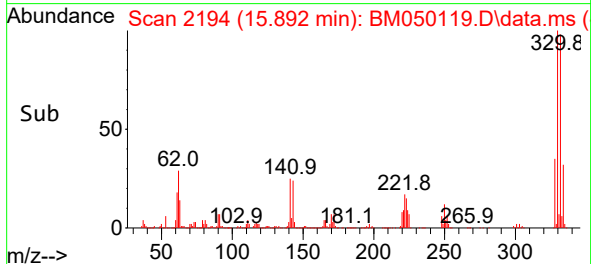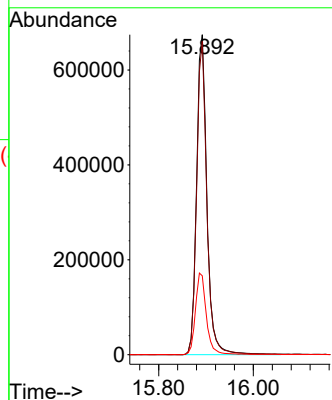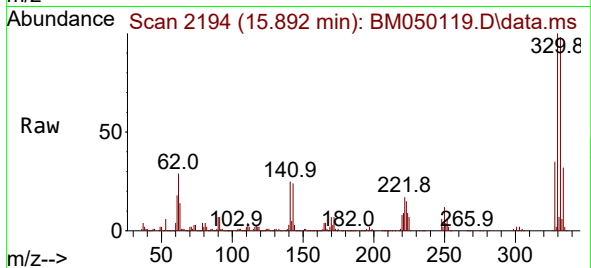

#45
2-Fluorobiphenyl
Concen: 51.908 ng
RT: 13.010 min Scan# 1704
Delta R.T. -0.024 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41

Tgt Ion:172 Resp: 3226992
Ion Ratio Lower Upper
172 100
171 34.6 27.8 41.6
170 23.2 18.6 28.0


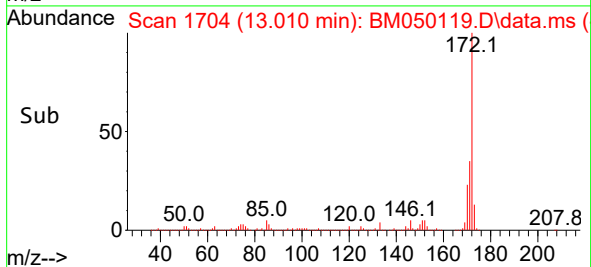
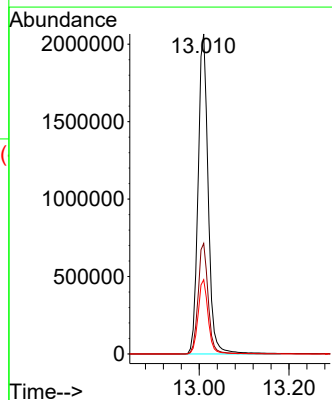
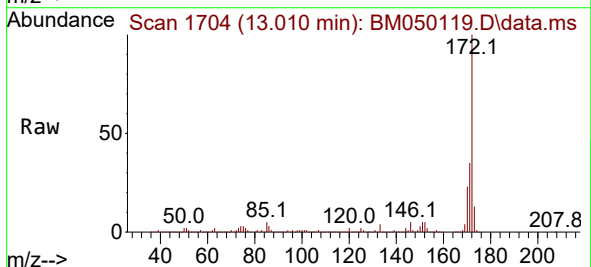


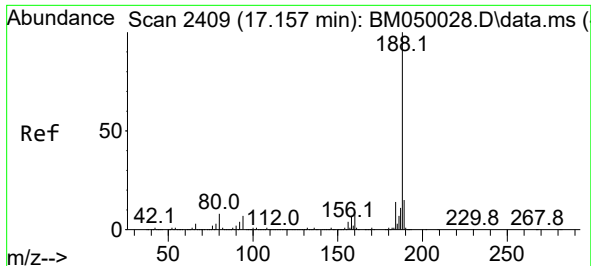

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.139 min Scan# 24
Delta R.T. -0.018 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41




Instrument :
BNA_M
ClientSampleId :
LARGE-PILE-E


Tgt Ion:188 Resp: 1445019
Ion Ratio Lower Upper
188 100
94 7.4 5.7 8.5
80 8.1 6.2 9.4

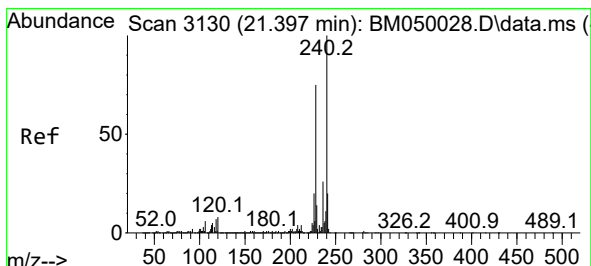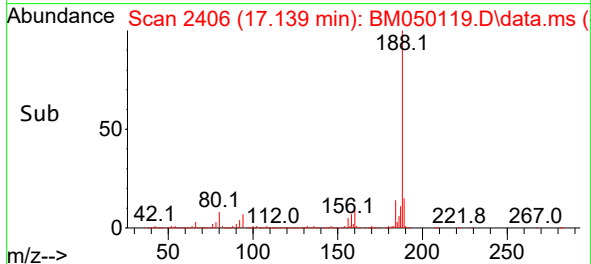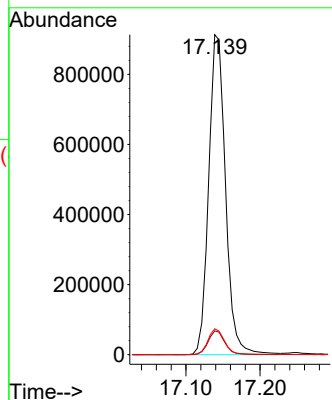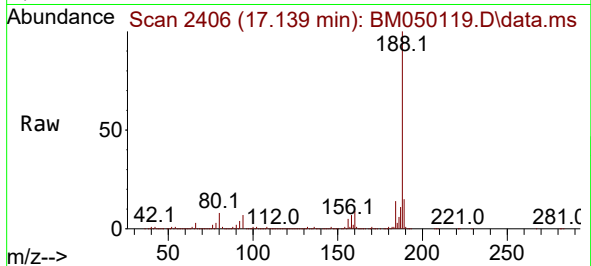

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.386 min Scan# 3128
Delta R.T. -0.011 min
Lab File: BM050119.D
Acq: 06 May 2025 14:41

Tgt Ion:240 Resp: 1331447
Ion Ratio Lower Upper
240 100
120 8.5 6.5 9.7
236 26.0 20.9 31.3

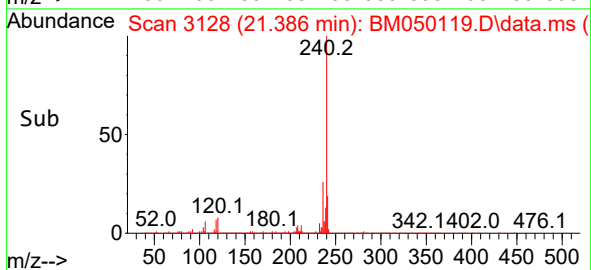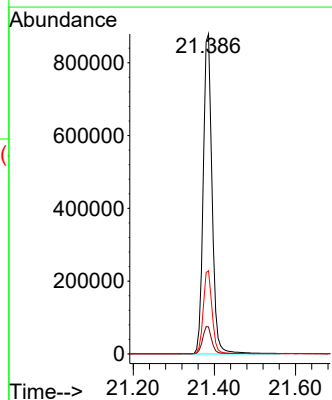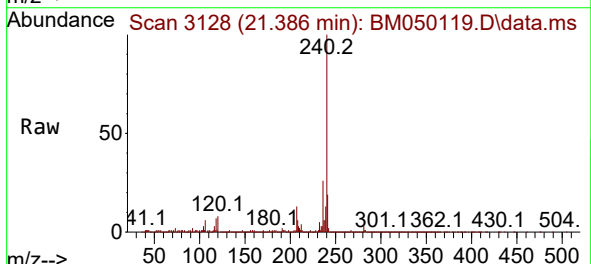

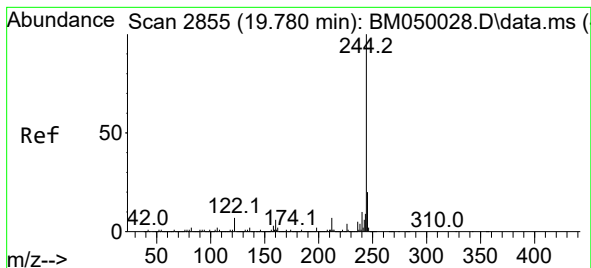

#79

Terphenyl-d14

Concen: 59.064 ng

RT: 19.768 min Scan# 2

Delta R.T. -0.012 min

Lab File: BM050119.D

Acq: 06 May 2025 14:41

Instrument :

BNA_M

ClientSampleId :

LARGE-PILE-E





Tgt Ion:244 Resp: 5314478

Ion Ratio Lower Upper

244 100

212 6.7 5.6 8.4

122 6.5 5.6 8.4

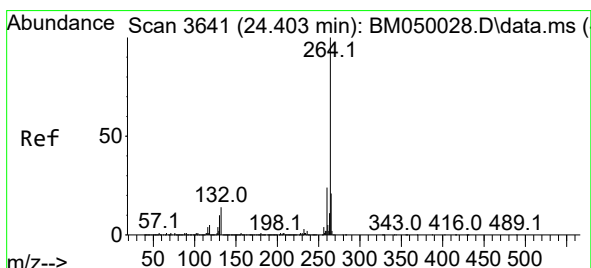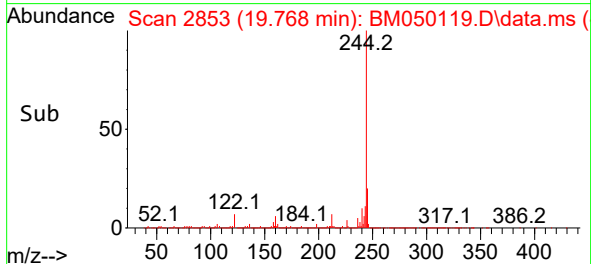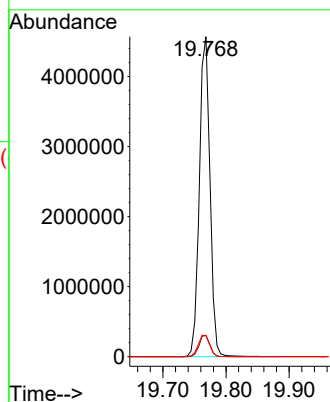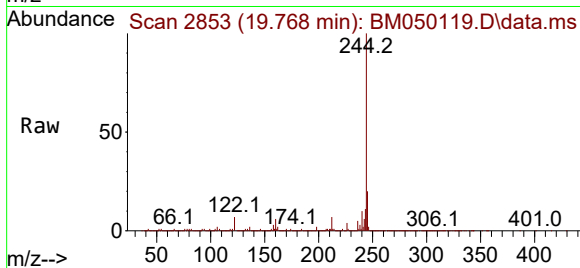

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.374 min Scan# 3636

Delta R.T. -0.029 min

Lab File: BM050119.D

Acq: 06 May 2025 14:41

Tgt Ion:264 Resp: 1358259

Ion Ratio Lower Upper

264 100

260 24.1 18.8 28.2

265 21.8 17.0 25.4

