


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050111.D
Acq On : 06 May 2025 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

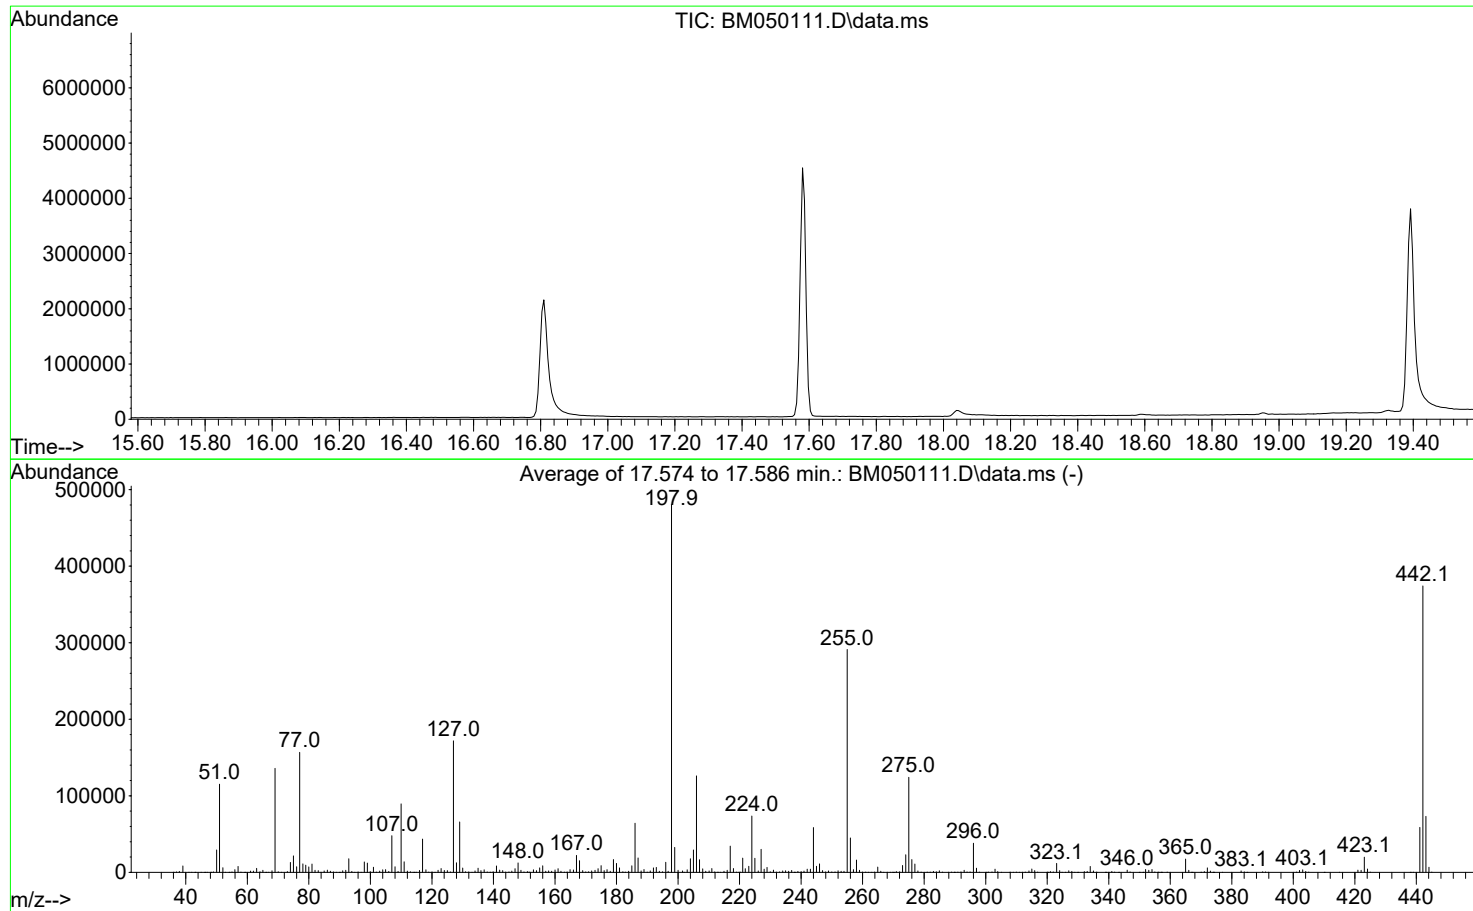

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	115234	PASS
68	69	0.00	2	1.5	2089	PASS
69	198	0.00	100	28.3	135803	PASS
70	69	0.00	2	0.6	795	PASS
127	198	10	80	35.7	171797	PASS
197	198	0.00	2	0.3	1392	PASS
198	198	100	100	100.0	480576	PASS
199	198	5	9	6.8	32581	PASS
275	198	10	60	25.9	124248	PASS
365	198	1	100	3.6	17315	PASS
441	198	0.01	100	12.2	58832	PASS
442	442	50	100	100.0	374165	PASS
443	442	15	24	19.6	73187	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/6/2025	BNA_M	<u>BM050111.D</u>
Compound Name	Response	Retention Time
DDT	1573453	20.621
DDD	31388	20.186
DDE	2518	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33906	1607359	2.11

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050111.D
Acq On : 06 May 2025 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 06 11:38:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

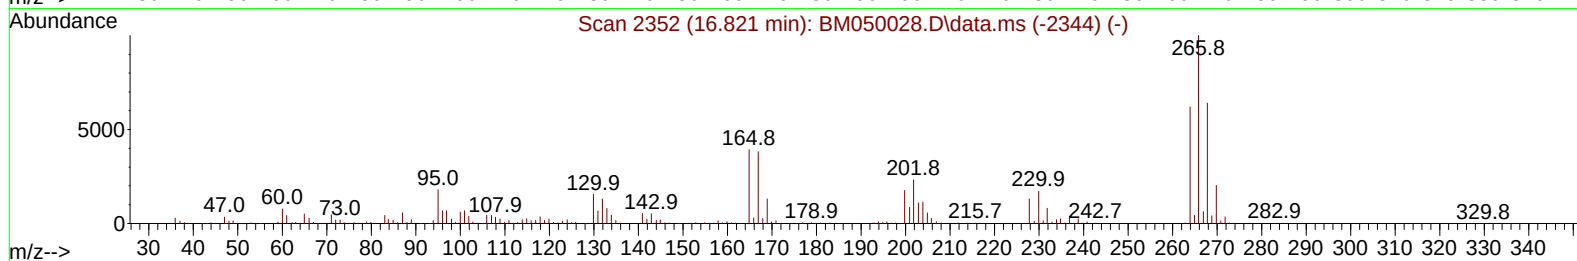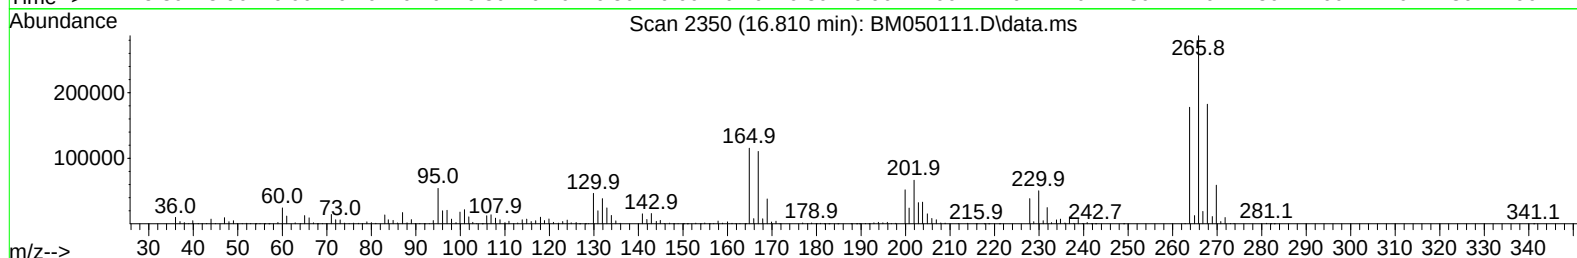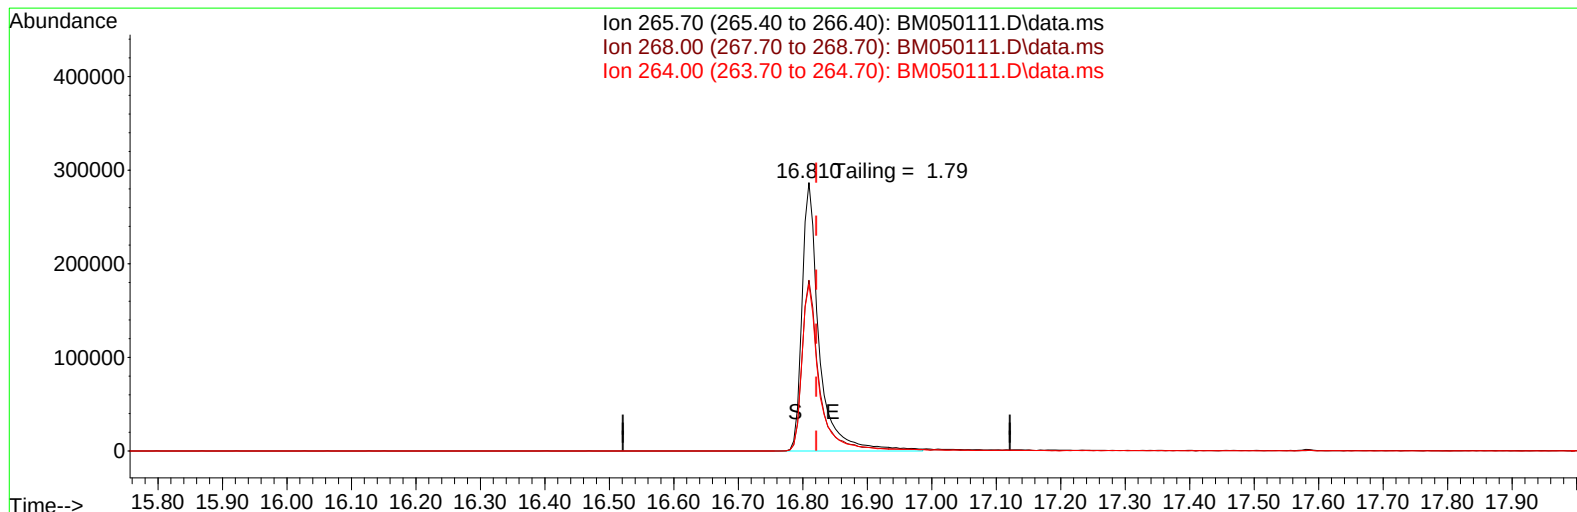

TIC: BM050111.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.012) 0.00 ng m




response 531699

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.59
264.00	62.00	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050625\
Data File : BM050111.D
Acq On : 06 May 2025 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 06 11:38:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

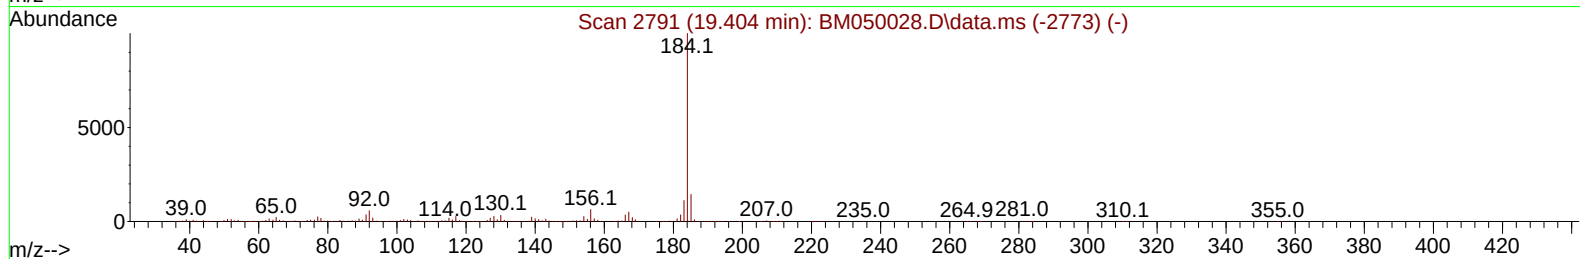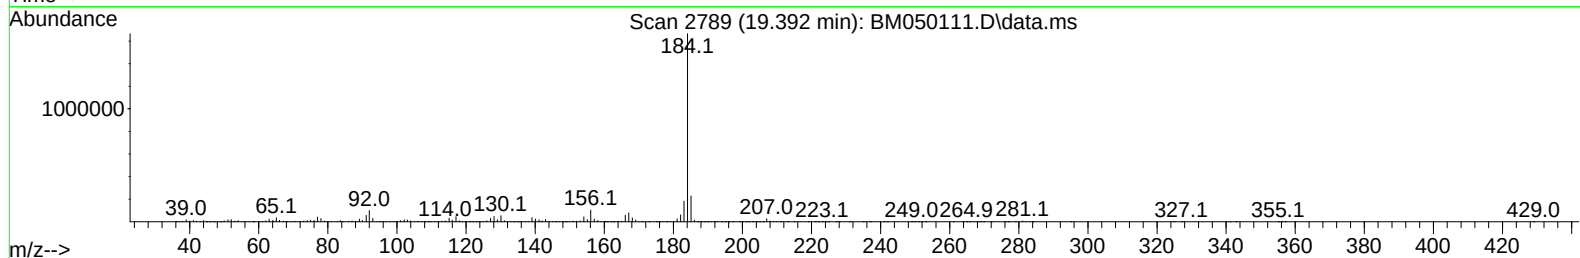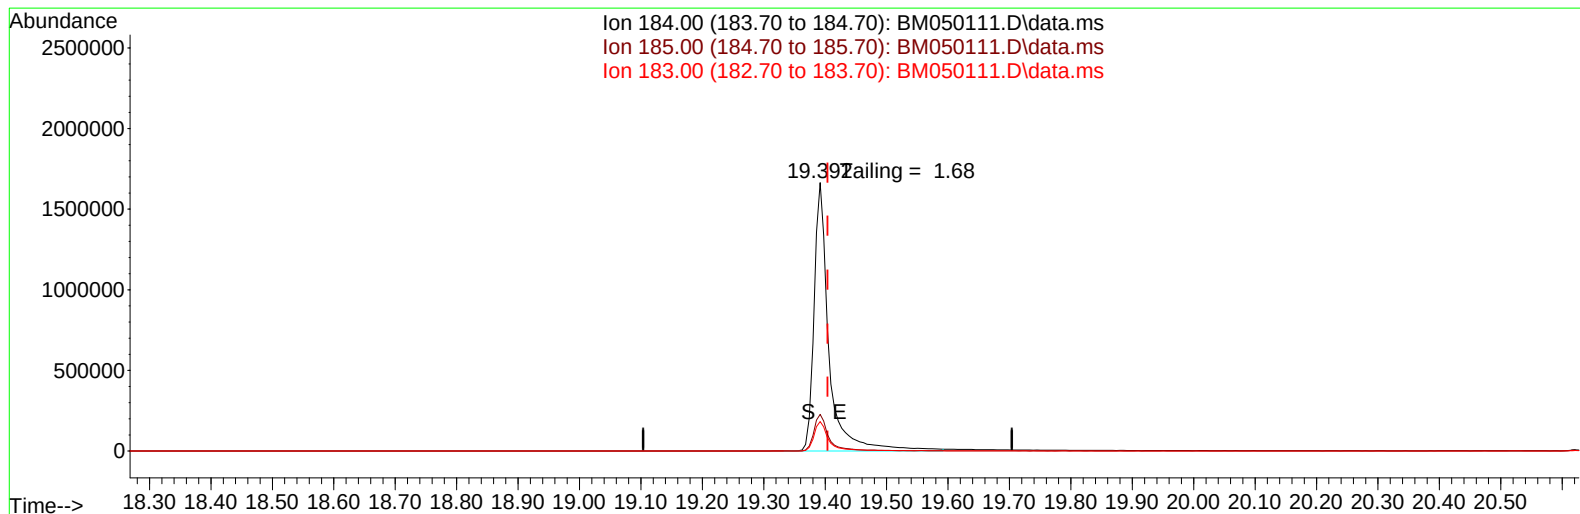

TIC: BM050111.D\data.ms

(77) Benzidine**19.392min (-0.012) 37075.87 ng****response 2852535**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.70
183.00	11.10	11.01
0.00	0.00	0.00