

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
 Data File : BM005337.D
 Acq On : 08 May 2016 08:30
 Operator : UM/SJ
 Sample : H2772-08
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A9

Quant Time: May 09 04:12:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 07 07:05:19 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	81927	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	394626	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	259009	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	624787	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	714417	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	615752	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	4576	2.63	ng/uL	0.00
5) Phenol-d5	6.94	99	96821	13.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	63127	14.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	79803	14.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	59576	9.70	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	41082	14.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	47322	14.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	86872	14.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	105527	14.79	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	351687	16.94	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	400234	16.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	43537	11.49	ng/ul	0.00
57) Fluorene-d10	15.40	176	306460	17.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	46730	13.30	ng/ul	0.00
70) Anthracene-d10	17.26	188	524460	18.99	ng/ul	0.00
76) Pyrene-d10	19.56	212	675376	20.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	576507	21.15	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	72890	3.51	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005337.D
Acq On : 08 May 2016 08:30
Operator : UM/SJ
Sample : H2772-08
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A9

Quant Time: May 09 04:12:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 07 07:05:19 2016
Response via : Initial Calibration

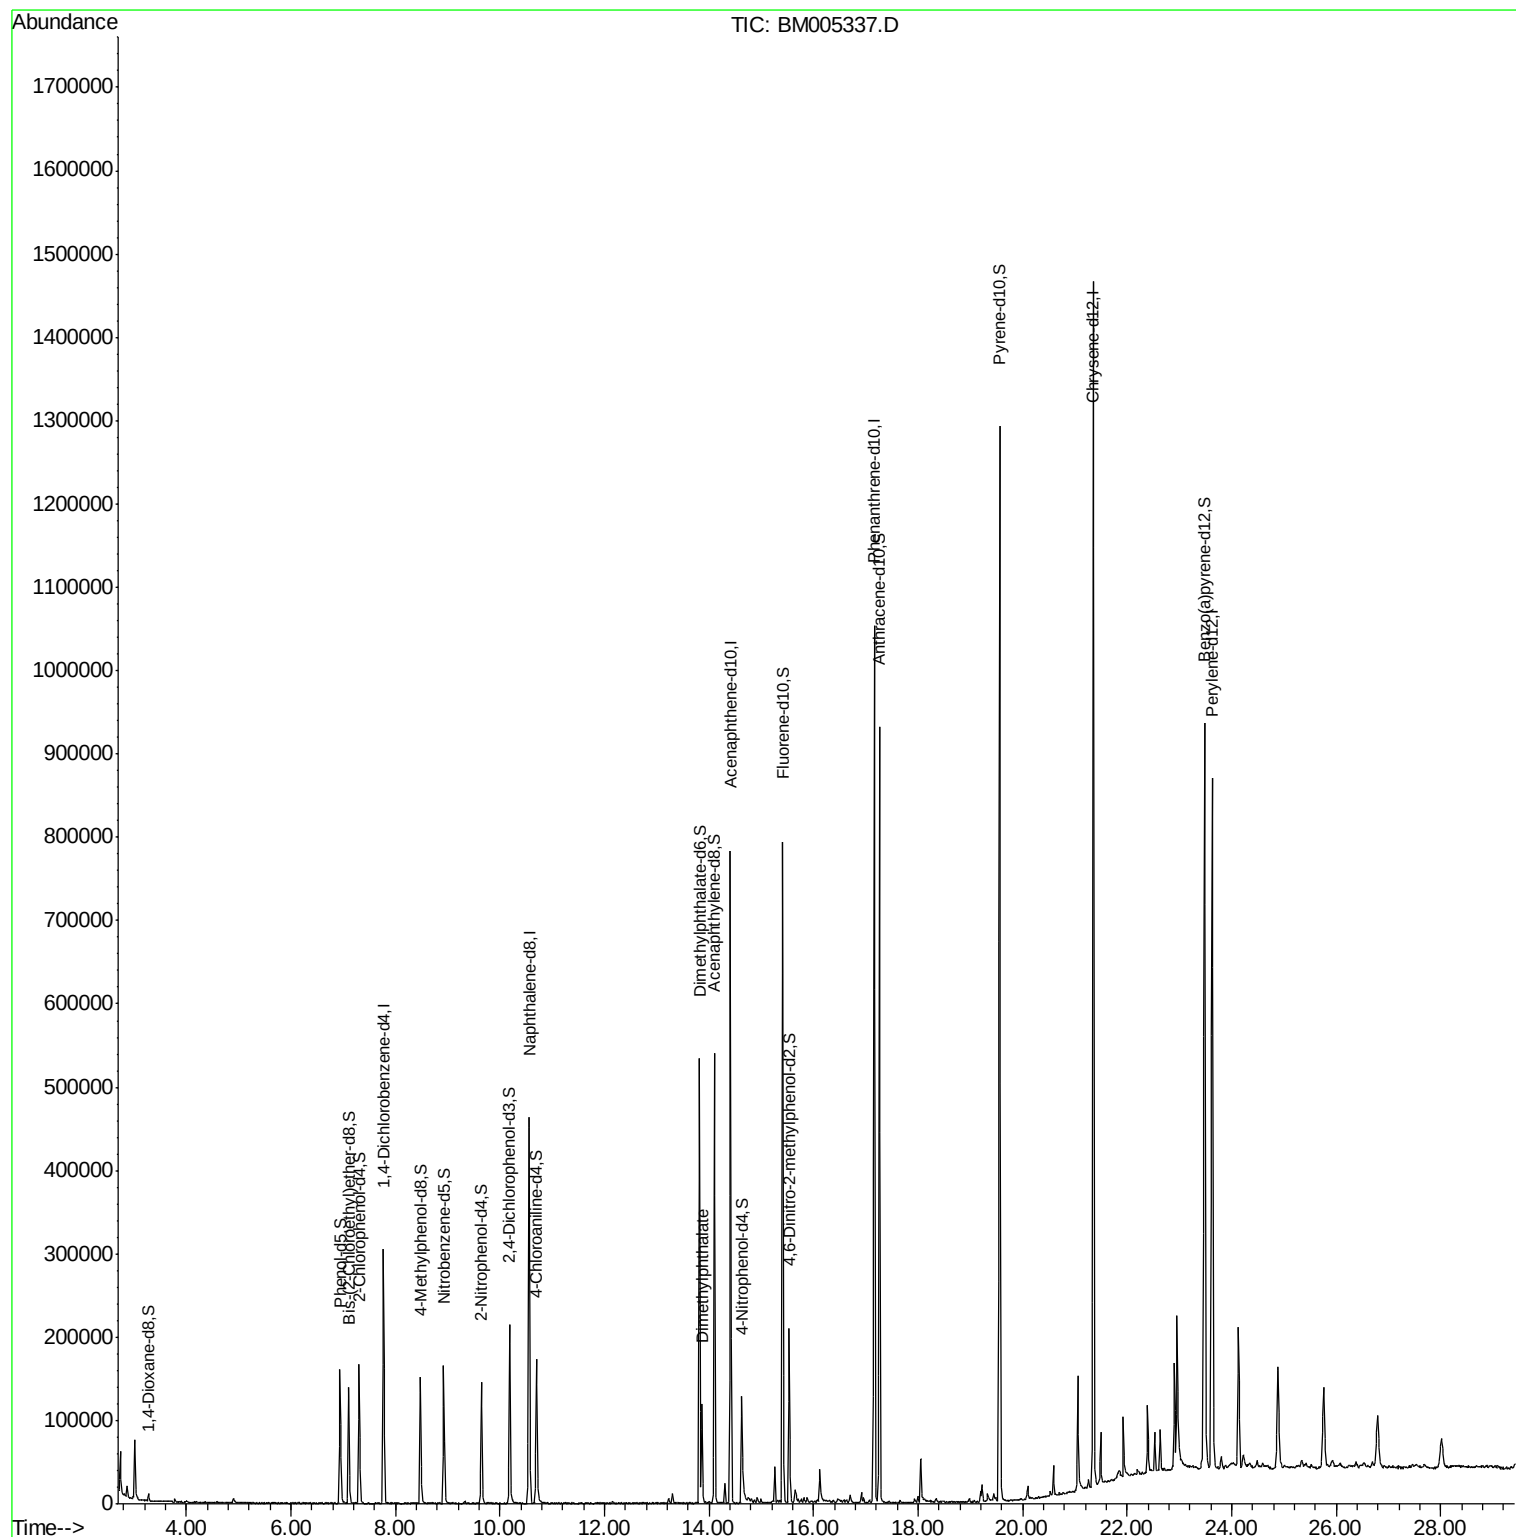

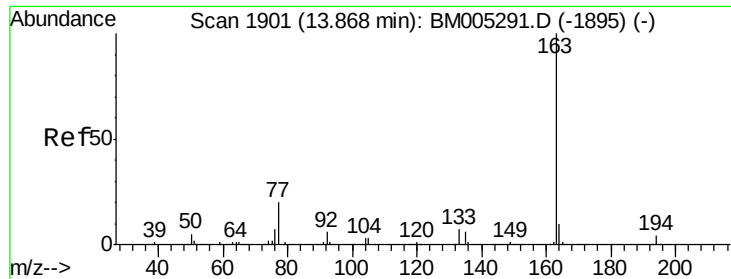

#44

Dimethylphthalate

Concen: 3.51 ng/ul

RT: 13.86 min Scan# 1900

Delta R.T. -0.01 min

Lab File: BM005337.D

Acq: 08 May 2016 08:30

Instrument :

BNA_M

ClientSampleId :

BD3A9


Tgt Ion:163 Resp: 72890

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.5 7.9 11.9

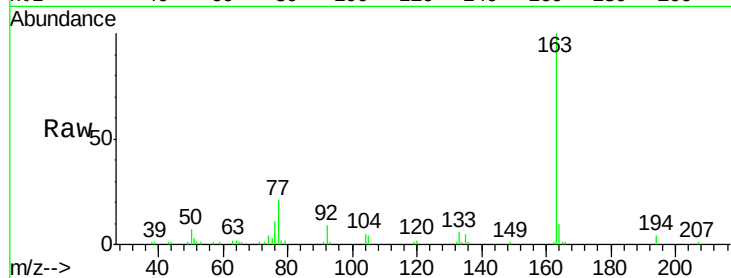

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

