

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
 Data File : BM005343.D
 Acq On : 08 May 2016 12:45
 Operator : UM/SJ
 Sample : H2772-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B4

Quant Time: May 09 04:13:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 07 07:05:19 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	98462	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	463193	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	292673	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	695924	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	804328	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	712921	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	8913	4.26	ng/uL	0.00
5) Phenol-d5	6.94	99	215909	24.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	136005	26.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	172136	25.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	185017	25.07	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	92733	28.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	99022	26.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	177609	25.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	171532	20.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	617281	26.31	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	799053	29.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	76452	17.85	ng/ul	0.00
57) Fluorene-d10	15.40	176	583890	28.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	71029	18.14	ng/ul	0.00
70) Anthracene-d10	17.26	188	930515	30.25	ng/ul	0.00
76) Pyrene-d10	19.56	212	1082870	29.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	965674	30.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	161509	6.89	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005343.D
Acq On : 08 May 2016 12:45
Operator : UM/SJ
Sample : H2772-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B4

Quant Time: May 09 04:13:34 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 07 07:05:19 2016
Response via : Initial Calibration

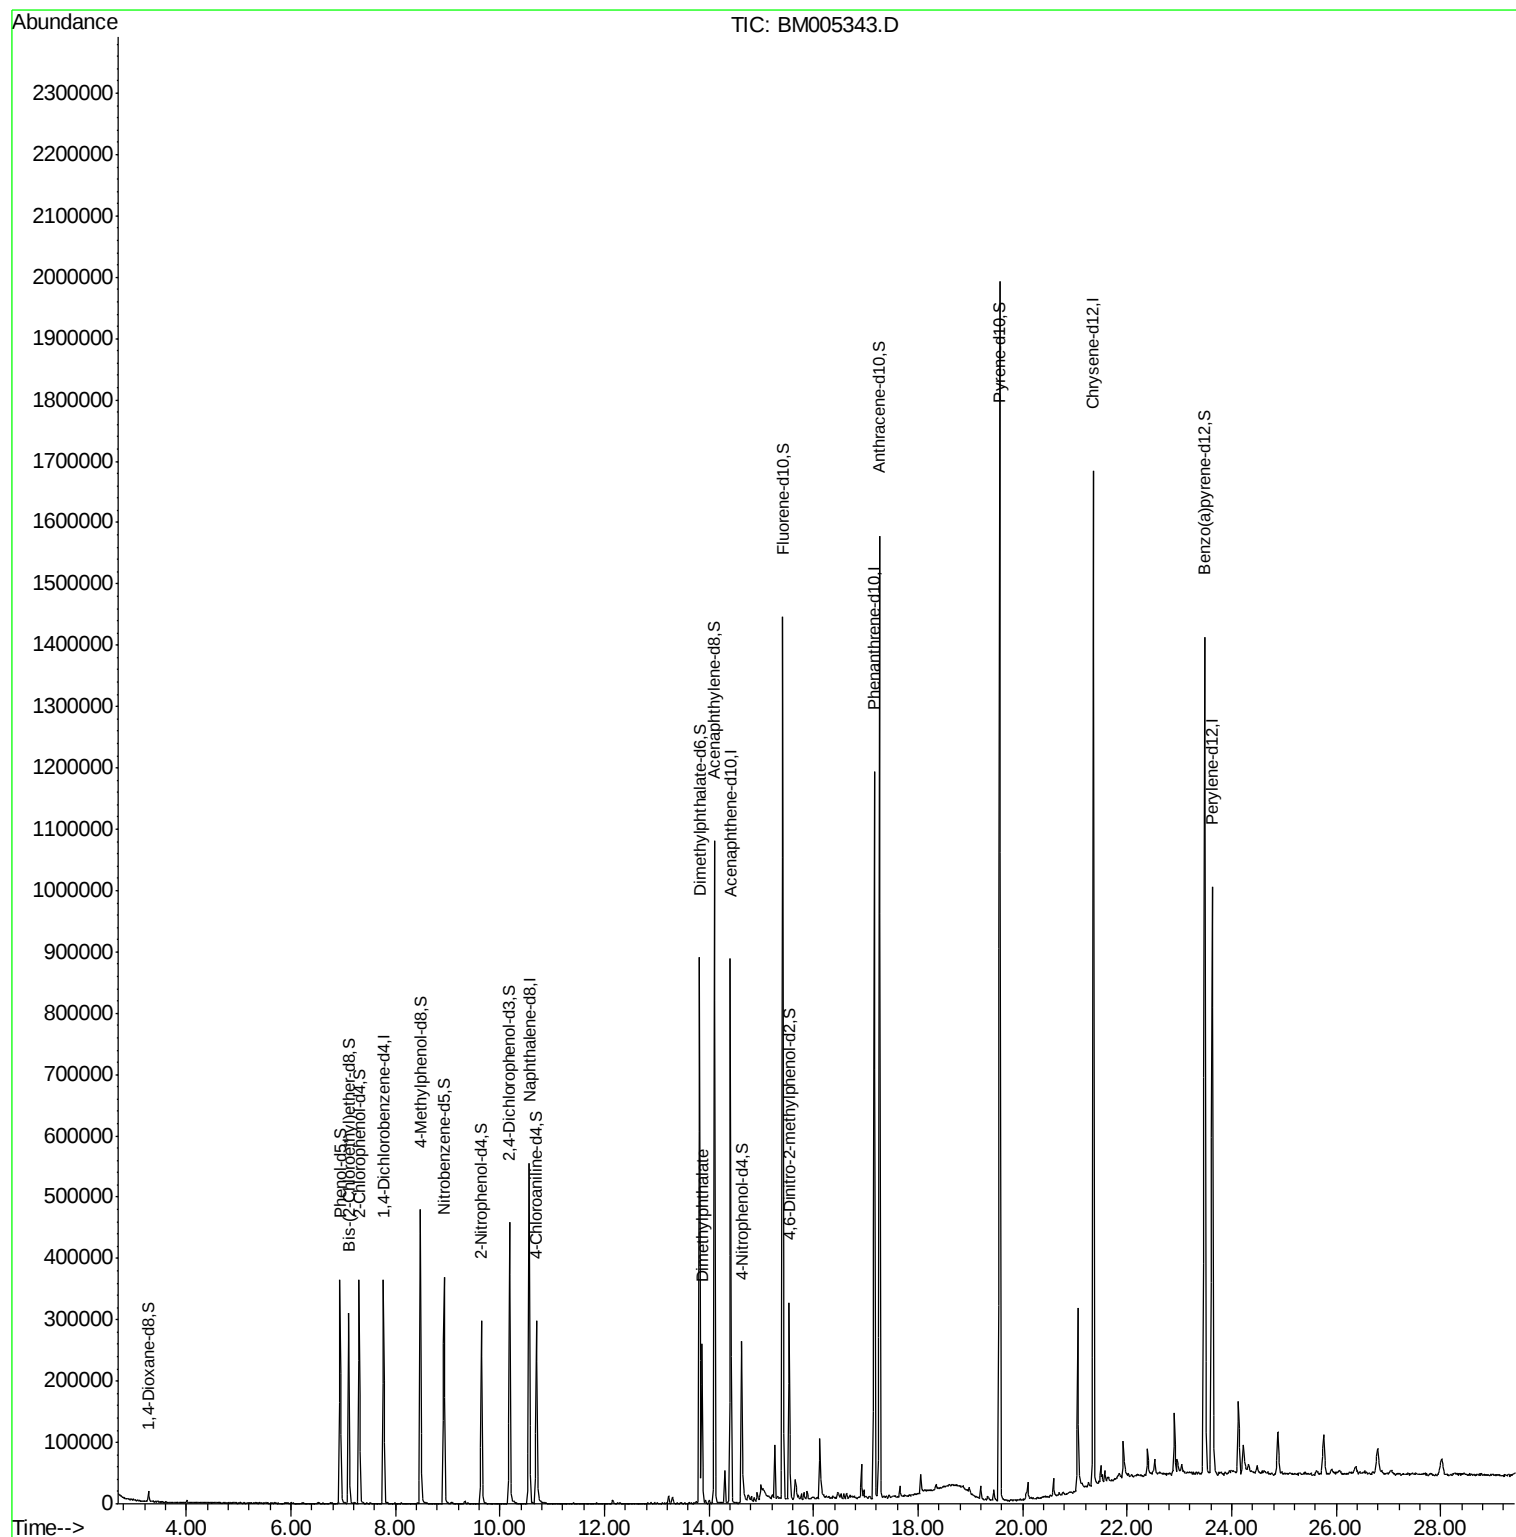

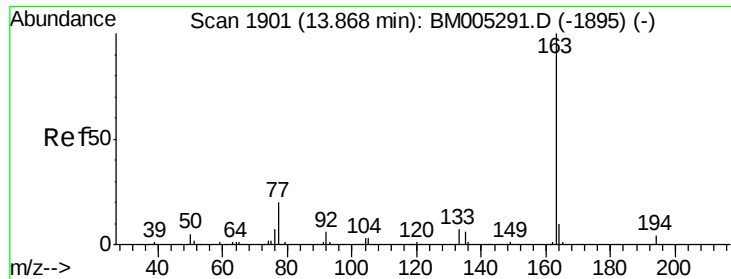

#44
 Dimethylphthalate
 Concen: 6.89 ng/ul
 RT: 13.86 min Scan# 1900
 Delta R.T. -0.01 min
 Lab File: BM005343.D
 Acq: 08 May 2016 12:45

Instrument :
 BNA_M
 ClientSampleId :
 BD3B4

Tgt Ion:	163	Resp:	161509
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.9	7.9	11.9

