

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050716\
 Data File : BM005317.D
 Acq On : 07 May 2016 19:47
 Operator : UM/SJ
 Sample : H2853-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9X16

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.945	719	724	733	rBV	74181	122657	4.41%	0.525%
2	7.104	745	751	762	rBV	270035	420337	15.10%	1.799%
3	7.304	779	785	796	rBV	283463	454181	16.32%	1.943%
4	7.769	858	864	876	rBV	256204	418010	15.02%	1.789%
5	8.475	979	984	995	rBV	242086	395354	14.21%	1.692%
6	8.928	1054	1061	1071	rBV	341529	568192	20.42%	2.431%
7	9.645	1177	1183	1198	rVB	296842	492669	17.70%	2.108%
8	10.181	1268	1274	1296	rBV	394877	710664	25.53%	3.041%
9	10.557	1331	1338	1347	rBV	399444	675906	24.29%	2.892%
10	13.821	1886	1893	1902	rBV	914166	1319156	47.40%	5.645%
11	14.104	1934	1941	1954	rBV	1013963	1535595	55.17%	6.571%
12	14.410	1987	1993	2002	rBV2	649231	1012044	36.36%	4.331%
13	14.627	2025	2030	2047	rBV2	45392	99363	3.57%	0.425%
14	15.410	2156	2163	2173	rBV	1291605	1992350	71.59%	8.525%
15	15.533	2179	2184	2193	rBV	493693	675927	24.29%	2.892%
16	17.162	2454	2461	2468	rBV2	889211	1317121	47.32%	5.636%
17	17.256	2471	2477	2488	rBV2	1451862	2264548	81.37%	9.690%
18	19.556	2862	2868	2876	rBV2	1898784	2783175	100.00%	11.909%
19	21.350	3168	3173	3185	rBV	1338349	1739474	62.50%	7.443%
20	22.903	3434	3437	3443	rVB	25461	37635	1.35%	0.161%
21	23.480	3527	3535	3551	rBV2	1333995	2637306	94.76%	11.285%
22	23.627	3552	3560	3571	rVB2	806997	1586786	57.01%	6.790%
23	24.127	3641	3645	3653	rVB	30752	55223	1.98%	0.236%
24	24.885	3769	3774	3781	rVB2	26795	56288	2.02%	0.241%


Sum of corrected areas: 23369961

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050716\
Data File : BM005317.D
Acq On : 07 May 2016 19:47
Operator : UM/SJ
Sample : H2853-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X16

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

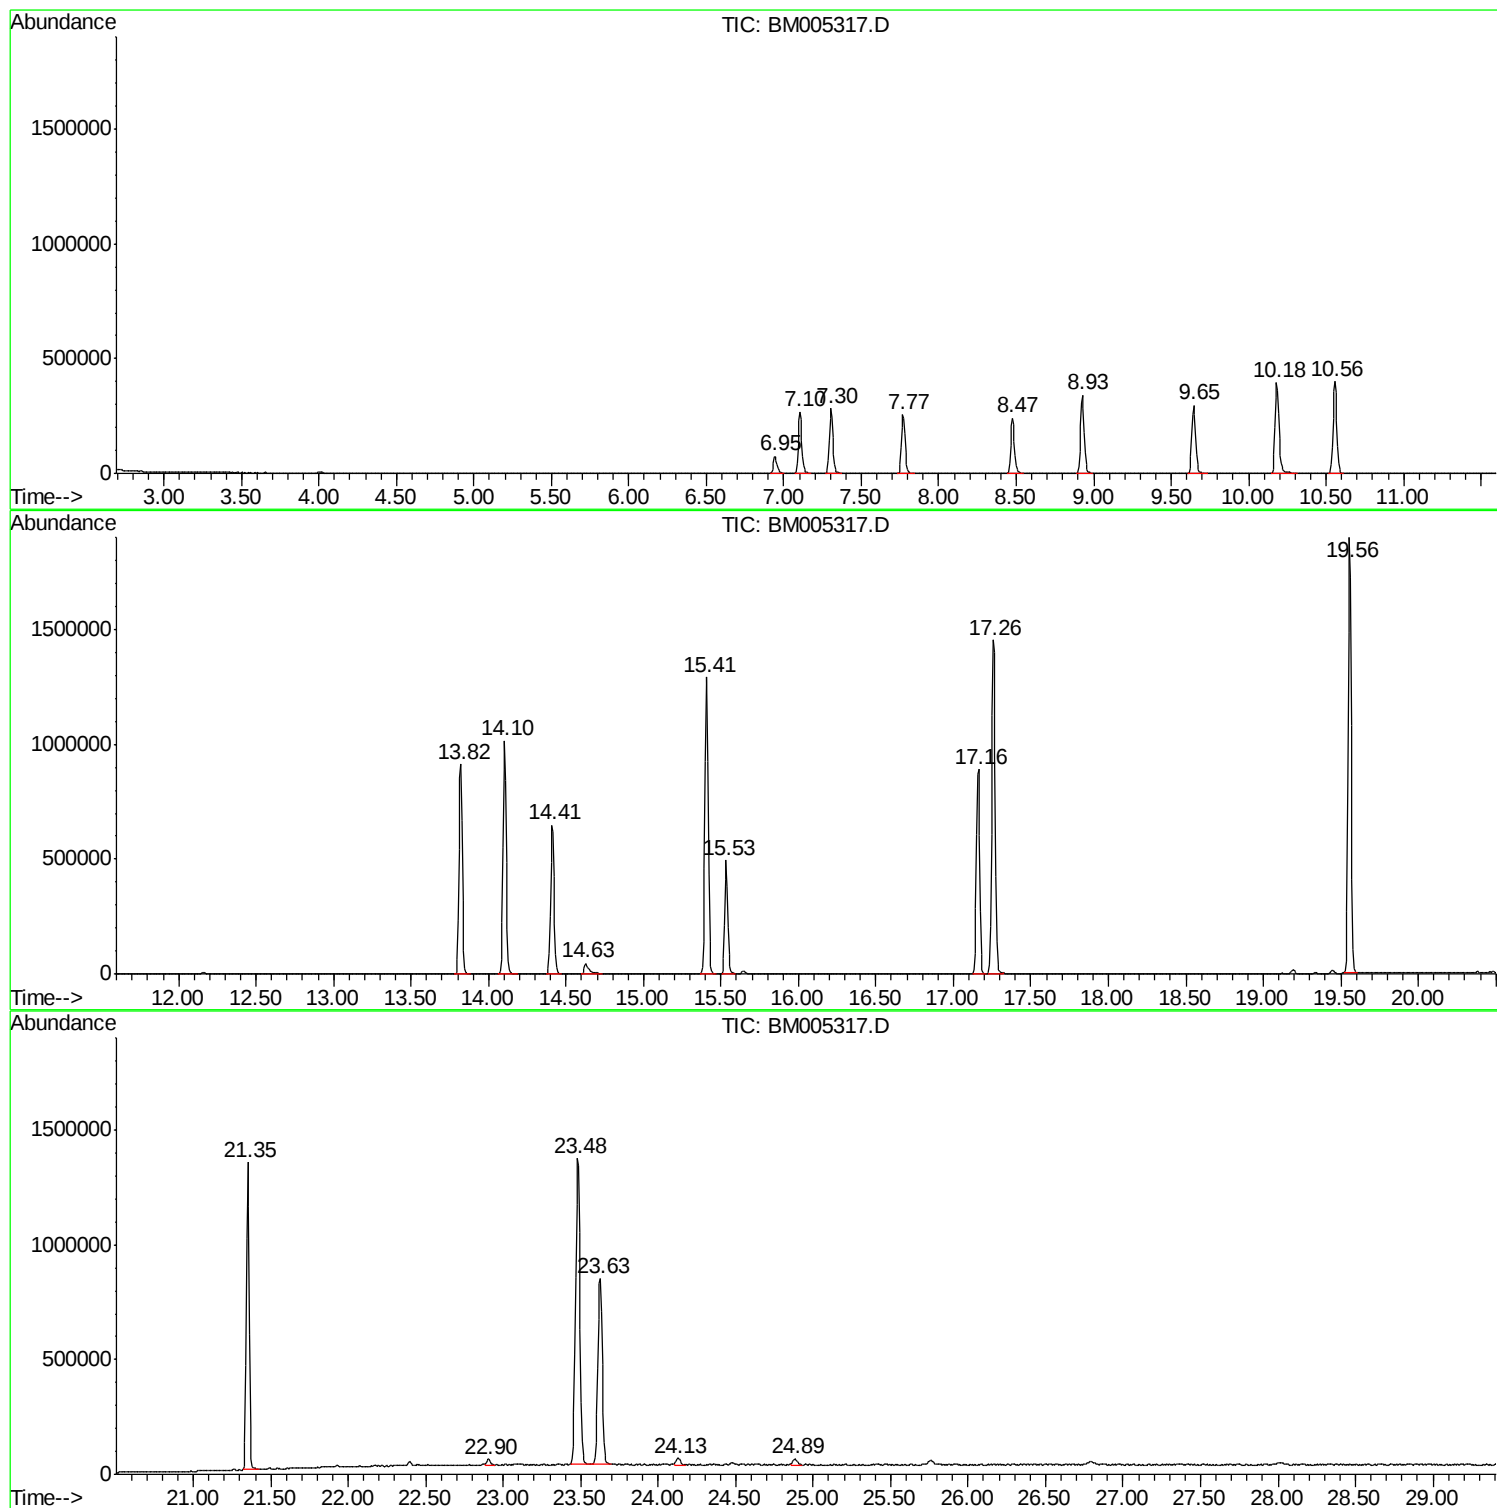

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005317.D
Acq On : 07 May 2016 19:47
Operator : UM/SJ
Sample : H2853-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X16

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005317.D
Acq On : 07 May 2016 19:47
Operator : UM/SJ
Sample : H2853-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X16

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc