

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050716\
 Data File : BM005318.D
 Acq On : 07 May 2016 20:23
 Operator : UM/SJ
 Sample : H2853-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9X17

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.946	719	724	735	rBV	64462	108492	4.20%	0.495%
2	7.104	744	751	762	rBV	237549	374526	14.50%	1.710%
3	7.304	779	785	795	rBV	252596	409071	15.84%	1.867%
4	7.769	857	864	871	rBV	244801	403999	15.64%	1.844%
5	8.475	978	984	996	rBV	221484	359948	13.93%	1.643%
6	8.928	1053	1061	1072	rBV	302379	506698	19.61%	2.313%
7	9.645	1177	1183	1193	rBV	263545	433621	16.79%	1.979%
8	10.181	1268	1274	1288	rBV	379055	674463	26.11%	3.079%
9	10.557	1331	1338	1346	rBV	394284	661078	25.59%	3.018%
10	13.822	1886	1893	1904	rBV	830295	1182529	45.78%	5.398%
11	14.104	1934	1941	1951	rBV	942925	1393901	53.96%	6.363%
12	14.410	1986	1993	2004	rVB2	631430	988379	38.26%	4.512%
13	14.627	2026	2030	2044	rBV	28545	66371	2.57%	0.303%
14	15.404	2156	2162	2173	rBV	1211058	1825322	70.66%	8.332%
15	15.533	2178	2184	2194	rVV	437540	593042	22.96%	2.707%
16	17.157	2454	2460	2471	rBV2	889514	1293616	50.08%	5.905%
17	17.257	2471	2477	2488	rBV2	1371024	2078102	80.45%	9.486%
18	19.333	2826	2830	2836	rBV	22277	32069	1.24%	0.146%
19	19.557	2862	2868	2882	rBV2	1808505	2583257	100.00%	11.792%
20	21.351	3167	3173	3183	rBV	1283468	1737581	67.26%	7.932%
21	22.909	3434	3438	3443	rVB2	27273	37073	1.44%	0.169%
22	23.480	3527	3535	3547	rBV2	1233211	2470738	95.64%	11.279%
23	23.627	3552	3560	3569	rVB2	790214	1568749	60.73%	7.161%
24	24.133	3641	3646	3651	rVB2	32114	59478	2.30%	0.272%
25	24.886	3769	3774	3781	rVB3	31534	64088	2.48%	0.293%


Sum of corrected areas: 21906191

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050716\
Data File : BM005318.D
Acq On : 07 May 2016 20:23
Operator : UM/SJ
Sample : H2853-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
D9X17

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

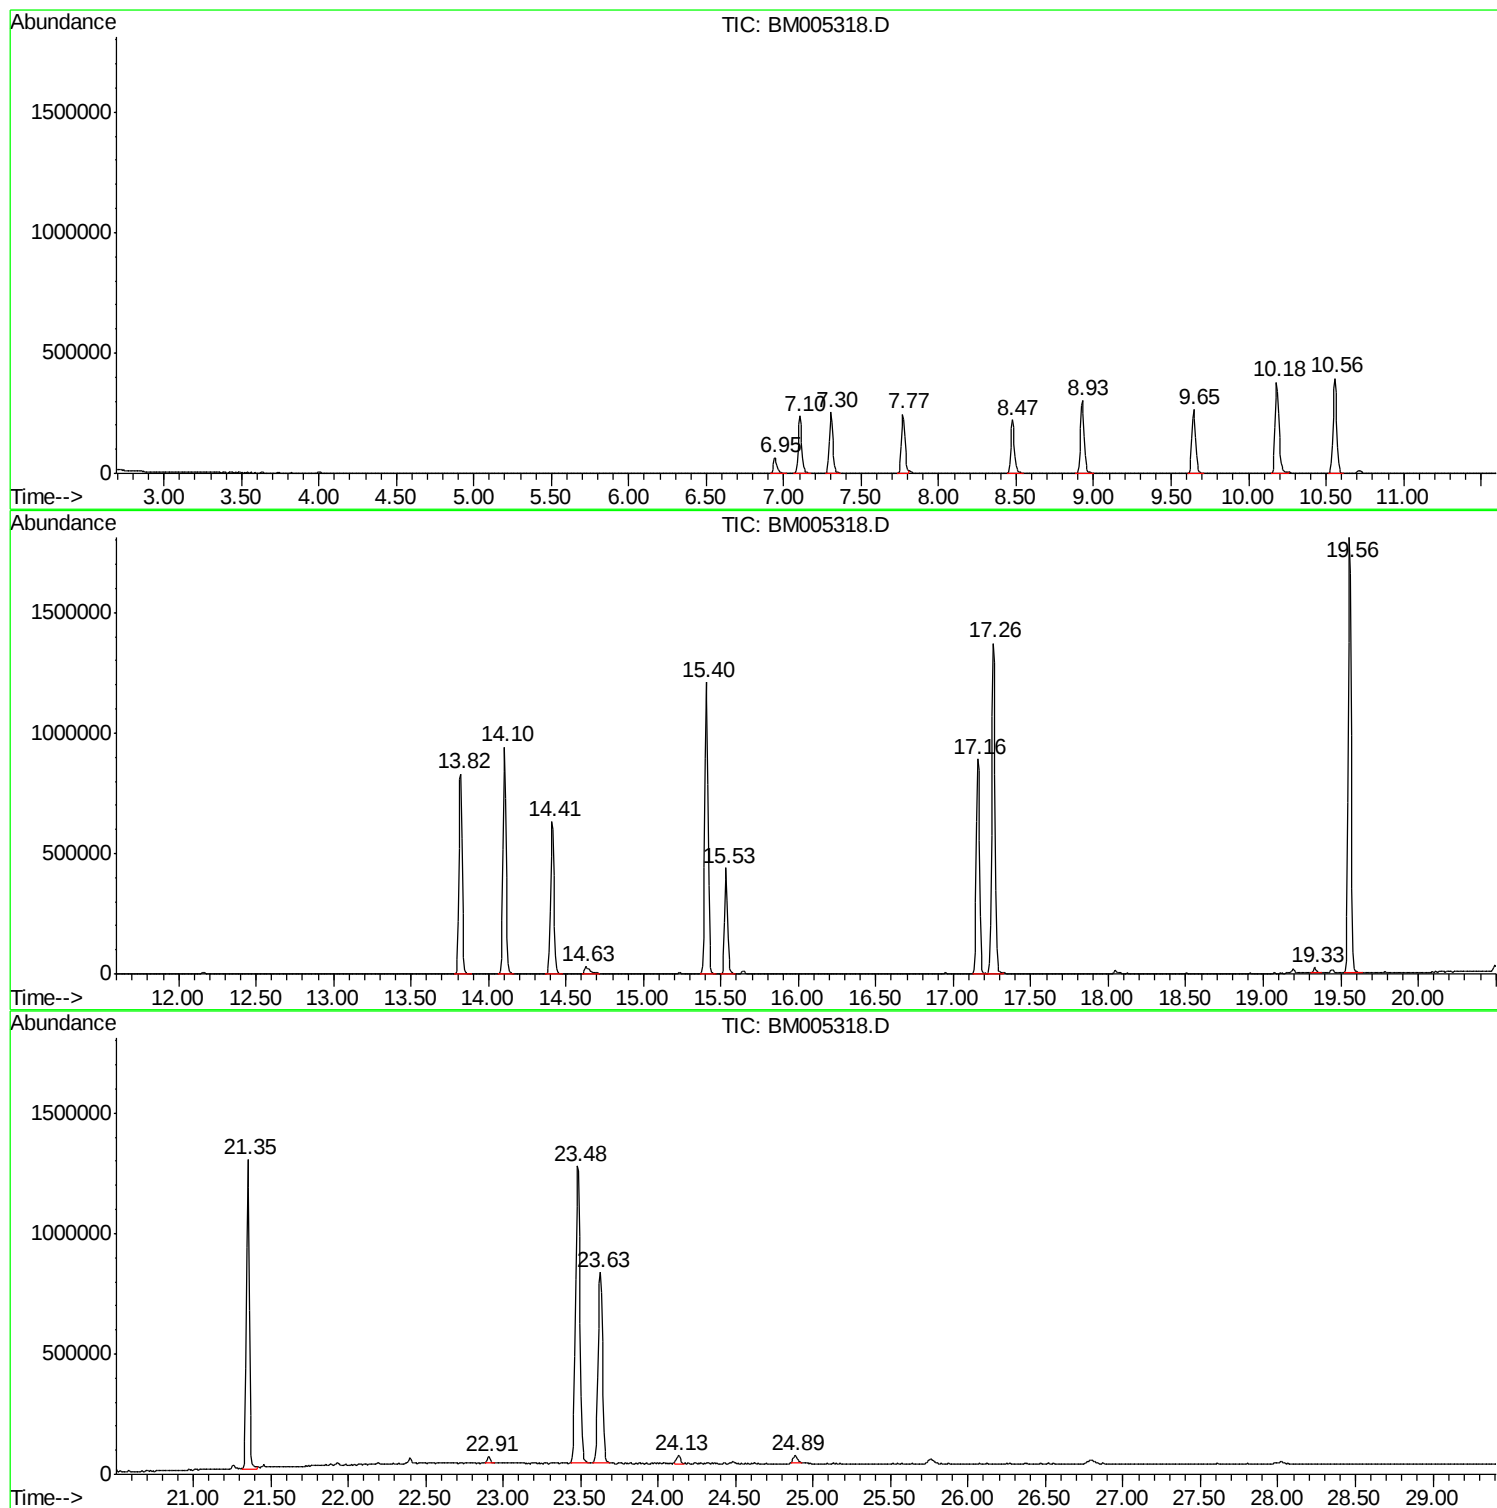

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005318.D
Acq On : 07 May 2016 20:23
Operator : UM/SJ
Sample : H2853-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X17

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050716\
Data File : BM005318.D
Acq On : 07 May 2016 20:23
Operator : UM/SJ
Sample : H2853-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X17

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc