

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\
 Data File : BM029887.D
 Acq On : 07 May 2021 22:10
 Operator : CG/JU
 Sample : M2129-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AC4

Manual Integrations
 APPROVED

mohammad
 5/10/2021 11:45:23 AM

Quant Time: May 08 00:06:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 07 13:53:15 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	123498	20.00	ng/ul	0.00
20) Naphthalene-d8	10.33	136	548641	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.20	164	371725	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.95	188	782720	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	858592	20.00	ng/ul	0.00
88) Perylene-d12	23.29	264	900511	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.07	96	5864	1.90	ng/uL	0.01
4) Pyridine-d5	3.55	84	34153m	4.41	ng/ul	0.06
7) Phenol-d5	6.75	99	105644	9.20	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.90	67	68422	9.61	ng/ul	0.00
11) 2-Chlorophenol-d4	7.09	132	90479	10.21	ng/ul	0.00
15) 4-Methylphenol-d8	8.27	113	90238	9.50	ng/ul	0.00
21) Nitrobenzene-d5	8.72	128	43412	11.48	ng/ul	0.00
24) 2-Nitrophenol-d4	9.43	143	44641	10.46	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	82190	9.61	ng/ul	0.00
31) 4-Chloroaniline-d4	10.49	131	99150	7.61	ng/ul	0.00
46) Dimethylphthalate-d6	13.62	166	376292	13.06	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	444772	12.18	ng/ul	0.00
54) 4-Nitrophenol-d4	14.46	143	28271m	6.02	ng/ul	0.02
60) Fluorene-d10	15.20	176	313832	12.83	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	36264	7.13	ng/ul	0.00
73) Anthracene-d10	17.04	188	525413	13.33	ng/ul	0.00
81) Pyrene-d10	19.34	212	677365	15.38	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.15	264	736247	14.42	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.67	163	35596	1.234	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\
Data File : BM029887.D
Acq On : 07 May 2021 22:10
Operator : CG/JU
Sample : M2129-08
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E0AC4

Quant Time: May 08 00:06:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 07 13:53:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/10/2021 11:45:23 AM

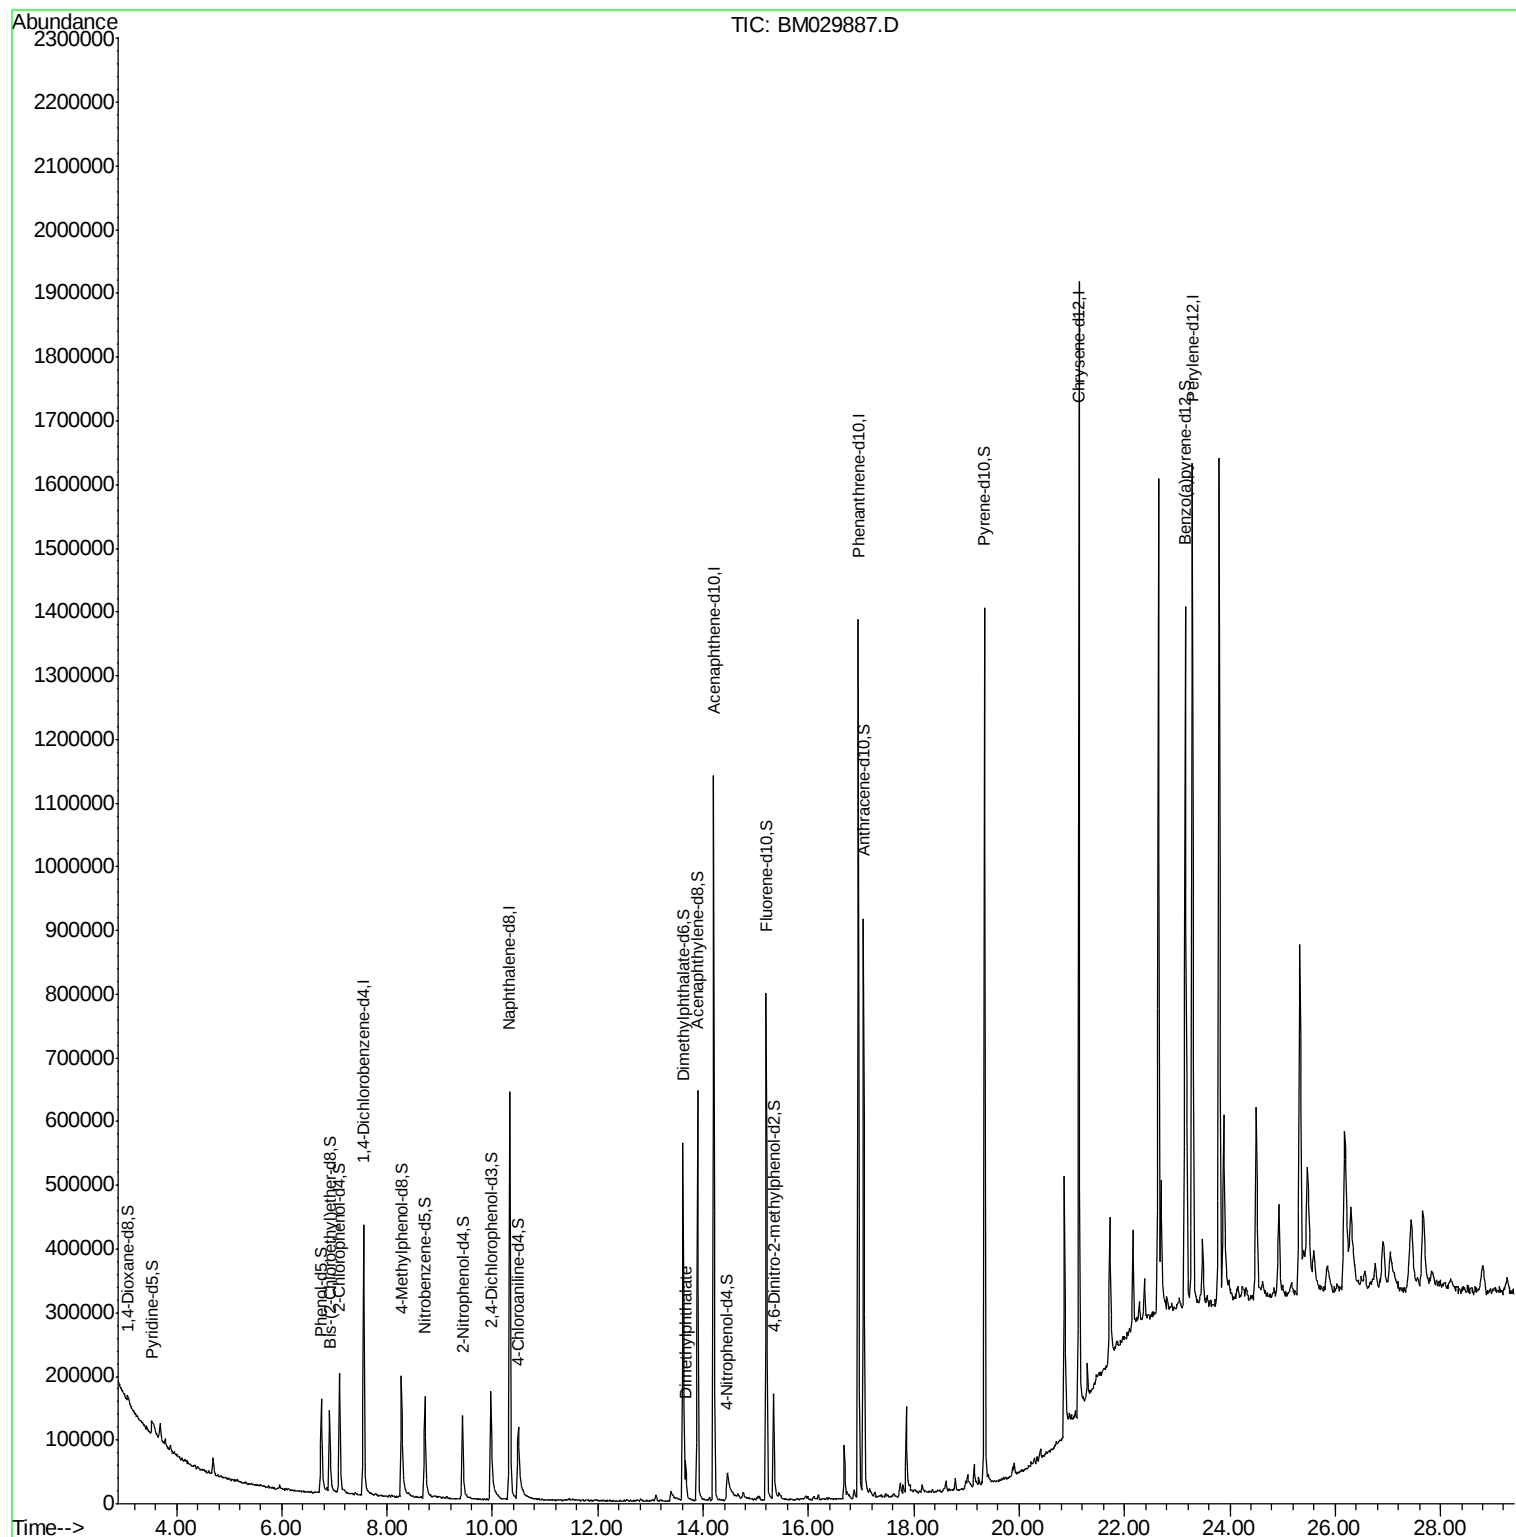

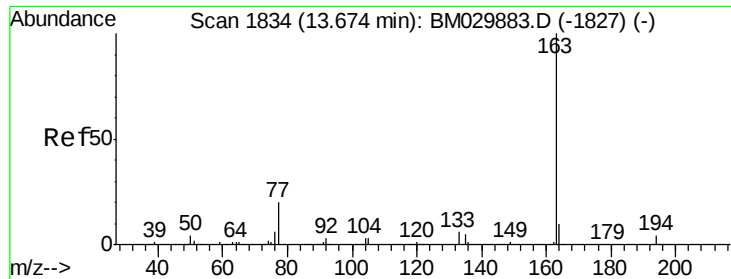


#47
 Dimethylphthalate
 Concen: 1.234 ng/ul
 RT: 13.67 min Scan# 1834
 Delta R.T. -0.00 min
 Lab File: BM029887.D
 Acq: 07 May 2021 22:10

Instrument :
 BNA_M
 ClientSampleId :
 E0AC4

Tot Ion	Ratio	Resp	Lower	Upper
163	100	35596		
194	4.6		3.4	5.0
164	9.4		7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/10/2021 11:45:23 AM

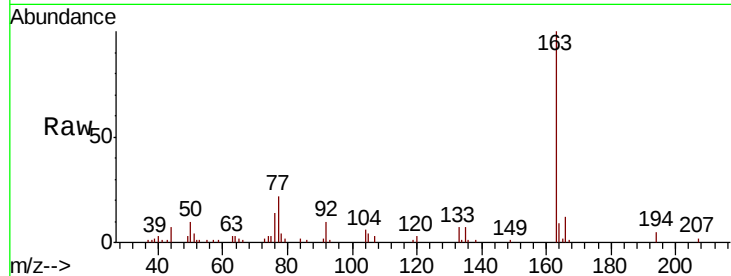

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

