

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\  
 Data File : BM029888.D  
 Acq On : 07 May 2021 22:46  
 Operator : CG/JU  
 Sample : M2129-04  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 E0AC0

Quant Time: May 08 00:13:58 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050721.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri May 07 23:49:53 2021  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min)      |
|--------------------------------|-------|------|----------|-------|-------|---------------|
| 1) 1,4-Dichlorobenzene-d4      | 7.56  | 152  | 133112   | 20.00 | ng/ul | 0.00          |
| 20) Naphthalene-d8             | 10.33 | 136  | 616080   | 20.00 | ng/ul | 0.00          |
| 38) Acenaphthene-d10           | 14.20 | 164  | 414715   | 20.00 | ng/ul | 0.00          |
| 64) Phenanthrene-d10           | 16.95 | 188  | 864793   | 20.00 | ng/ul | 0.00          |
| 79) Chrysene-d12               | 21.13 | 240  | 935739   | 20.00 | ng/ul | 0.00          |
| 88) Perylene-d12               | 23.29 | 264  | 933122   | 20.00 | ng/ul | 0.00          |
| System Monitoring Compounds    |       |      |          |       |       |               |
| 3) 1,4-Dioxane-d8              | 3.06  | 96   | 15789    | 4.74  | ng/uL | 0.00          |
| 4) Pyridine-d5                 | 3.49  | 84   | 168455   | 20.19 | ng/ul | 0.00          |
| 7) Phenol-d5                   | 6.74  | 99   | 279402   | 22.57 | ng/ul | 0.00          |
| 9) Bis-(2-Chloroethyl)ether-d  | 6.90  | 67   | 191428   | 24.94 | ng/ul | 0.00          |
| 11) 2-Chlorophenol-d4          | 7.09  | 132  | 237792   | 24.89 | ng/ul | 0.00          |
| 15) 4-Methylphenol-d8          | 8.27  | 113  | 239005   | 23.35 | ng/ul | 0.00          |
| 21) Nitrobenzene-d5            | 8.71  | 128  | 122618   | 28.88 | ng/ul | 0.00          |
| 24) 2-Nitrophenol-d4           | 9.43  | 143  | 133317   | 27.82 | ng/ul | 0.00          |
| 28) 2,4-Dichlorophenol-d3      | 9.96  | 165  | 236456   | 24.61 | ng/ul | 0.00          |
| 31) 4-Chloroaniline-d4         | 10.48 | 131  | 323832   | 22.15 | ng/ul | 0.00          |
| 46) Dimethylphthalate-d6       | 13.62 | 166  | 894819   | 27.84 | ng/ul | 0.00          |
| 49) Acenaphthylene-d8          | 13.89 | 160  | 1124988  | 27.62 | ng/ul | 0.00          |
| 54) 4-Nitrophenol-d4           | 14.44 | 143  | 89111    | 17.02 | ng/ul | 0.00          |
| 60) Fluorene-d10               | 15.20 | 176  | 786058   | 28.81 | ng/ul | 0.00          |
| 65) 4,6-Dinitro-2-methylphenol | 15.33 | 200  | 107892   | 19.21 | ng/ul | 0.00          |
| 73) Anthracene-d10             | 17.04 | 188  | 1236192  | 28.39 | ng/ul | 0.00          |
| 81) Pyrene-d10                 | 19.34 | 212  | 1425361  | 29.69 | ng/ul | 0.00          |
| 92) Benzo(a)pyrene-d12         | 23.16 | 264  | 1444518  | 27.31 | ng/ul | 0.00          |
| Target Compounds               |       |      |          |       |       |               |
| 47) Dimethylphthalate          | 13.67 | 163  | 51514    | 1.600 | ng/ul | Ovalue<br>100 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\  
Data File : BM029888.D  
Acq On : 07 May 2021 22:46  
Operator : CG/JU  
Sample : M2129-04  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
E0AC0

Quant Time: May 08 00:13:58 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050721.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri May 07 23:49:53 2021  
Response via : Initial Calibration

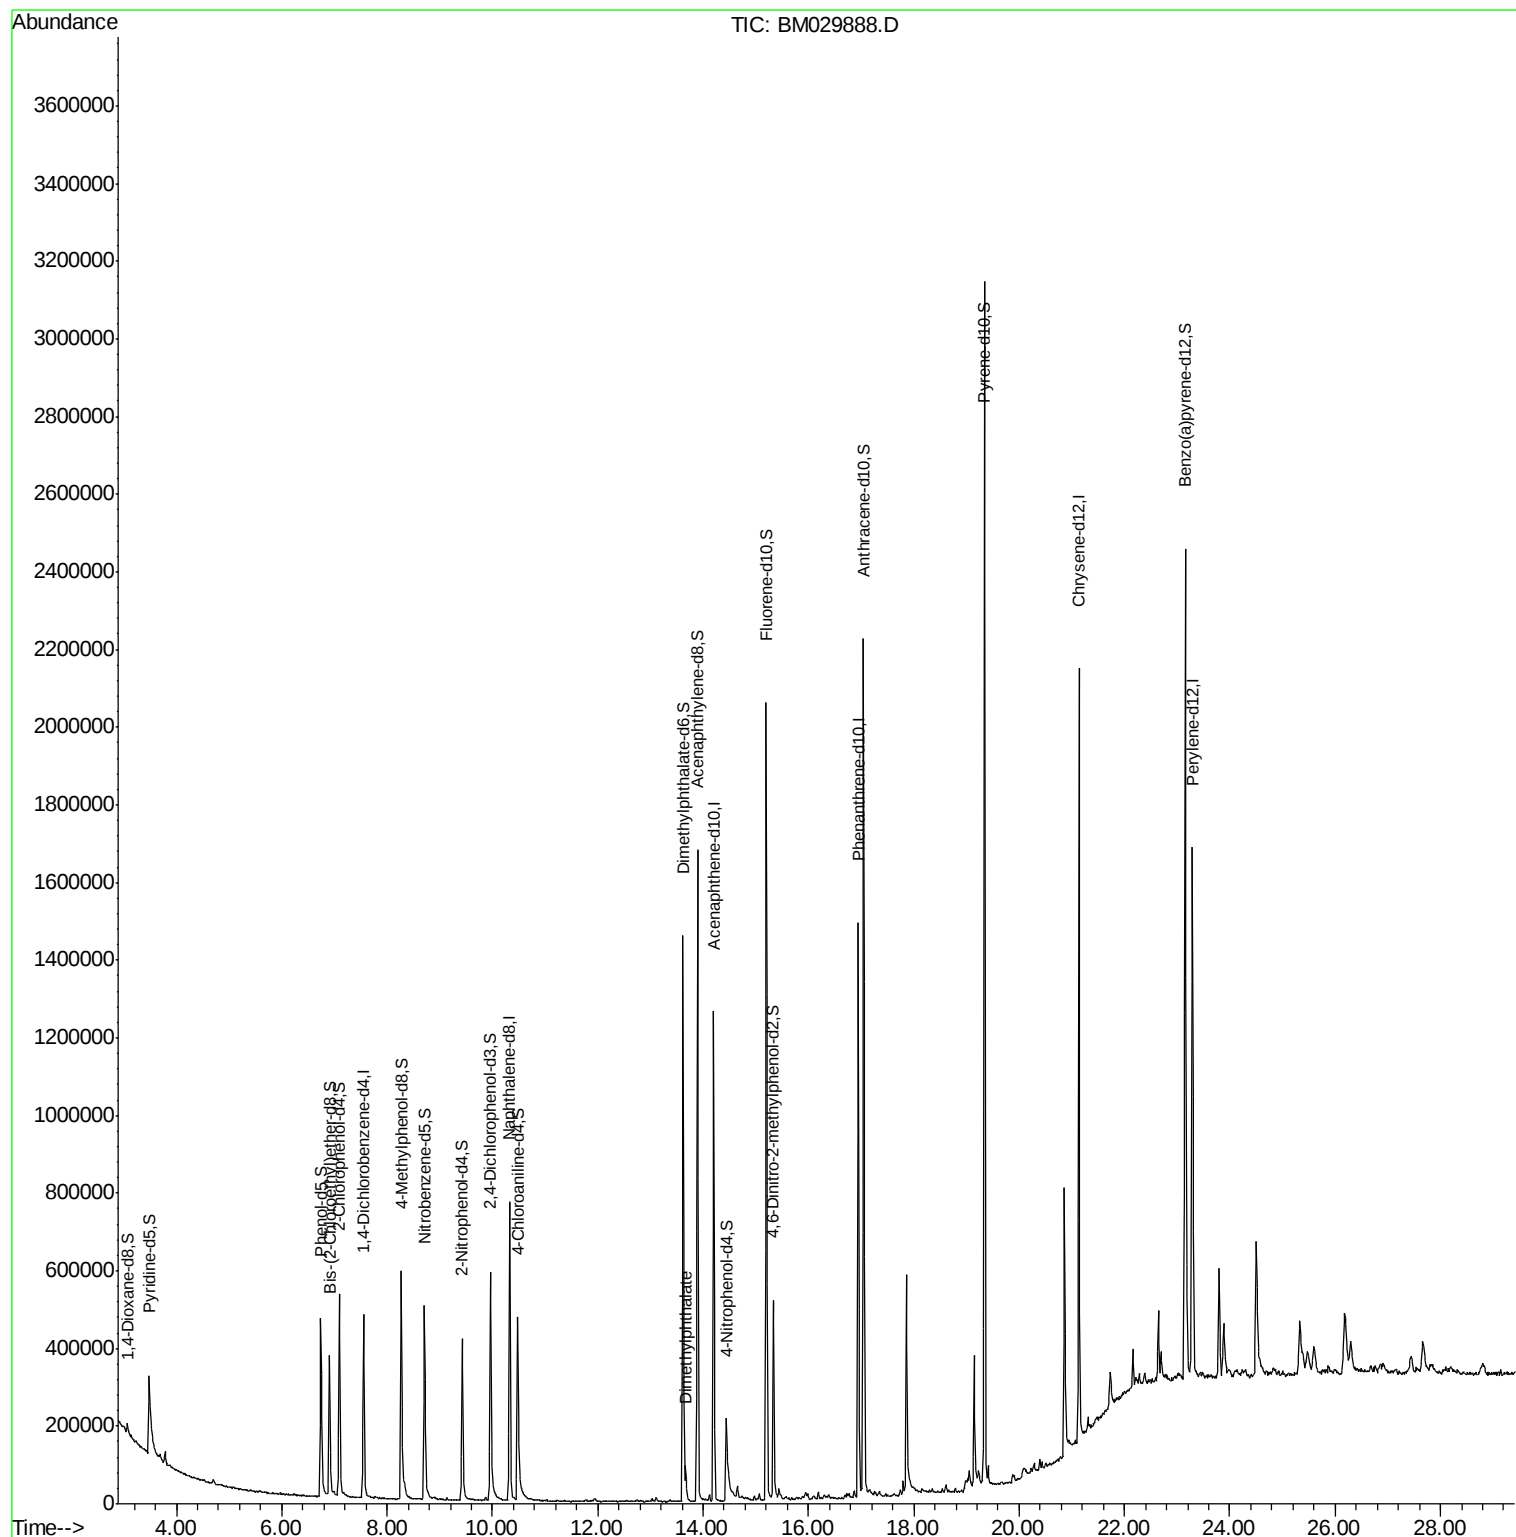

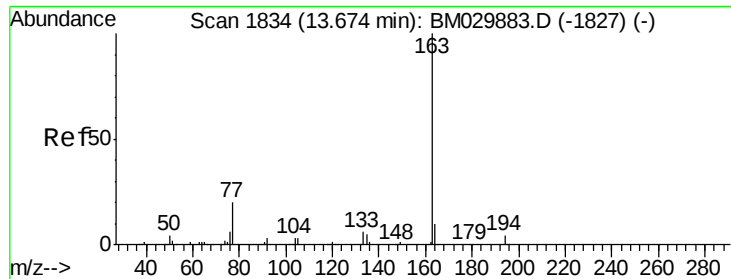

#47

Dimethylphthalate

Concen: 1.600 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BM029888.D

Acq: 07 May 2021 22:46

Instrument :

BNA\_M

ClientSampleId :

E0AC0


Tot Ion:163 Resp: 51514

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.7 7.8 11.8

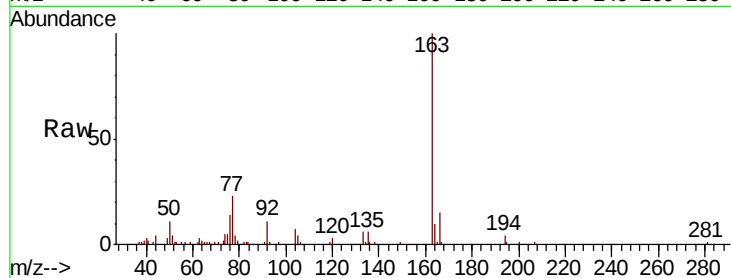

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

