

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\
 Data File : BM029890.D
 Acq On : 07 May 2021 23:58
 Operator : CG/JU
 Sample : M2129-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AC6

Quant Time: May 08 00:35:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 07 23:49:53 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	141488	20.00	ng/ul	0.00
20) Naphthalene-d8	10.33	136	660373	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.20	164	445730	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.95	188	932331	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	998895	20.00	ng/ul	0.00
88) Perylene-d12	23.29	264	1013948	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	19773	5.58	ng/uL	0.00
4) Pyridine-d5	3.49	84	190428	21.47	ng/ul	0.00
7) Phenol-d5	6.74	99	322773	24.53	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.90	67	209757	25.71	ng/ul	0.00
11) 2-Chlorophenol-d4	7.09	132	265730	26.17	ng/ul	0.00
15) 4-Methylphenol-d8	8.27	113	278064	25.55	ng/ul	0.00
21) Nitrobenzene-d5	8.71	128	130357	28.65	ng/ul	0.00
24) 2-Nitrophenol-d4	9.43	143	145643	28.36	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.96	165	265237	25.75	ng/ul	0.00
31) 4-Chloroaniline-d4	10.48	131	381762	24.36	ng/ul	0.00
46) Dimethylphthalate-d6	13.62	166	965698	27.95	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	1222652	27.93	ng/ul	0.00
54) 4-Nitrophenol-d4	14.44	143	103950	18.47	ng/ul	0.00
60) Fluorene-d10	15.20	176	851812	29.04	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.33	200	113338	18.72	ng/ul	0.00
73) Anthracene-d10	17.05	188	1303878	27.77	ng/ul	0.00
81) Pyrene-d10	19.34	212	1531921	29.90	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.16	264	1579758	27.49	ng/ul	0.00
Target Compounds						
8) Phenol	6.77	94	20617	1.535	ng/ul#	78
47) Dimethylphthalate	13.67	163	59860	1.730	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050721\
Data File : BM029890.D
Acq On : 07 May 2021 23:58
Operator : CG/JU
Sample : M2129-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AC6

Quant Time: May 08 00:35:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 07 23:49:53 2021
Response via : Initial Calibration

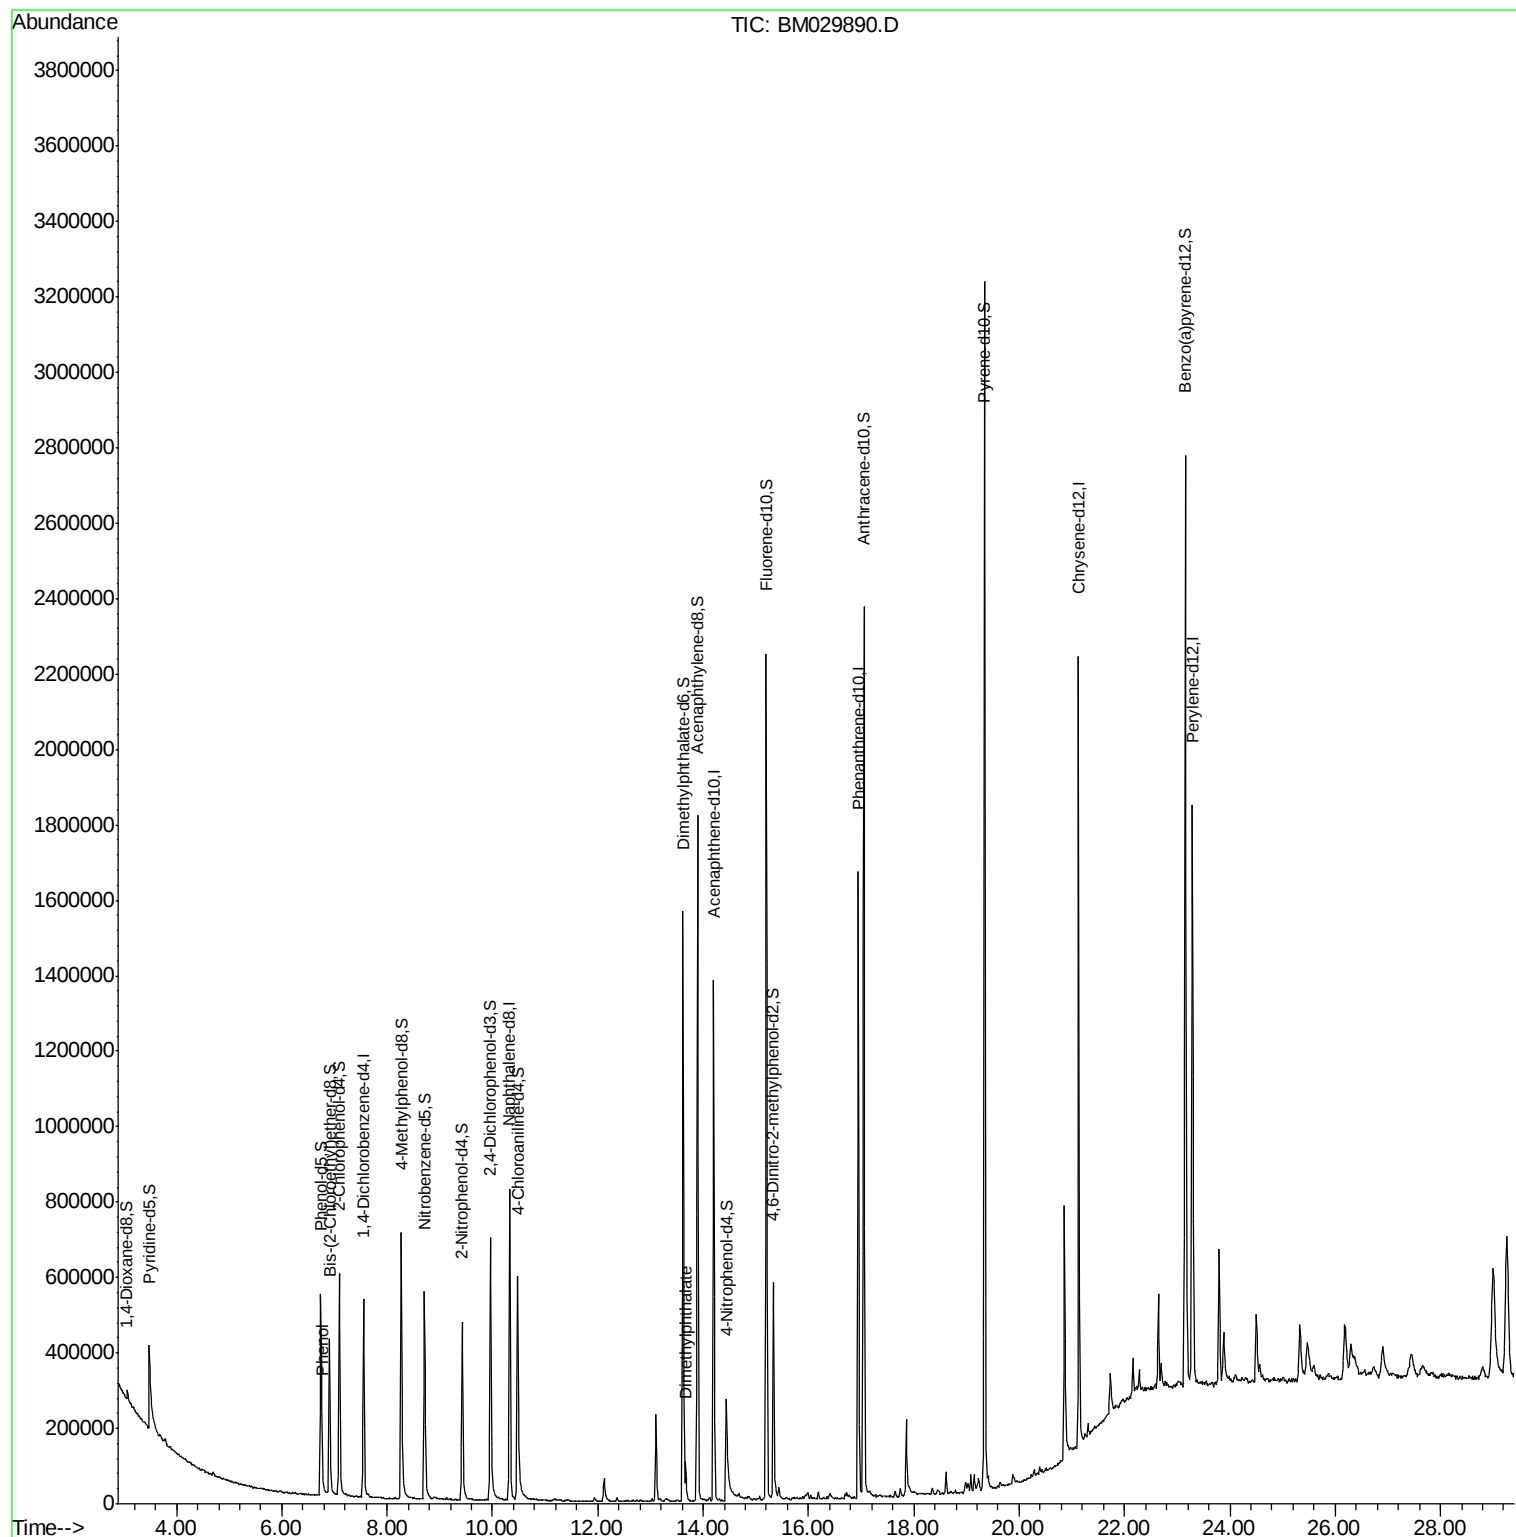

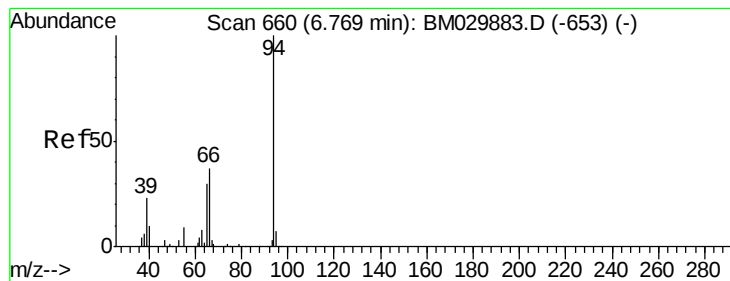





#8

Phenol

Concen: 1.535 ng/ul
 RT: 6.77 min Scan# 660
 Delta R.T. -0.00 min
 Lab File: BM029890.D
 Acq: 07 May 2021 23:58

Instrument :
 BNA_M
 ClientSampleId :
 E0AC6

Tot Ion: 94 Resp: 20617
 Ion Ratio Lower Upper
 94 100
 65 33.0 23.3 34.9
 66 58.6 30.6 45.8#

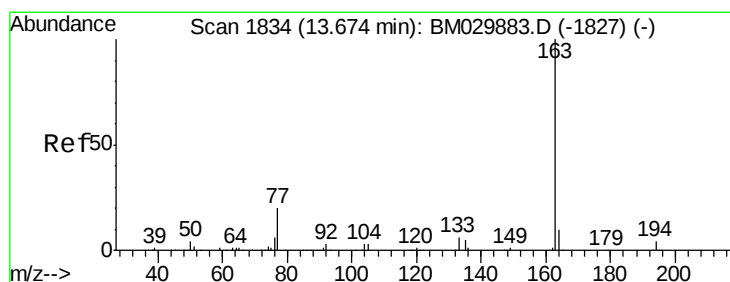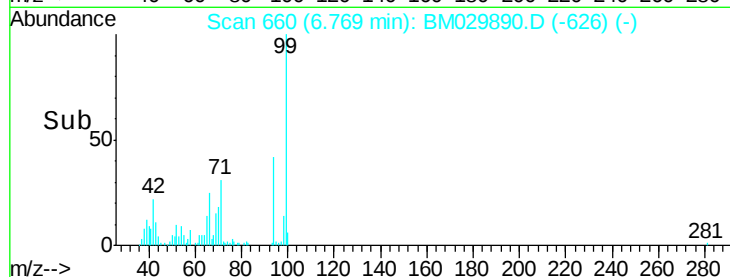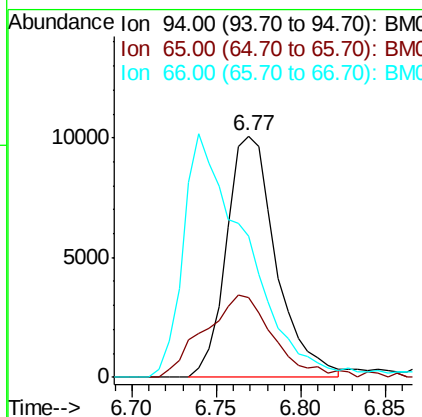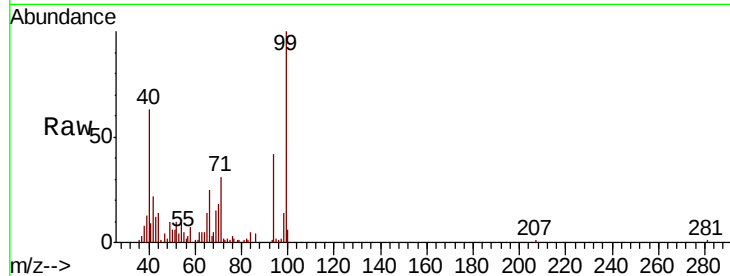

#47

Dimethylphthalate

Concen: 1.730 ng/ul
 RT: 13.67 min Scan# 1833
 Delta R.T. -0.01 min
 Lab File: BM029890.D
 Acq: 07 May 2021 23:58

Tgt Ion:163 Resp: 59860
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.4 5.0
 164 9.6 7.8 11.8

