

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
 Data File : BM050137.D
 Acq On : 07 May 2025 16:24
 Operator : RC/JU
 Sample : Q1945-01DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB1WDL

Quant Time: May 07 17:05:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.746	152	237908	20.000	ng	-0.02
21) Naphthalene-d8	10.540	136	833708	20.000	ng	-0.02
39) Acenaphthene-d10	14.392	164	563306	20.000	ng	-0.02
64) Phenanthrene-d10	17.145	188	1154973	20.000	ng	-0.01
76) Chrysene-d12	21.392	240	1121664	20.000	ng	0.00
86) Perylene-d12	24.386	264	1136201	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.346	112	193342	14.231	ng	-0.01
7) Phenol-d6	6.957	99	135739	7.949	ng	0.00
23) Nitrobenzene-d5	8.910	82	275583	16.288	ng	-0.02
42) 2,4,6-Tribromophenol	15.898	330	223621	26.848	ng	0.00
45) 2-Fluorobiphenyl	13.010	172	748052	15.710	ng	-0.02
79) Terphenyl-d14	19.768	244	1216066	16.043	ng	-0.01
Target Compounds						
35) Caprolactam	11.492	113	95555m	23.603	ng	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050137.D
Acq On : 07 May 2025 16:24
Operator : RC/JU
Sample : Q1945-01DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB1WDL

Quant Time: May 07 17:05:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

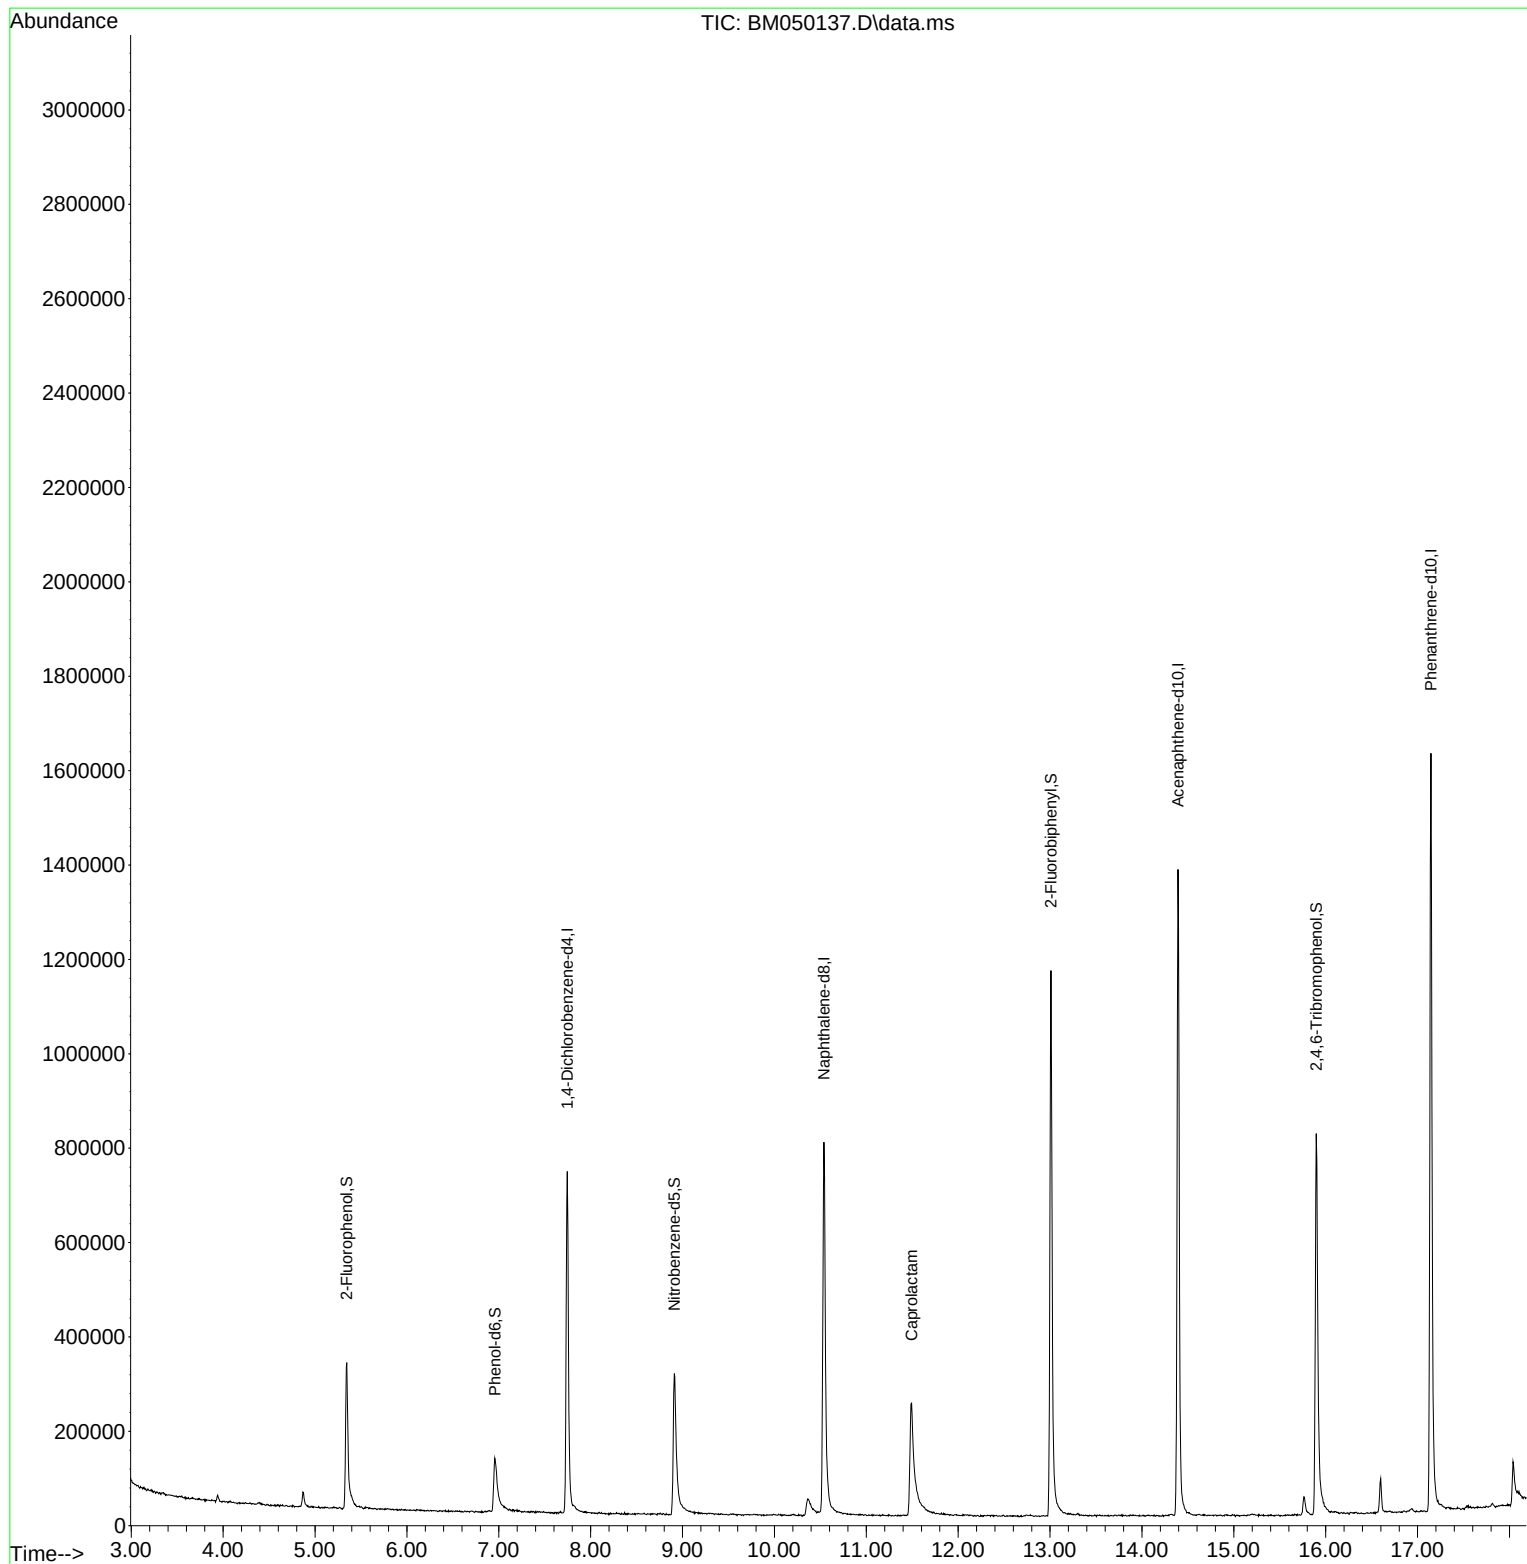

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050137.D
Acq On : 07 May 2025 16:24
Operator : RC/JU
Sample : Q1945-01DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB1WDL

Quant Time: May 07 17:05:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

