

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050725\  
 Data File : BM050138.D  
 Acq On : 07 May 2025 17:03  
 Operator : RC/JU  
 Sample : Q1945-02DL 5X  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 GB3WDL

Quant Time: May 07 18:00:48 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Apr 28 18:09:16 2025  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc   | Units | Dev(Min)  |
|-----------------------------|--------|------|----------|--------|-------|-----------|
| -----                       |        |      |          |        |       |           |
| Internal Standards          |        |      |          |        |       |           |
| 1) 1,4-Dichlorobenzene-d4   | 7.745  | 152  | 252681   | 20.000 | ng    | -0.02     |
| 21) Naphthalene-d8          | 10.539 | 136  | 948637   | 20.000 | ng    | -0.02     |
| 39) Acenaphthene-d10        | 14.392 | 164  | 680621   | 20.000 | ng    | -0.02     |
| 64) Phenanthrene-d10        | 17.145 | 188  | 1371677  | 20.000 | ng    | -0.01     |
| 76) Chrysene-d12            | 21.386 | 240  | 1252991  | 20.000 | ng    | -0.01     |
| 86) Perylene-d12            | 24.385 | 264  | 1255099  | 20.000 | ng    | -0.02     |
| System Monitoring Compounds |        |      |          |        |       |           |
| 5) 2-Fluorophenol           | 5.340  | 112  | 231975   | 16.076 | ng    | -0.02     |
| 7) Phenol-d6                | 6.951  | 99   | 184138   | 10.153 | ng    | 0.00      |
| 23) Nitrobenzene-d5         | 8.910  | 82   | 305105   | 15.849 | ng    | -0.02     |
| 42) 2,4,6-Tribromophenol    | 15.898 | 330  | 269859   | 26.815 | ng    | 0.00      |
| 45) 2-Fluorobiphenyl        | 13.010 | 172  | 867165   | 15.072 | ng    | -0.02     |
| 79) Terphenyl-d14           | 19.768 | 244  | 1273016  | 15.034 | ng    | -0.01     |
| Target Compounds            |        |      |          |        |       |           |
| 35) Caprolactam             | 11.486 | 113  | 130629   | 28.357 | ng    | Qvalue 93 |
| -----                       |        |      |          |        |       |           |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050725\  
Data File : BM050138.D  
Acq On : 07 May 2025 17:03  
Operator : RC/JU  
Sample : Q1945-02DL 5X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
GB3WDL

Quant Time: May 07 18:00:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 28 18:09:16 2025  
Response via : Initial Calibration

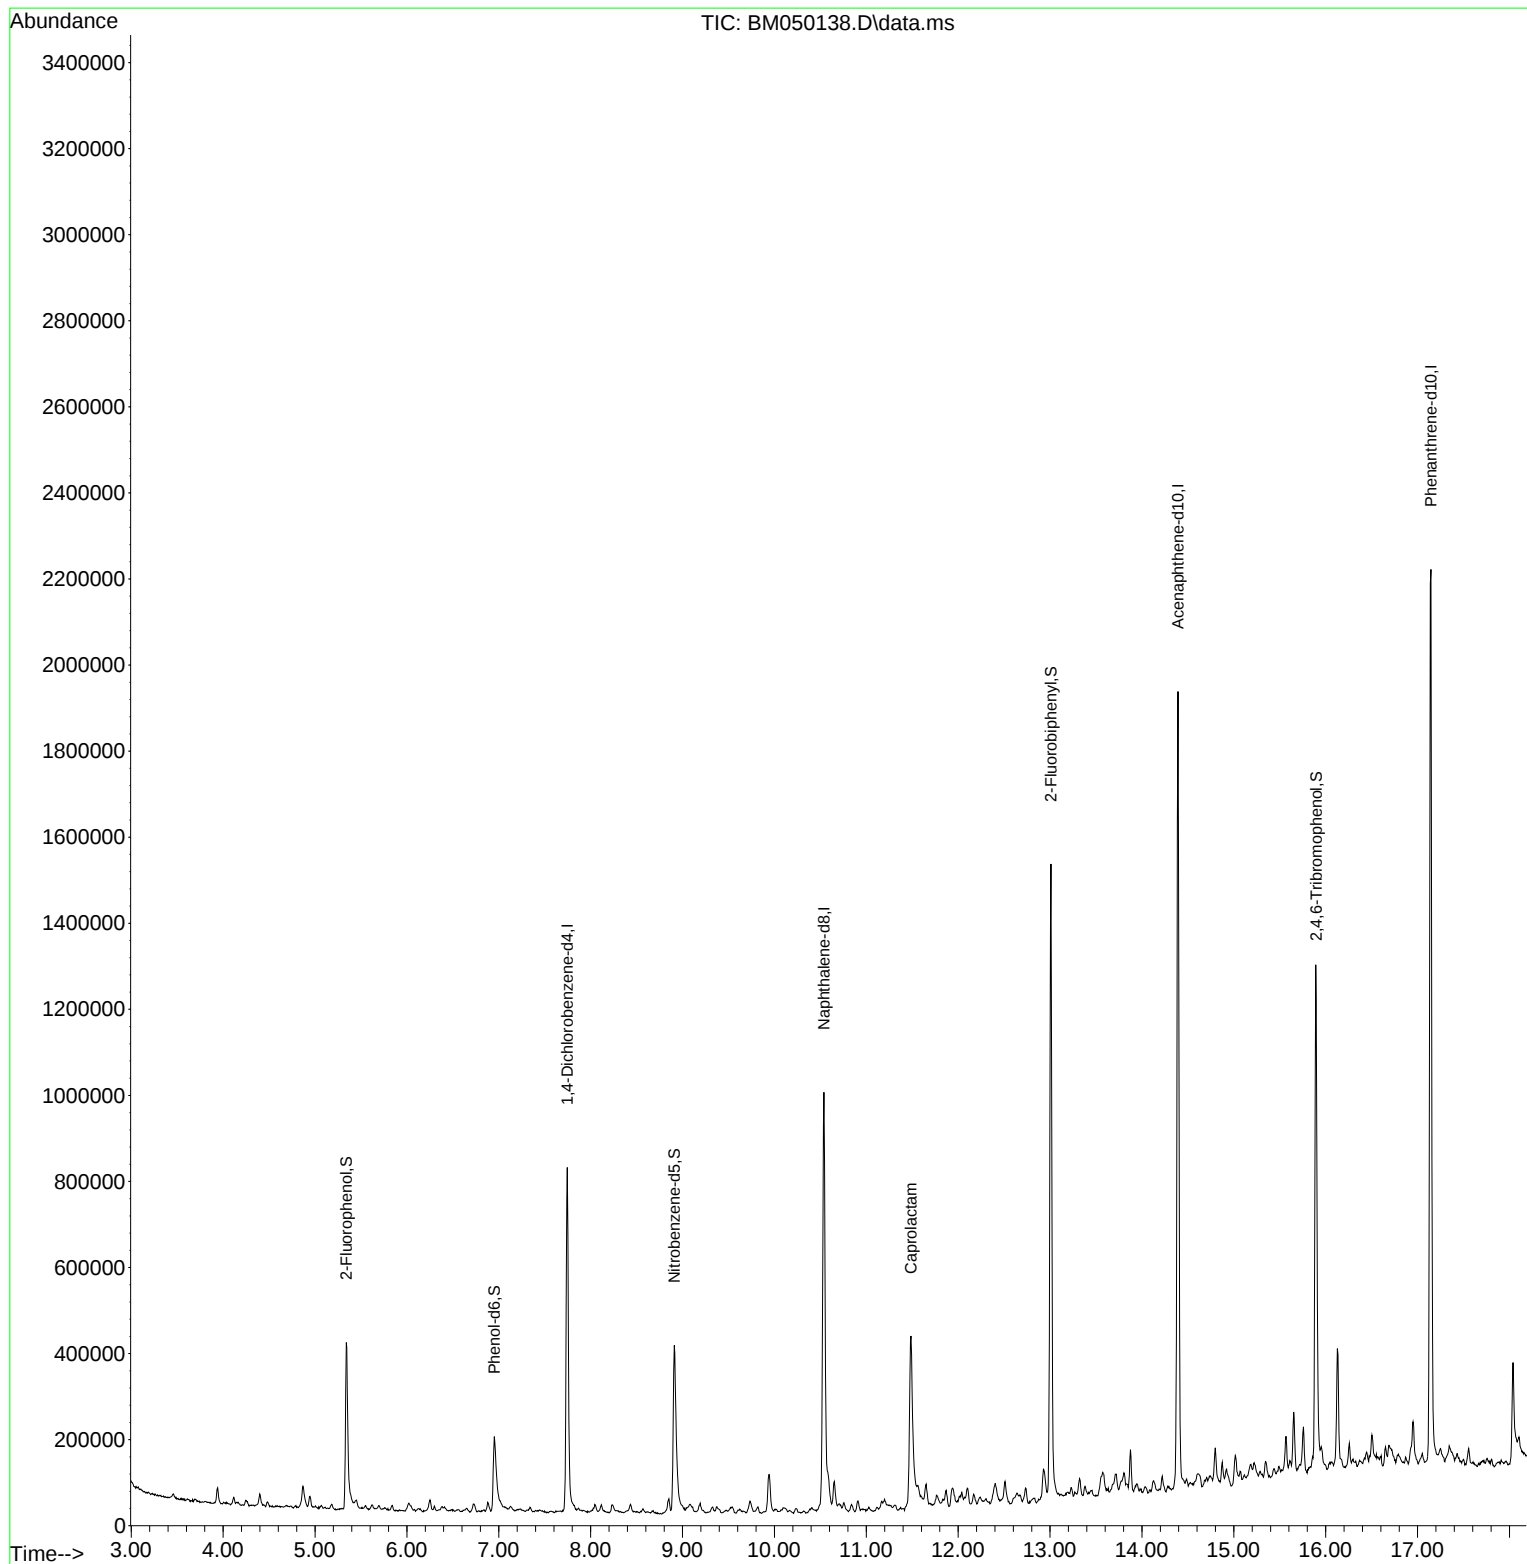

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050725\  
Data File : BM050138.D  
Acq On : 07 May 2025 17:03  
Operator : RC/JU  
Sample : Q1945-02DL 5X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
GB3WDL

Quant Time: May 07 18:00:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 28 18:09:16 2025  
Response via : Initial Calibration

