
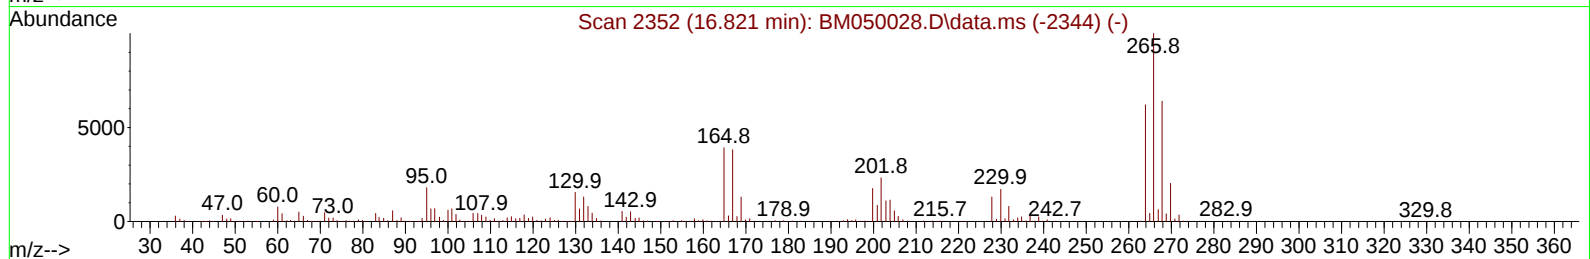
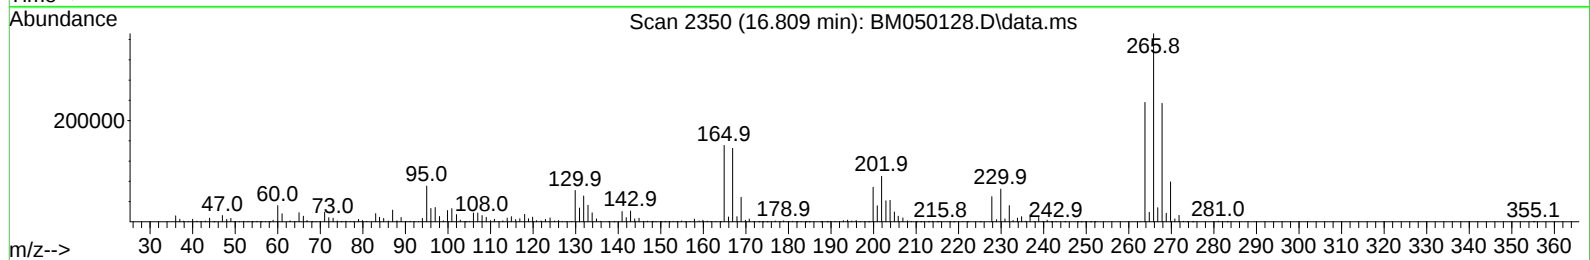


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050128.D
Acq On : 07 May 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 11:57:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

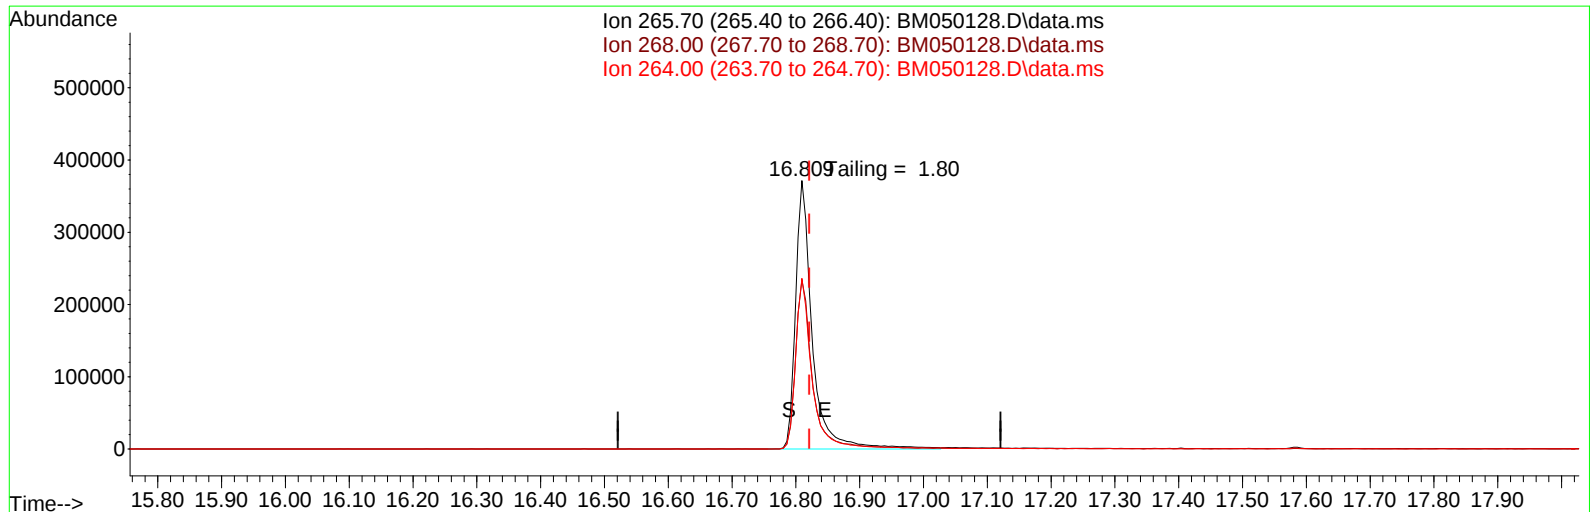

TIC: BM050128.D\data.ms

(70) Pentachlorophenol (C)




16.809min (-0.012) 191312.72 ng

response 680000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.98
264.00	62.00	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050128.D
Acq On : 07 May 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 11:57:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

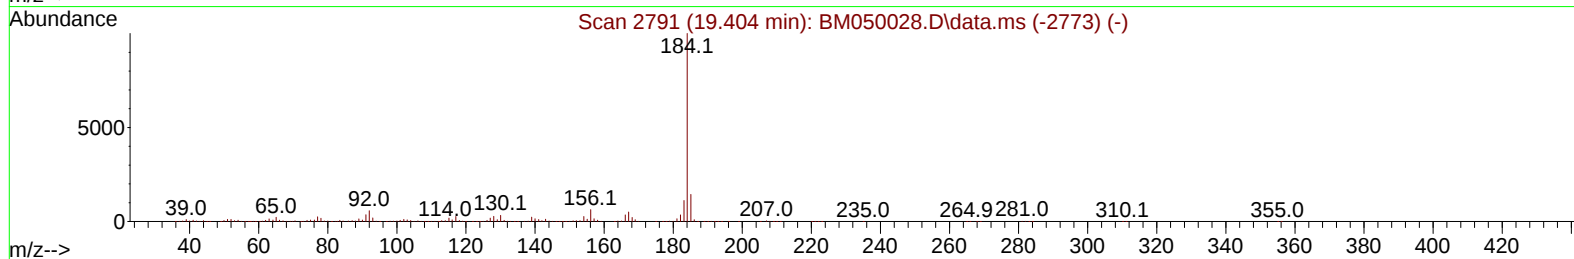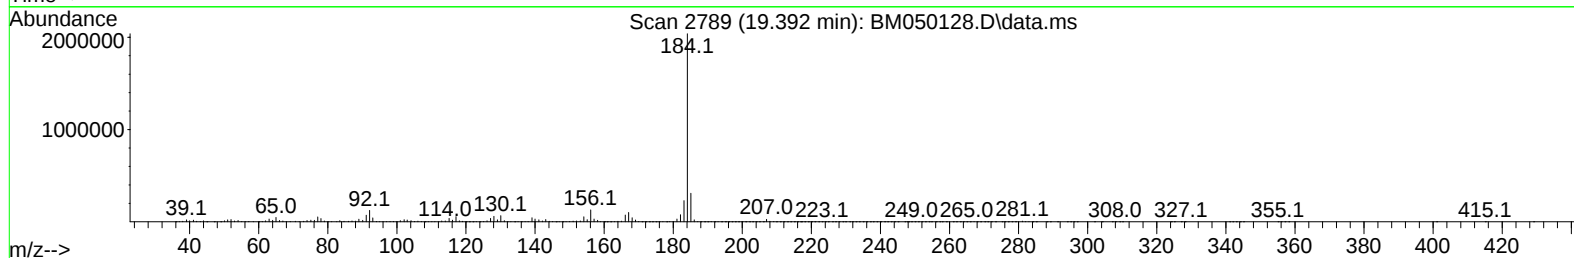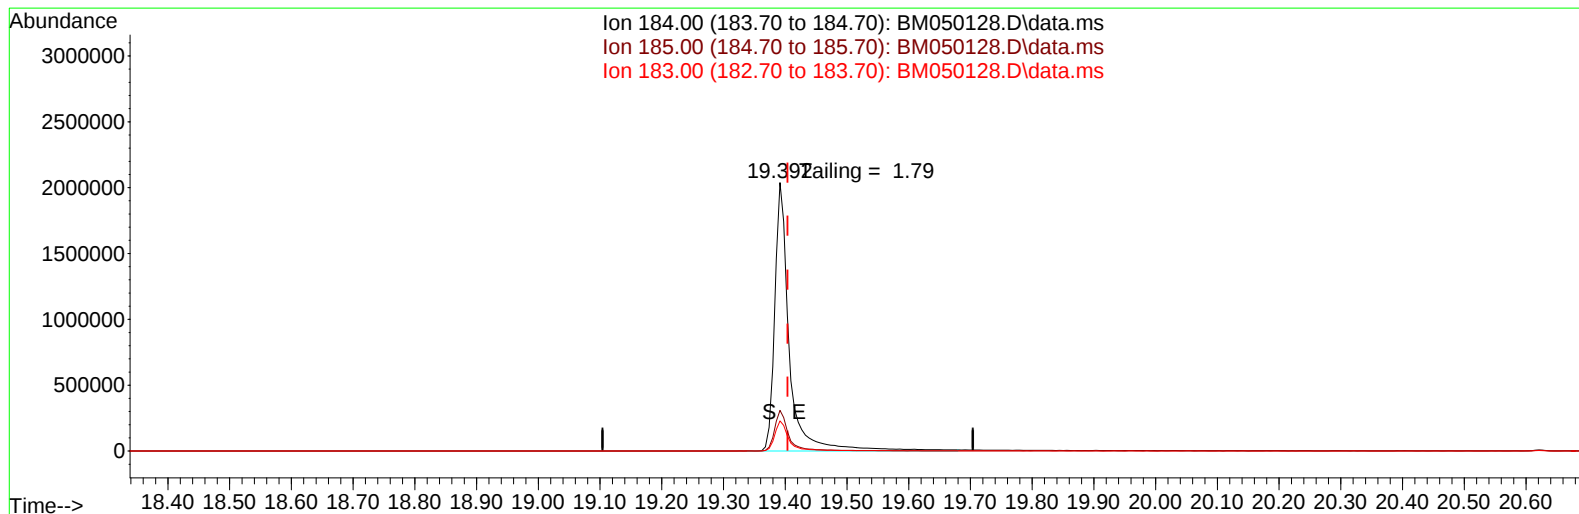

TIC: BM050128.D\data.ms

(77) Benzidine**19.392min (-0.012) 51539.94 ng****response 3372211**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.17
183.00	11.10	11.22
0.00	0.00	0.00