

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
 Data File : BM020194.D
 Acq On : 08 May 2019 14:41
 Operator : JU/SJ
 Sample : PB119288BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119288BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	414	rBV	3366165	4828957	53.42%	9.225%
2	6.957	665	675	691	rBV	3203166	5029776	55.64%	9.609%
3	7.322	729	737	750	rBV	3251687	5317156	58.82%	10.158%
4	7.787	809	816	825	rVB	577576	914899	10.12%	1.748%
5	8.104	861	870	880	rBV	2538663	4064869	44.97%	7.765%
6	8.951	1007	1014	1026	rBV	1833284	3158499	34.94%	6.034%
7	10.581	1282	1291	1302	rBV	639664	1095103	12.11%	2.092%
8	13.045	1703	1710	1720	rBV	4955142	7218985	79.86%	13.791%
9	14.427	1939	1945	1953	rBV2	917991	1432751	15.85%	2.737%
10	15.921	2192	2199	2215	rBV	3810454	5523677	61.10%	10.552%
11	17.180	2406	2413	2421	rBV2	1106394	1664581	18.41%	3.180%
12	19.804	2853	2859	2869	rBV	7224554	9039929	100.00%	17.269%
13	21.362	3119	3124	3130	rBV	1179483	1576722	17.44%	3.012%
14	23.656	3509	3514	3522	rVB	770100	1480940	16.38%	2.829%


Sum of corrected areas: 52346844

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
Data File : BM020194.D
Acq On : 08 May 2019 14:41
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119288BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

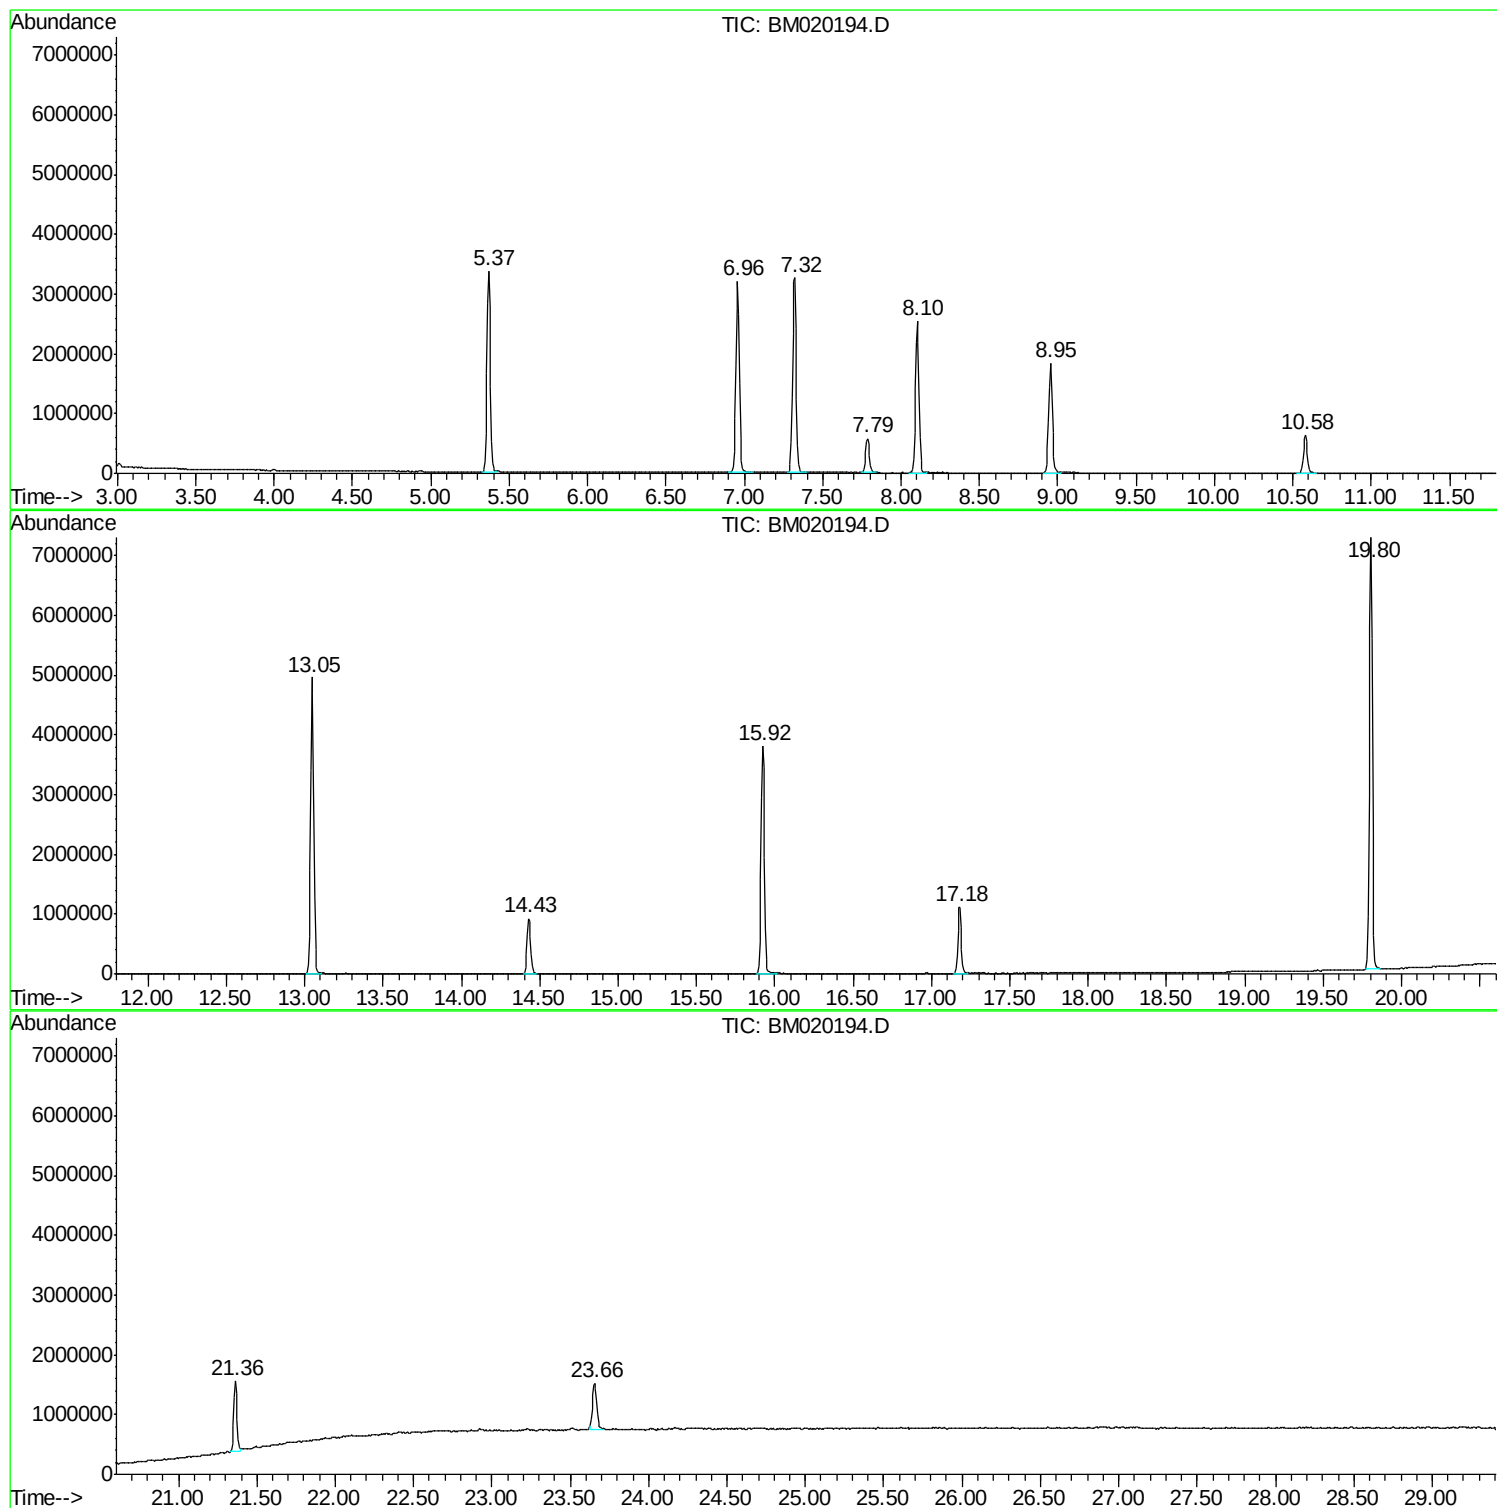

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
Data File : BM020194.D
Acq On : 08 May 2019 14:41
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119288BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	116.24 ng	5317160	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	22
3		Pvrazolo(2,3-a)pvridine, 7-methyl-	132	C8H8N2	034760-58-2	22
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22

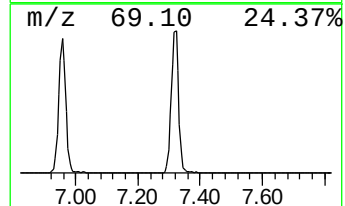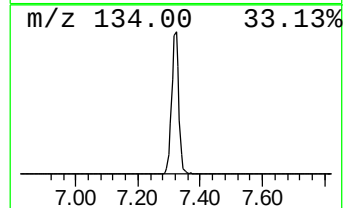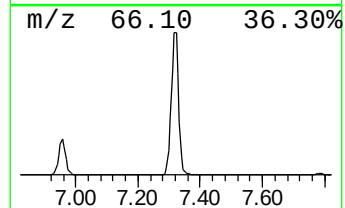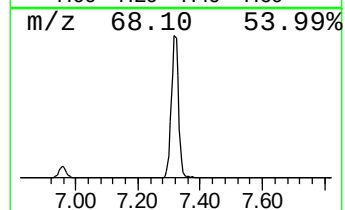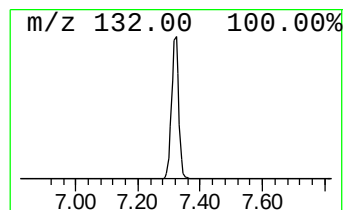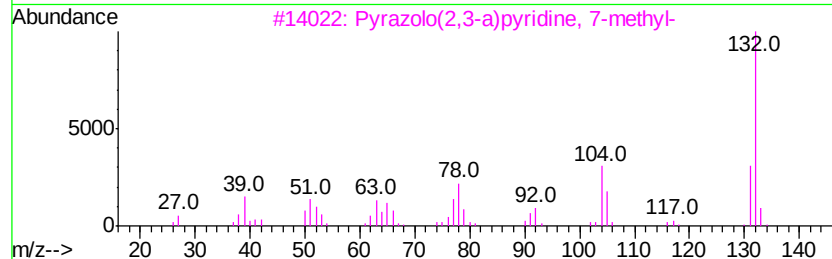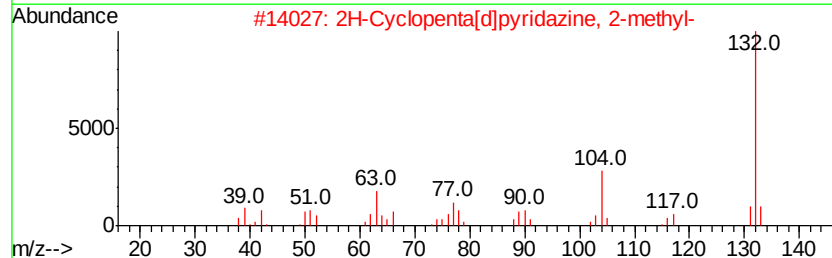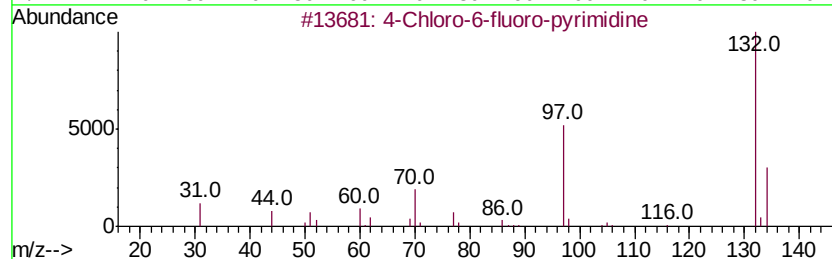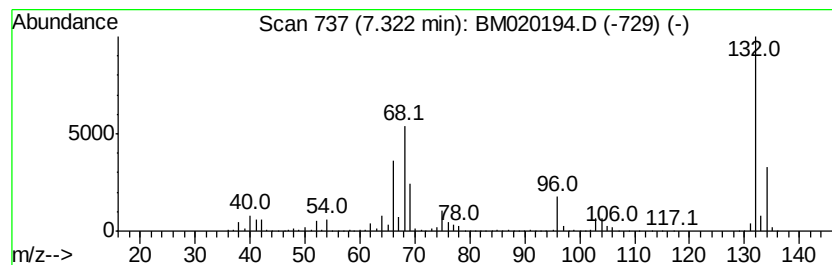

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050819\
Data File : BM020194.D
Acq On : 08 May 2019 14:41
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119288BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.32	7.32	116.2	ng	5317160	1	7.79	914899	20.0