

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
Data File : BM020197.D
Acq On : 08 May 2019 16:31
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119532BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	415	rBV	3312910	4727969	51.71%	9.111%
2	6.957	667	675	686	rBV	3061225	4938972	54.02%	9.518%
3	7.316	729	736	748	rBV	3306268	5228536	57.18%	10.076%
4	7.787	806	816	828	rBV	551835	910505	9.96%	1.755%
5	8.104	862	870	883	rBV	2443645	3973414	43.46%	7.657%
6	8.951	1005	1014	1027	rBV	1890994	3117911	34.10%	6.009%
7	10.581	1282	1291	1301	rBV	605947	1075075	11.76%	2.072%
8	13.045	1703	1710	1723	rBV	4909619	7109797	77.76%	13.701%
9	14.427	1938	1945	1958	rBV2	934116	1423175	15.57%	2.743%
10	15.921	2192	2199	2214	rBV	3816885	5430640	59.39%	10.465%
11	17.174	2407	2412	2421	rBV2	1104228	1634377	17.88%	3.150%
12	19.803	2853	2859	2869	rBV	7405780	9143353	100.00%	17.620%
13	21.362	3119	3124	3129	rBV	1234098	1617853	17.69%	3.118%
14	23.650	3508	3513	3522	rVB	772933	1559506	17.06%	3.005%


Sum of corrected areas: 51891083

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
Data File : BM020197.D
Acq On : 08 May 2019 16:31
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119532BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

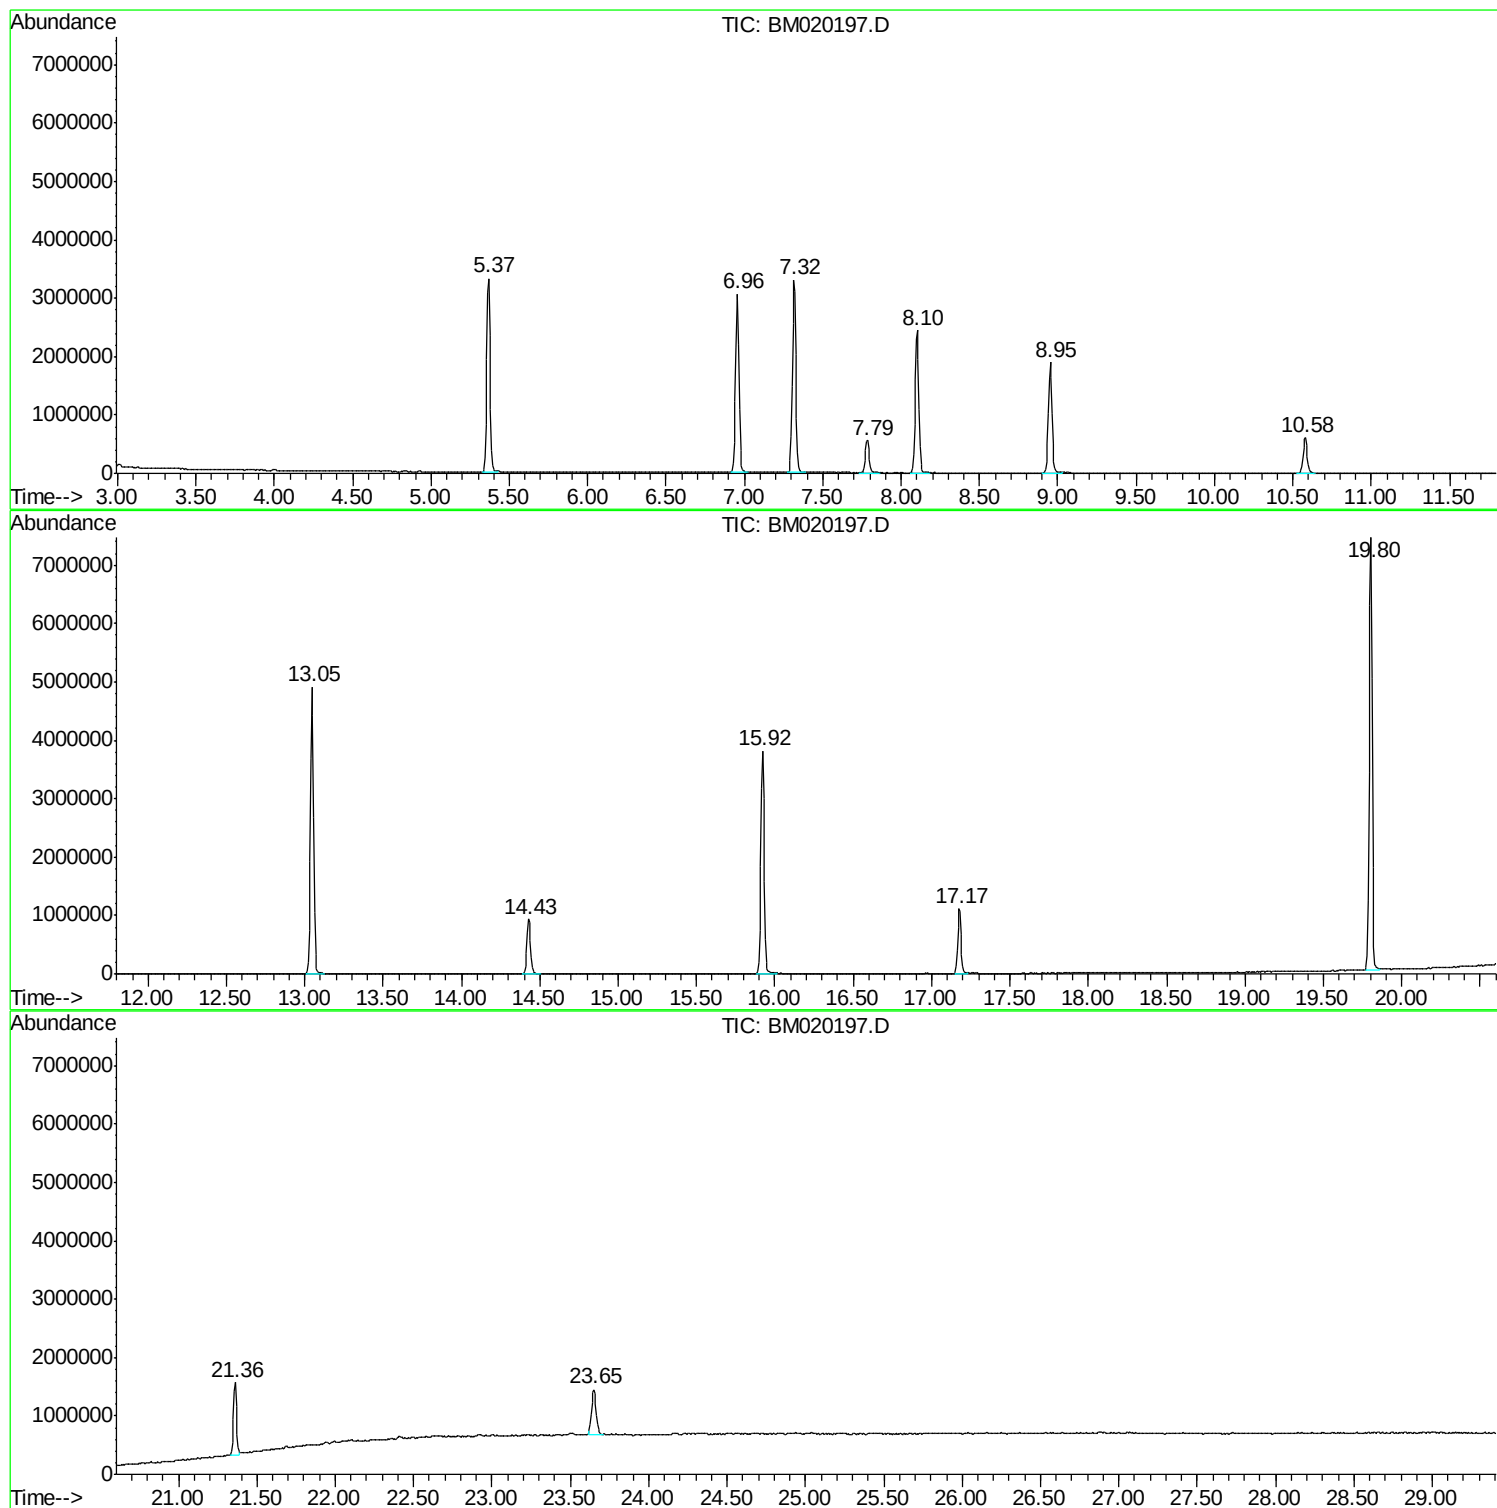

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
Data File : BM020197.D
Acq On : 08 May 2019 16:31
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119532BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	114.85 ng	5228540	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	10
5		Xenon	132	Xe	007440-63-3	9

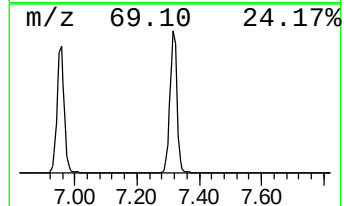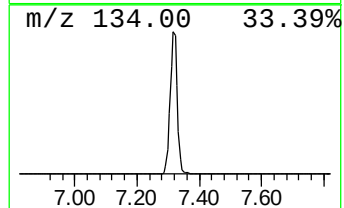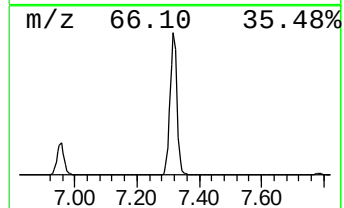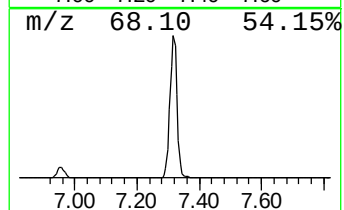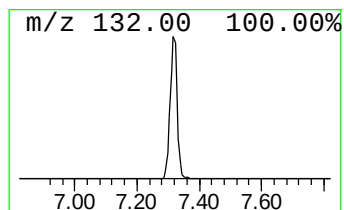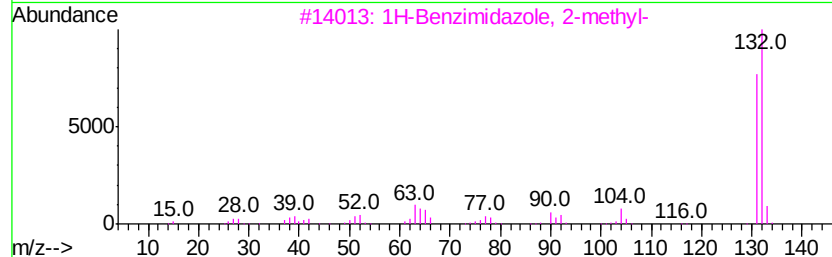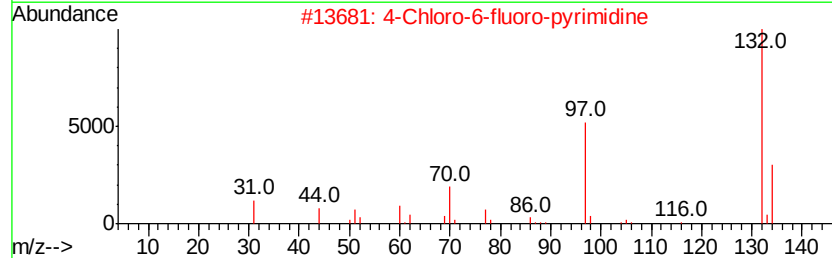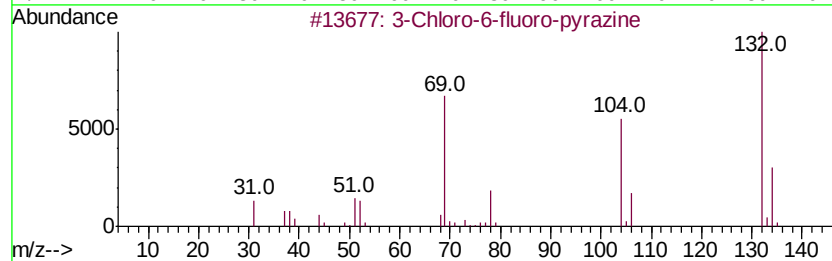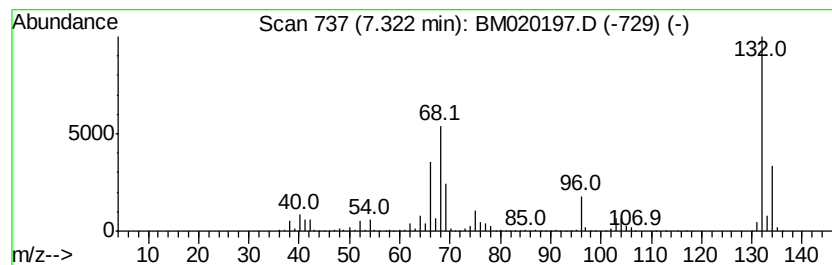

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050819\
Data File : BM020197.D
Acq On : 08 May 2019 16:31
Operator : JU/SJ
Sample : PB119288BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119532BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.32	7.32	114.8	ng	5228540	1	7.79	910505	20.0