


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050819\
 Data File : BM020191.D
 Acq On : 08 May 2019 12:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

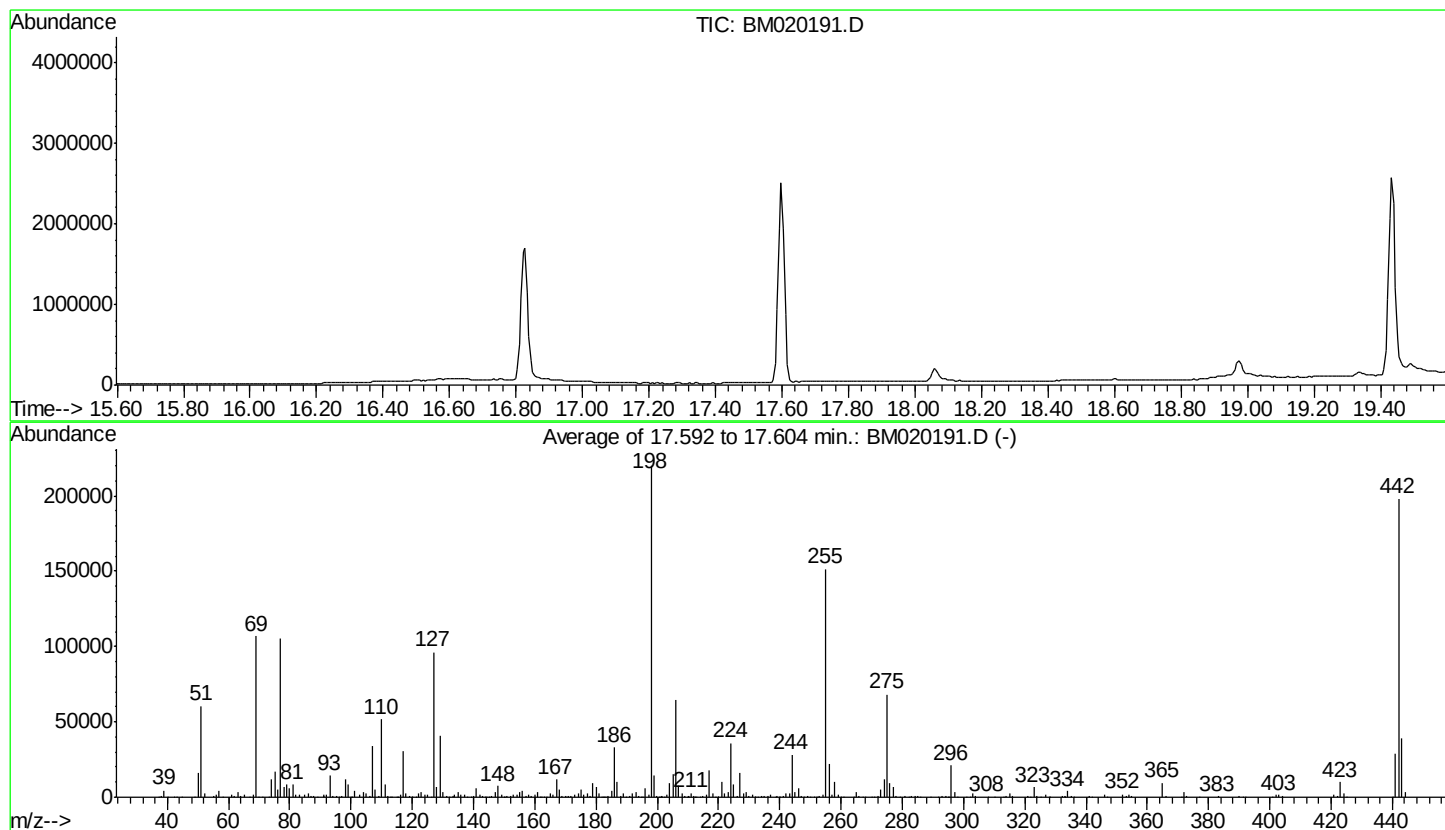

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	60568	PASS
68	69	0.00	2	1.7	1820	PASS
69	198	0.00	100	48.6	106927	PASS
70	69	0.00	2	0.4	378	PASS
127	198	10	80	43.6	96024	PASS
197	198	0.00	2	0.7	1510	PASS
198	198	100	100	100.0	220053	PASS
199	198	5	9	6.6	14535	PASS
275	198	10	60	31.1	68370	PASS
365	198	1	100	4.3	9412	PASS
441	198	0.01	100	13.0	28696	PASS
442	198	50	100	90.1	198229	PASS
443	442	15	24	19.8	39248	PASS