

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050823\
 Data File : BM039880.D
 Acq On : 08 May 2023 22:36
 Operator : CG/JU
 Sample : 02620-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFZD9

Quant Time: May 09 02:37:09 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 02:35:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.783	152	2686	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.578	136	10302	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.432	164	5968	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.187	188	13421	0.400	ng/ul	-0.01
17) Chrysene-d12	21.398	240	10047	0.400	ng/ul	0.00
23) Perylene-d12	23.736	264	9317	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.172	96	16126	4.074	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	4646	0.352	ng/ul	0.02
18) Fluoranthene-d10	19.229	212	13848	0.512	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.210	88	2569	0.626	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050823\
Data File : BM039880.D
Acq On : 08 May 2023 22:36
Operator : CG/JU
Sample : 02620-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFZD9

Quant Time: May 09 02:37:09 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 02:35:28 2023
Response via : Initial Calibration

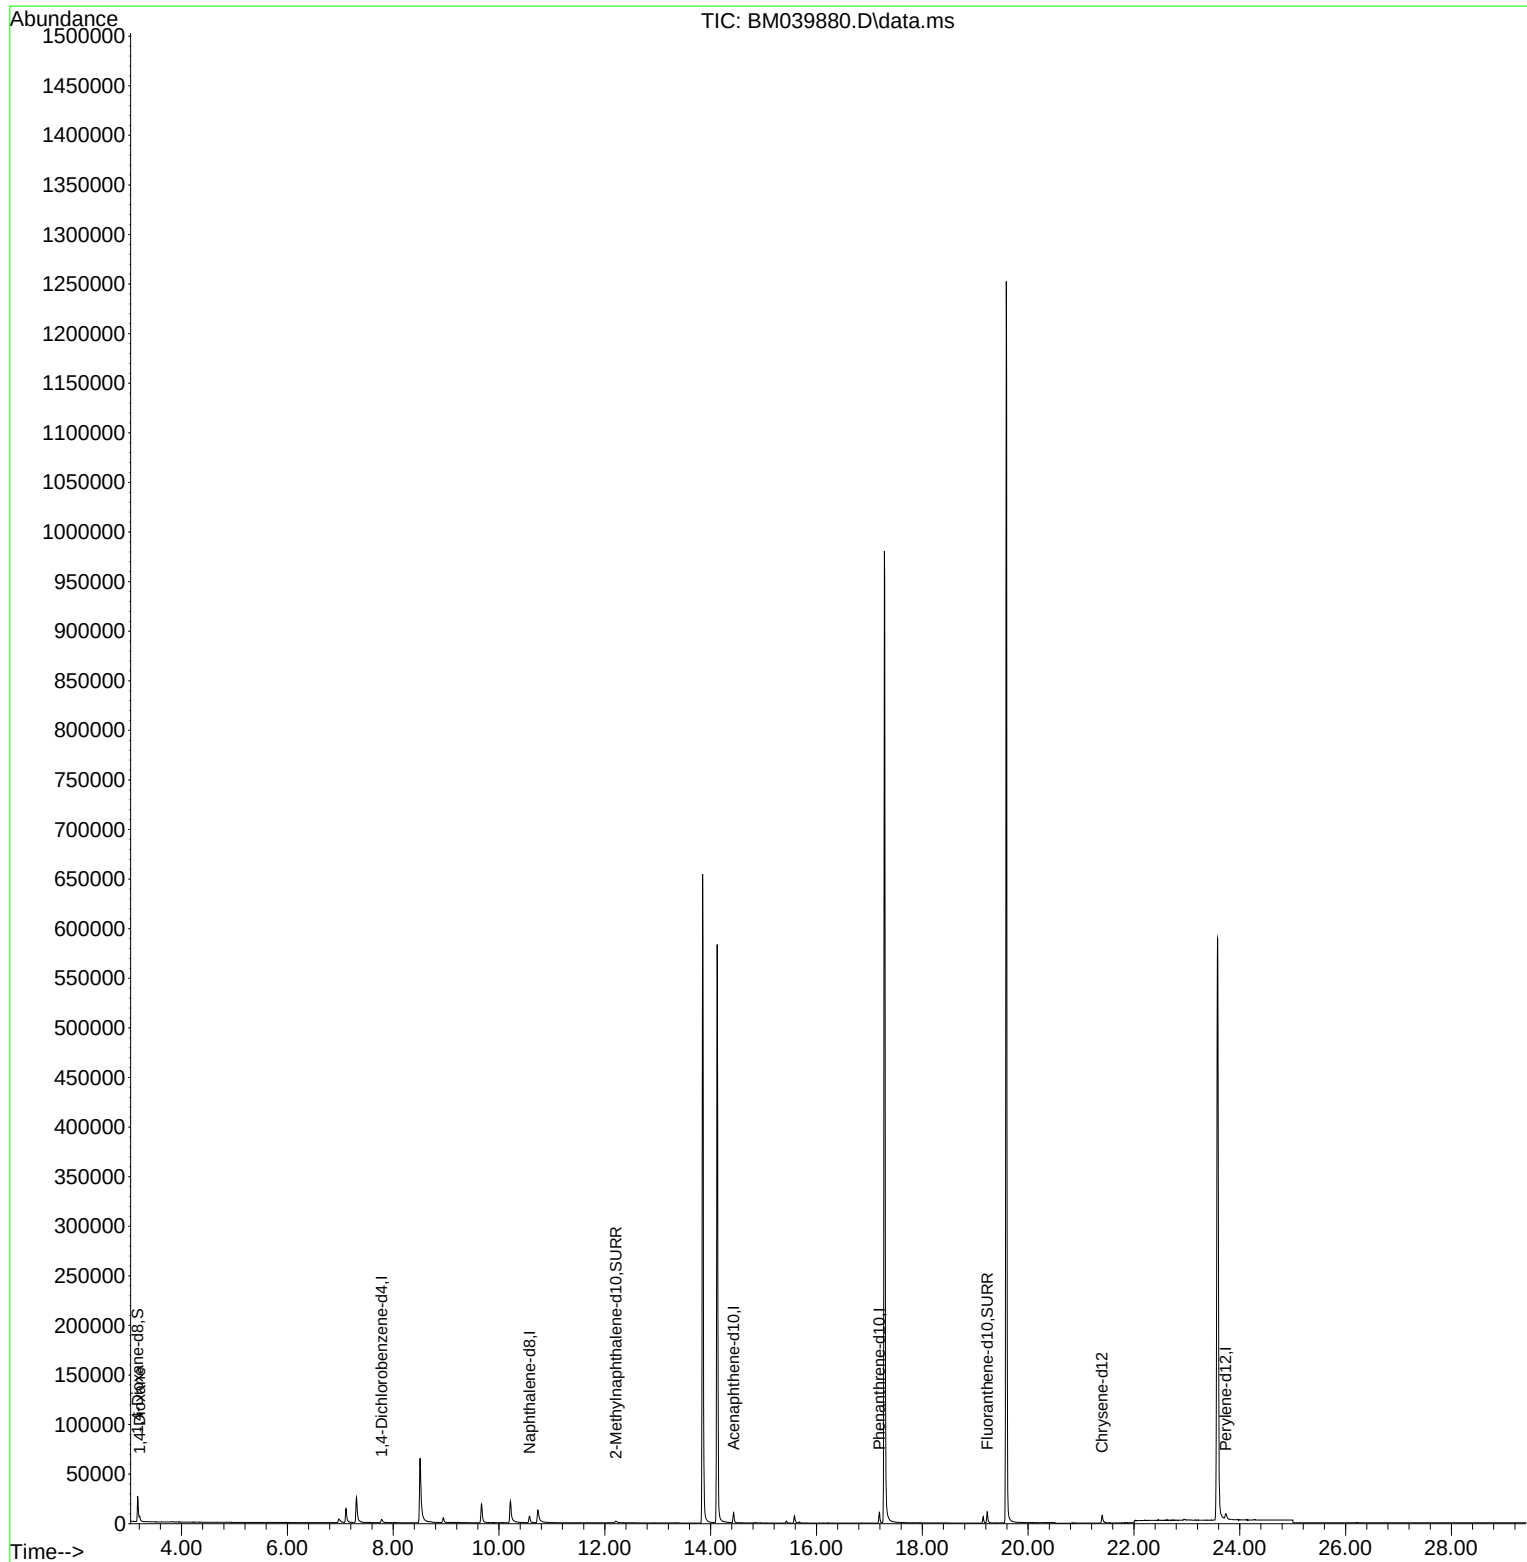

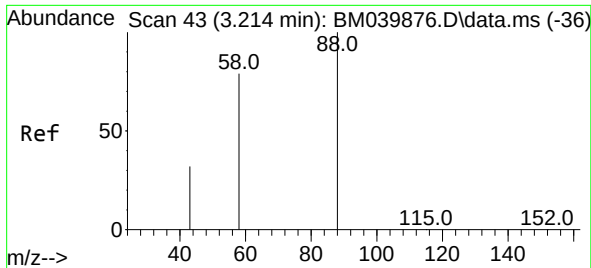

#2
 1,4-Dioxane
 Concen: 0.626 ng/ul
 RT: 3.210 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BM039880.D
 Acq: 08 May 2023 22:36

Instrument :
 BNA_M
 ClientSampleId :
 BFZD9

Tgt Ion: 88 Resp: 2569

Ion	Ratio	Lower	Upper
88	100		
43	38.1	102.6	153.8#
58	54.9	40.6	61.0

