

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
 Data File : BM050140.D
 Acq On : 08 May 2025 10:41
 Operator : RC/JU
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDCCC040

Quant Time: May 08 12:03:45 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 08 12:03:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	370324	20.000	ng	0.00
21) Naphthalene-d8	10.534	136	1368857	20.000	ng	0.00
39) Acenaphthene-d10	14.392	164	879874	20.000	ng	0.00
64) Phenanthrene-d10	17.139	188	1654930	20.000	ng	0.00
76) Chrysene-d12	21.386	240	1237713	20.000	ng	0.00
86) Perylene-d12	24.380	264	1026252	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	1642415	77.661	ng	0.00
7) Phenol-d6	6.934	99	2111558	79.439	ng	0.00
23) Nitrobenzene-d5	8.904	82	2134237	76.829	ng	0.00
42) 2,4,6-Tribromophenol	15.892	330	1005758	77.306	ng	0.00
45) 2-Fluorobiphenyl	13.010	172	5771543	77.598	ng	0.00
79) Terphenyl-d14	19.768	244	7699588	92.052	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.234	88	335516	37.001	ng	99
3) Pyridine	3.634	79	904531	38.824	ng	96
4) n-Nitrosodimethylamine	3.546	42	359788	39.374	ng	98
6) Aniline	7.075	93	1314457	39.162	ng	99
8) 2-Chlorophenol	7.316	128	887499	38.813	ng	98
9) Benzaldehyde	6.887	77	690756	38.833	ng	98
10) Phenol	6.963	94	1065717	39.605	ng	98
11) bis(2-Chloroethyl)ether	7.169	93	863881	38.447	ng	99
12) 1,3-Dichlorobenzene	7.634	146	1038233	37.588	ng	99
13) 1,4-Dichlorobenzene	7.775	146	1040843	37.509	ng	99
14) 1,2-Dichlorobenzene	8.093	146	1005092	37.497	ng	99
15) Benzyl Alcohol	7.993	79	751209	40.752	ng	98
16) 2,2'-oxybis(1-Chloropr...	8.263	45	1076308	39.406	ng	99
17) 2-Methylphenol	8.204	107	693712	39.133	ng	98
18) Hexachloroethane	8.816	117	369976	37.507	ng	100
19) n-Nitroso-di-n-propyla...	8.551	70	674550	39.568	ng	100
20) 3+4-Methylphenols	8.534	107	947336	39.573	ng	98
22) Acetophenone	8.569	105	1298428	38.153	ng	98
24) Nitrobenzene	8.945	77	922534	38.408	ng	100
25) Isophorone	9.475	82	1815169	38.333	ng	100
26) 2-Nitrophenol	9.657	139	500100	40.755	ng	99
27) 2,4-Dimethylphenol	9.728	122	800845	39.354	ng	100
28) bis(2-Chloroethoxy)met...	9.951	93	1125441	38.454	ng	100
29) 2,4-Dichlorophenol	10.210	162	882444	38.708	ng	99
30) 1,2,4-Trichlorobenzene	10.404	180	1043351	37.563	ng	100
31) Naphthalene	10.586	128	2598647	37.486	ng	100
32) Benzoic acid	9.916	122	496992	38.186	ng	98
33) 4-Chloroaniline	10.704	127	1093472	38.483	ng	99
34) Hexachlorobutadiene	10.869	225	666762	37.817	ng	99
35) Caprolactam	11.516	113	246749	37.121	ng	94
36) 4-Chloro-3-methylphenol	11.857	107	803329	38.140	ng	98
37) 2-Methylnaphthalene	12.204	142	1761314	37.896	ng	100
38) 1-Methylnaphthalene	12.422	142	1840027	37.410	ng	100
40) 1,2,4,5-Tetrachloroben...	12.580	216	1207652	39.649	ng	100
41) Hexachlorocyclopentadiene	12.551	237	692945	37.227	ng	100
43) 2,4,6-Trichlorophenol	12.833	196	781494	40.452	ng	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
 Data File : BM050140.D
 Acq On : 08 May 2025 10:41
 Operator : RC/JU
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDCCC040

Quant Time: May 08 12:03:45 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 08 12:03:21 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.922	196	827607	39.727	ng	99
46) 1,1'-Biphenyl	13.222	154	2502138	38.256	ng	99
47) 2-Chloronaphthalene	13.263	162	1978827	38.200	ng	99
48) 2-Nitroaniline	13.480	65	487178	40.071	ng	100
49) Acenaphthylene	14.116	152	3100974	37.967	ng	100
50) Dimethylphthalate	13.851	163	2380206	37.016	ng	99
51) 2,6-Dinitrotoluene	13.975	165	516023	38.760	ng	98
52) Acenaphthene	14.457	154	1780304	37.658	ng	99
53) 3-Nitroaniline	14.316	138	495431	38.978	ng	99
54) 2,4-Dinitrophenol	14.539	184	272567	35.437	ng	98
55) Dibenzofuran	14.792	168	2956841	37.591	ng	99
56) 4-Nitrophenol	14.669	139	319245	33.657	ng	98
57) 2,4-Dinitrotoluene	14.774	165	719782	39.126	ng	98
58) Fluorene	15.445	166	2401802	37.305	ng	99
59) 2,3,4,6-Tetrachlorophenol	15.033	232	677686	37.581	ng	99
60) Diethylphthalate	15.216	149	2205320	36.397	ng	99
61) 4-Chlorophenyl-phenyle...	15.433	204	1351541	38.219	ng	99
62) 4-Nitroaniline	15.480	138	432649	35.280	ng	99
63) Azobenzene	15.727	77	1882944	37.081	ng	99
65) 4,6-Dinitro-2-methylph...	15.545	198	400737	38.684	ng	96
66) n-Nitrosodiphenylamine	15.651	169	1995726	39.272	ng	100
67) 4-Bromophenyl-phenylether	16.327	248	793425	39.646	ng	98
68) Hexachlorobenzene	16.451	284	896115	38.846	ng	98
69) Atrazine	16.610	200	701944	38.293	ng	99
70) Pentachlorophenol	16.810	266	489963	37.733	ng	99
71) Phenanthrene	17.186	178	3506508	37.567	ng	100
72) Anthracene	17.274	178	3566867	37.761	ng	100
73) Carbazole	17.551	167	3040432	37.093	ng	99
74) Di-n-butylphthalate	18.104	149	3579619	36.672	ng	99
75) Fluoranthene	19.204	202	3923349	35.801	ng	100
77) Benzidine	19.392	184	1769429	40.247	ng	99
78) Pyrene	19.568	202	3921227	45.115	ng	100
80) Butylbenzylphthalate	20.462	149	1331850	40.913	ng	99
81) Benzo(a)anthracene	21.368	228	3251627	38.150	ng	100
82) 3,3'-Dichlorobenzidine	21.292	252	1193314	36.574	ng	100
83) Chrysene	21.427	228	2971758	37.672	ng	100
84) Bis(2-ethylhexyl)phtha...	21.280	149	1827791	37.590	ng	100
85) Di-n-octyl phthalate	22.403	149	2757430	34.387	ng	100
87) Indeno(1,2,3-cd)pyrene	27.762	276	2903047	37.964	ng	100
88) Benzo(b)fluoranthene	23.433	252	2548858	38.191	ng	100
89) Benzo(k)fluoranthene	23.497	252	2625481	38.890	ng	99
90) Benzo(a)pyrene	24.239	252	2381402	38.097	ng	99
91) Dibenzo(a,h)anthracene	27.809	278	2367754	37.985	ng	100
92) Benzo(g,h,i)perylene	28.826	276	2251454	37.727	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
Data File : BM050140.D
Acq On : 08 May 2025 10:41
Operator : RC/JU
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDCCC040

Quant Time: May 08 12:03:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration

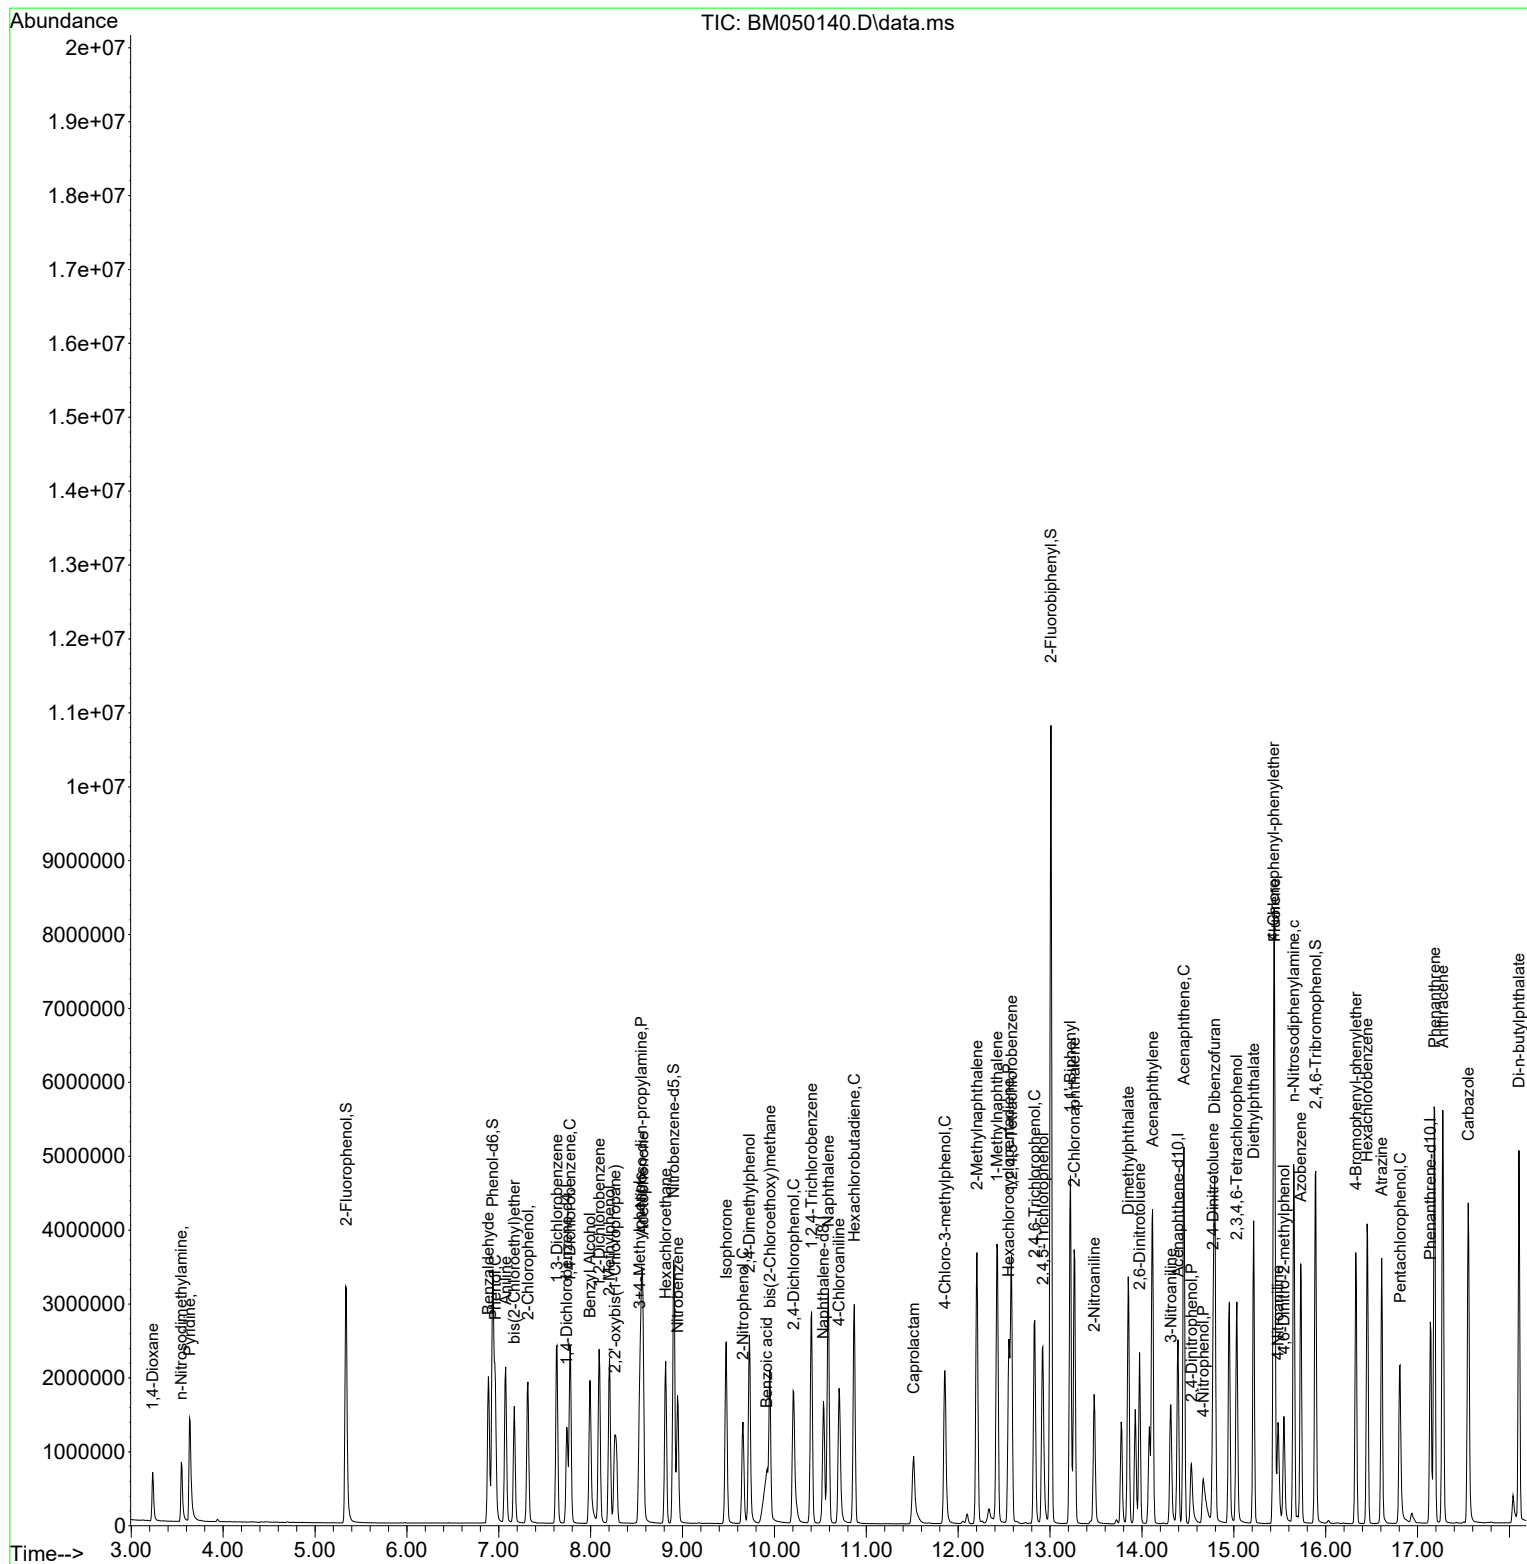

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
Data File : BM050140.D
Acq On : 08 May 2025 10:41
Operator : RC/JU
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDCCC040

Quant Time: May 08 12:03:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration

