
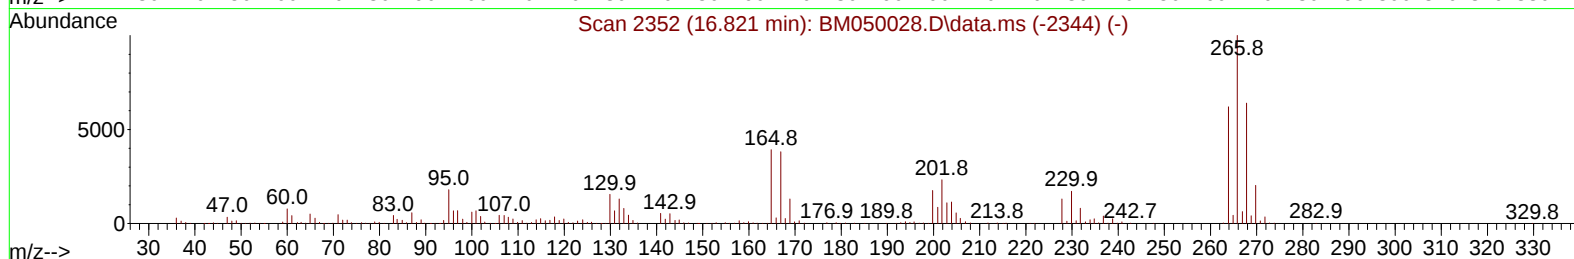
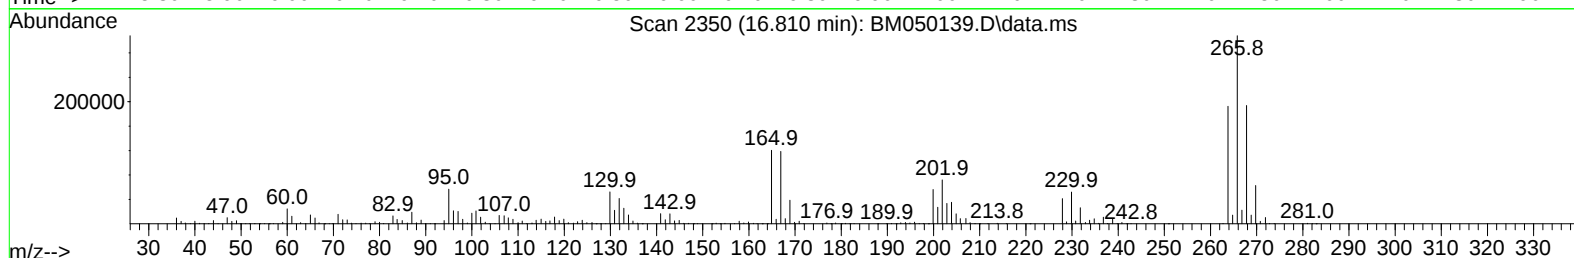


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
Data File : BM050139.D
Acq On : 08 May 2025 09:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 11:50:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

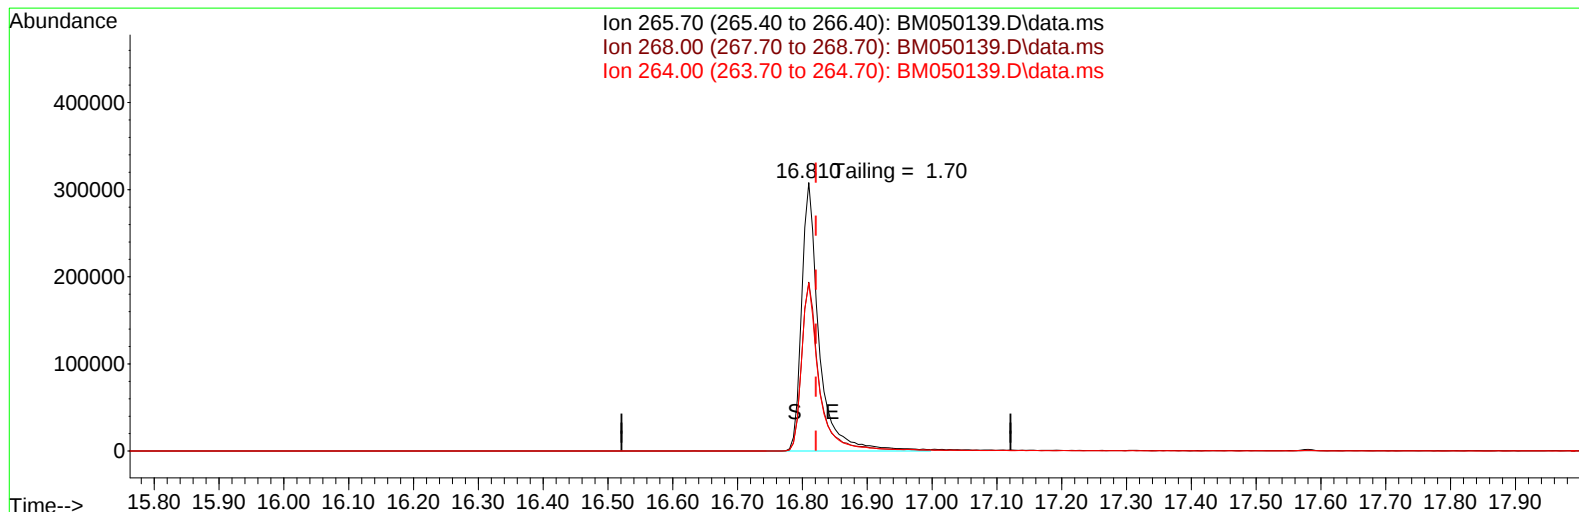

TIC: BM050139.D\data.ms

(70) Pentachlorophenol (C)




16.810min (-0.011) 902047.65 ng

response 580377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.90
264.00	62.00	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
Data File : BM050139.D
Acq On : 08 May 2025 09:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 11:50:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

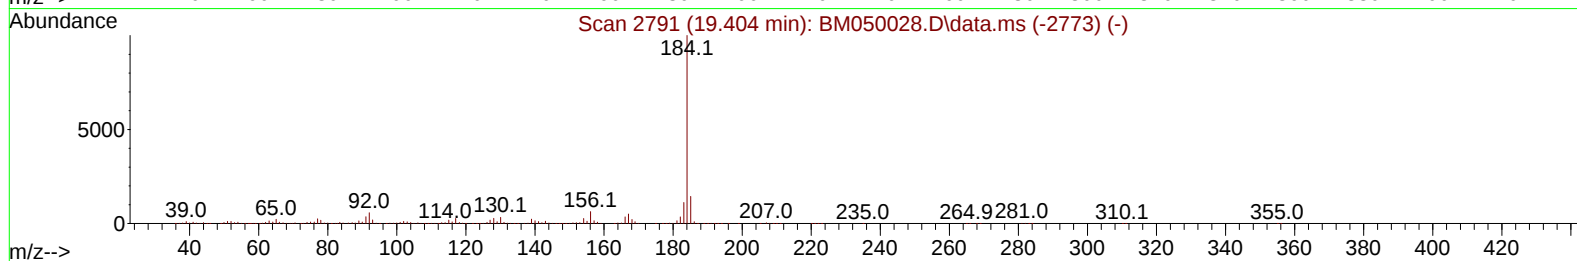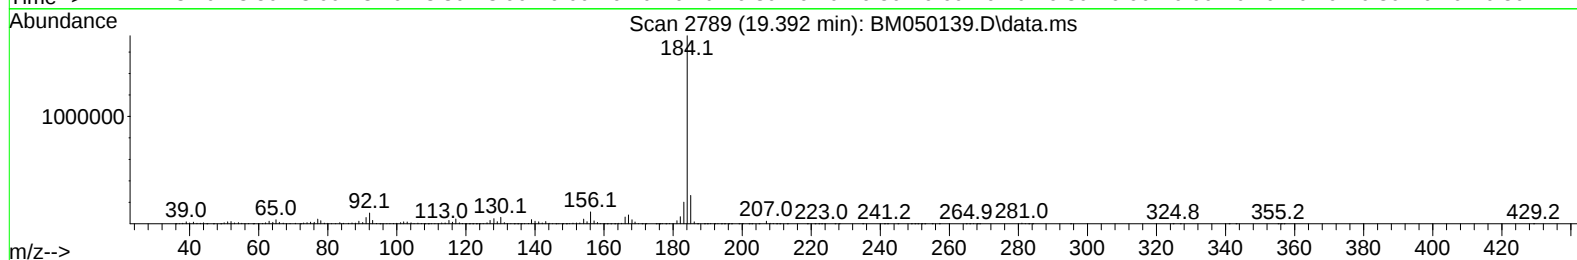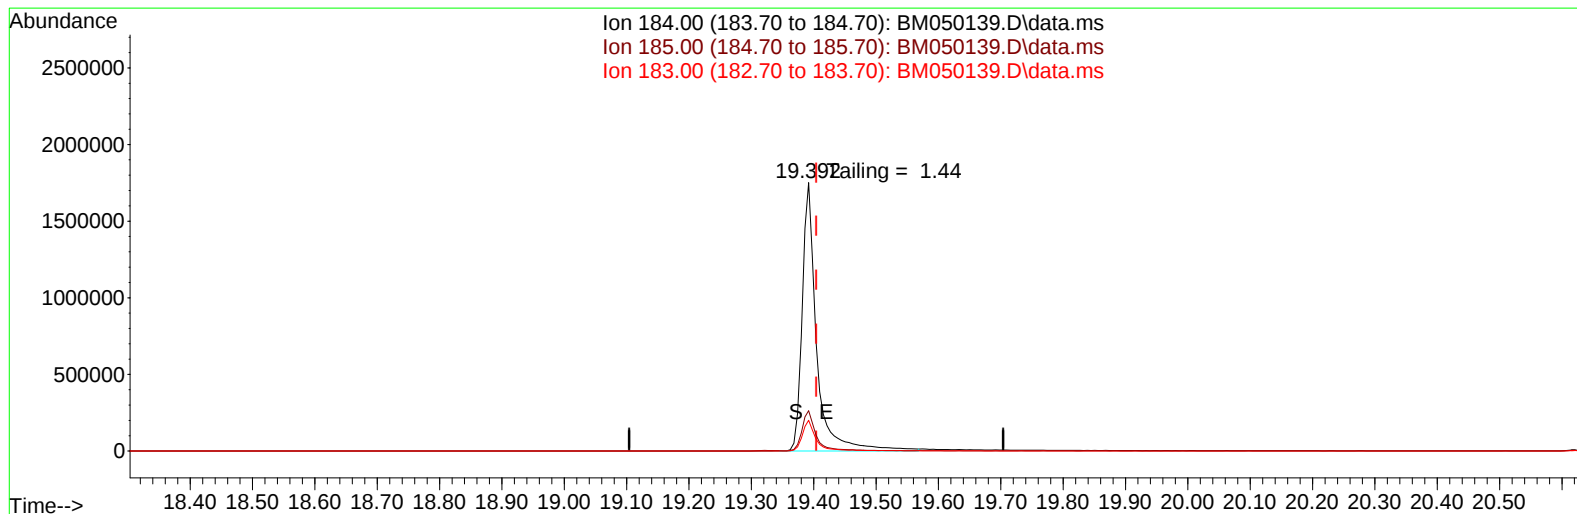

TIC: BM050139.D\data.ms

(77) Benzidine**19.392min (-0.012) 27949.85 ng****response 2854293**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.07
183.00	11.10	11.46
0.00	0.00	0.00