

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
 Data File : BM005356.D
 Acq On : 09 May 2016 12:34
 Operator : UM/SJ
 Sample : H2888-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WS2

Quant Time: May 10 04:24:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	79459	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	380363	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	234250	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	547552	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	618237	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	554405	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	6166	3.65	ng/uL	0.00
5) Phenol-d5	6.94	99	134189	18.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	81393	19.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	107876	19.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	113906	19.12	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	53719	19.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	61774	20.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	111894	19.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	151722	22.06	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	387847	20.66	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	467241	21.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	47367	13.82	ng/ul	0.00
57) Fluorene-d10	15.40	176	343963	21.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	53240	17.28	ng/ul	0.00
70) Anthracene-d10	17.26	188	536923	22.18	ng/ul	0.00
76) Pyrene-d10	19.56	212	627573	21.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	539897	22.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	91628	4.88	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
Data File : BM005356.D
Acq On : 09 May 2016 12:34
Operator : UM/SJ
Sample : H2888-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS2

Quant Time: May 10 04:24:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration

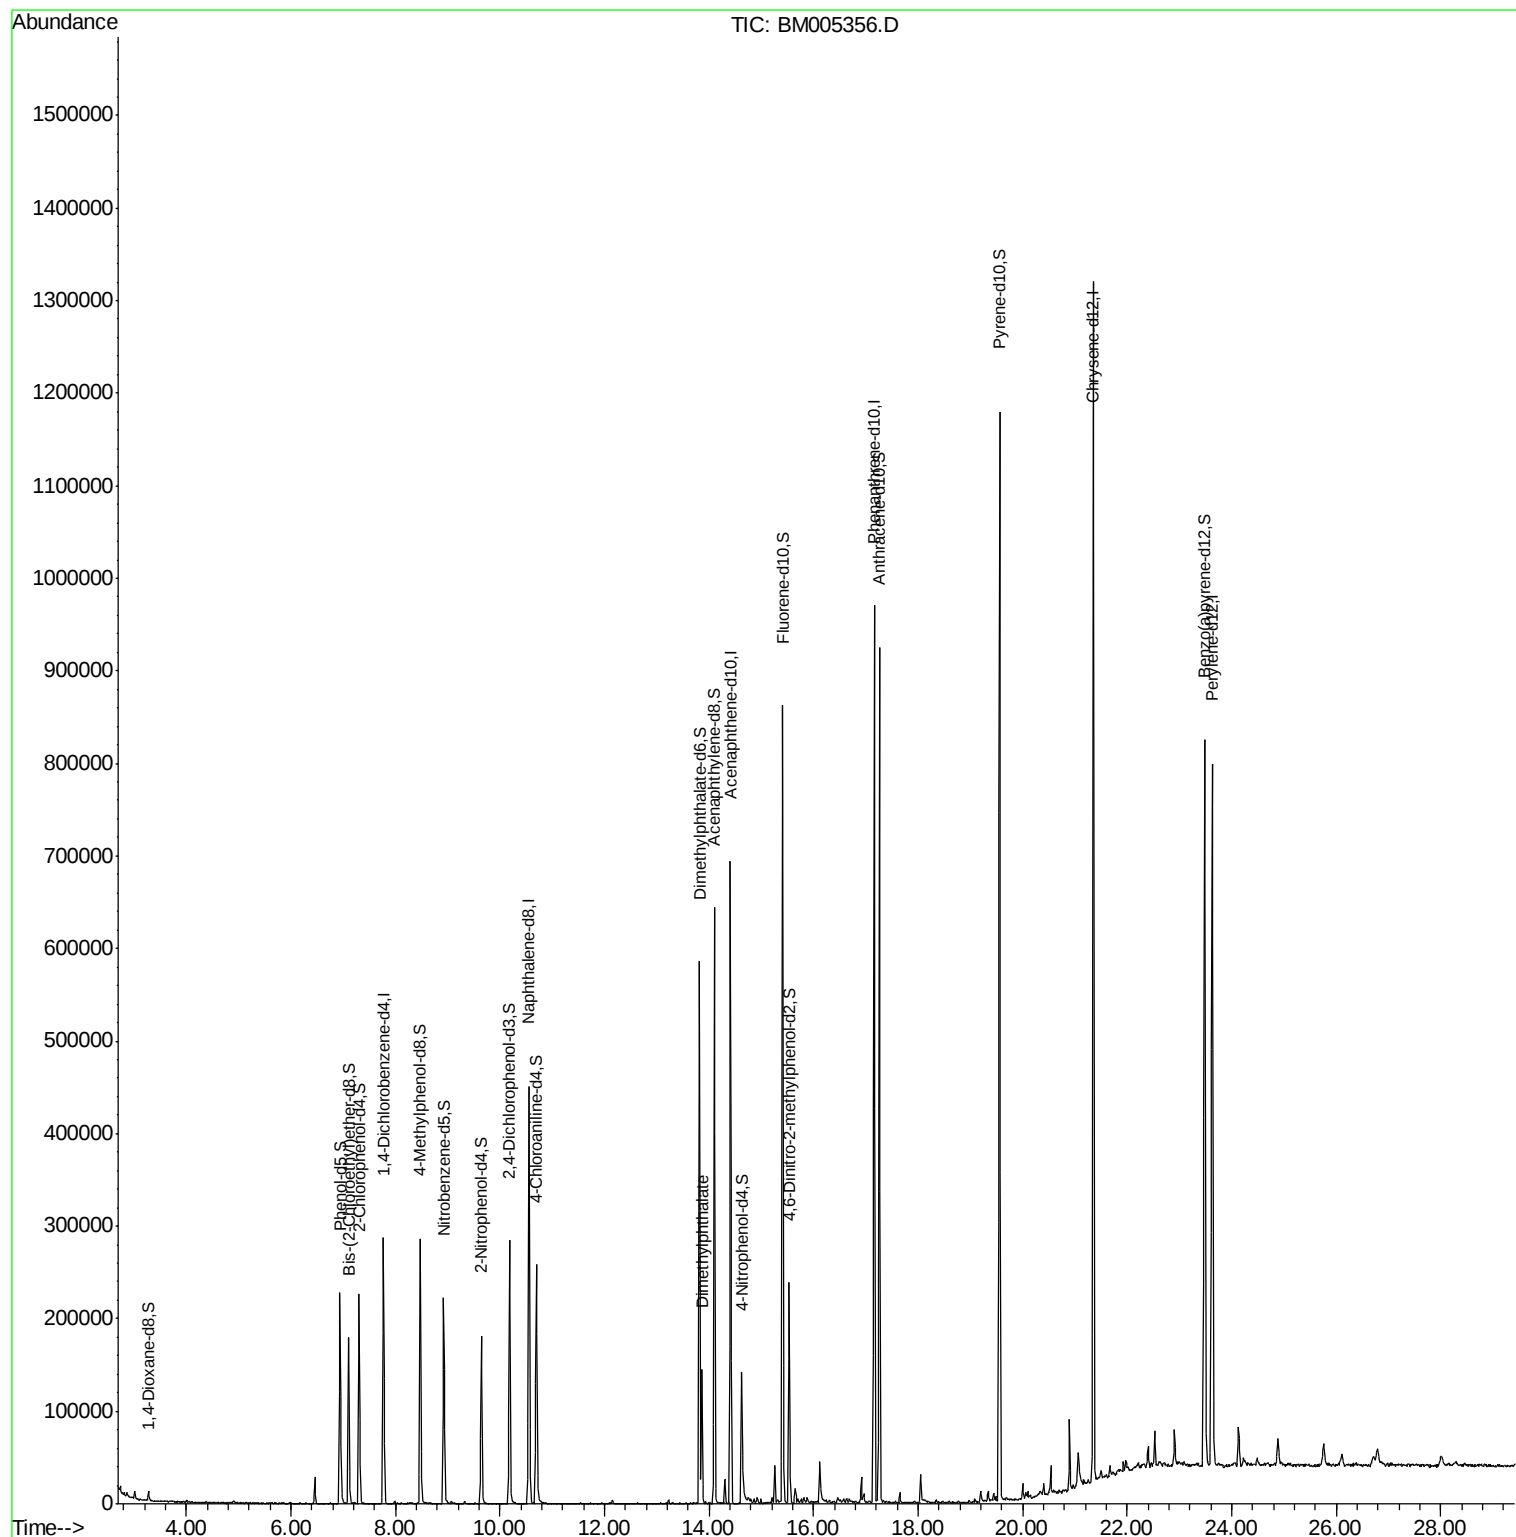

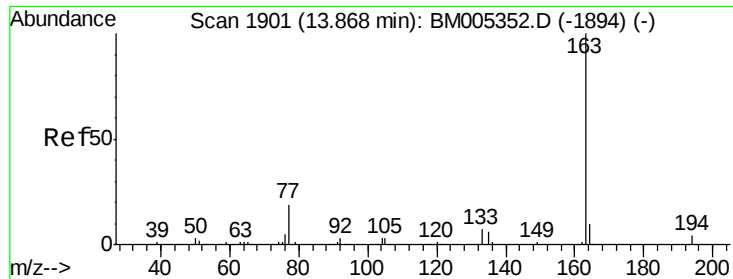

#44

Dimethylphthalate

Concen: 4.88 ng/ul

RT: 13.86 min Scan# 1900

Delta R.T. -0.01 min

Lab File: BM005356.D

Acq: 09 May 2016 12:34

Instrument :

BNA_M

ClientSampleId :

D9WS2


Tgt Ion:163 Resp: 91628

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.0 7.9 11.9

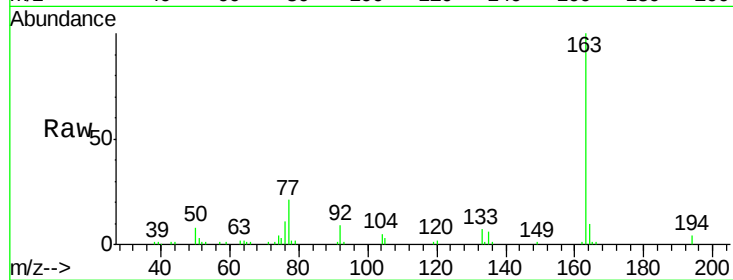

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

