

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
 Data File : BM005361.D
 Acq On : 09 May 2016 15:37
 Operator : UM/SJ
 Sample : H2888-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW2

Quant Time: May 10 04:25:32 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	87282	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	399121	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	237610	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	528332	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	474176	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	372834	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	5922	3.19	ng/uL	0.00
5) Phenol-d5	6.94	99	152438	19.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	89115	19.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	123683	20.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	72844	11.13	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	60506	21.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	69485	21.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	125419	20.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	68430	9.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	416036	21.84	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	503071	22.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	48454	13.94	ng/ul	0.00
57) Fluorene-d10	15.40	176	367397	22.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	52531	17.67	ng/ul	0.00
70) Anthracene-d10	17.26	188	542005	23.21	ng/ul	0.00
76) Pyrene-d10	19.56	212	592547	27.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	382189	23.16	ng/ul	0.00

Target Compounds


						Qvalue
14) Acetophenone	8.59	105	10255	1.06	ng/ul	96
44) Dimethylphthalate	13.86	163	86817	4.56	ng/ul	99
47) Acenaphthylene	14.13	152	29966	1.27	ng/ul	99
63) 4,6-Dinitro-2-methylphenol	15.46	198	5075	1.63	ng/ul#	51
69) Phenanthrene	17.20	178	257343	9.26	ng/ul	99
71) Anthracene	17.29	178	68457	2.47	ng/ul	99
72) Carbazole	17.56	167	25899	1.06	ng/ul	96
74) Fluoranthene	19.22	202	606552	19.71	ng/ul	98
77) Pyrene	19.59	202	567459	20.63	ng/ul	97
80) Benzo(a)anthracene	21.34	228	290304	10.64	ng/ul	97
82) Chrysene	21.39	228	283016	10.94	ng/ul	97
85) Benzo(b)fluoranthene	22.94	252	327702	15.04	ng/ul	98
86) Benzo(k)fluoranthene	22.94	252	327702	15.97	ng/ul	98
88) Benzo(a)pyrene	23.53	252	211036	10.24	ng/ul	97
89) Indeno(1,2,3-cd)pyrene	25.92	276	133639	5.94	ng/ul#	93
90) Dibenzo(a,h)anthracene	25.92	278	35866	1.91	ng/ul#	79
91) Benzo(g,h,i)perylene	26.62	276	119726	6.29	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
Data File : BM005361.D
Acq On : 09 May 2016 15:37
Operator : UM/SJ
Sample : H2888-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WW2

Quant Time: May 10 04:25:32 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration




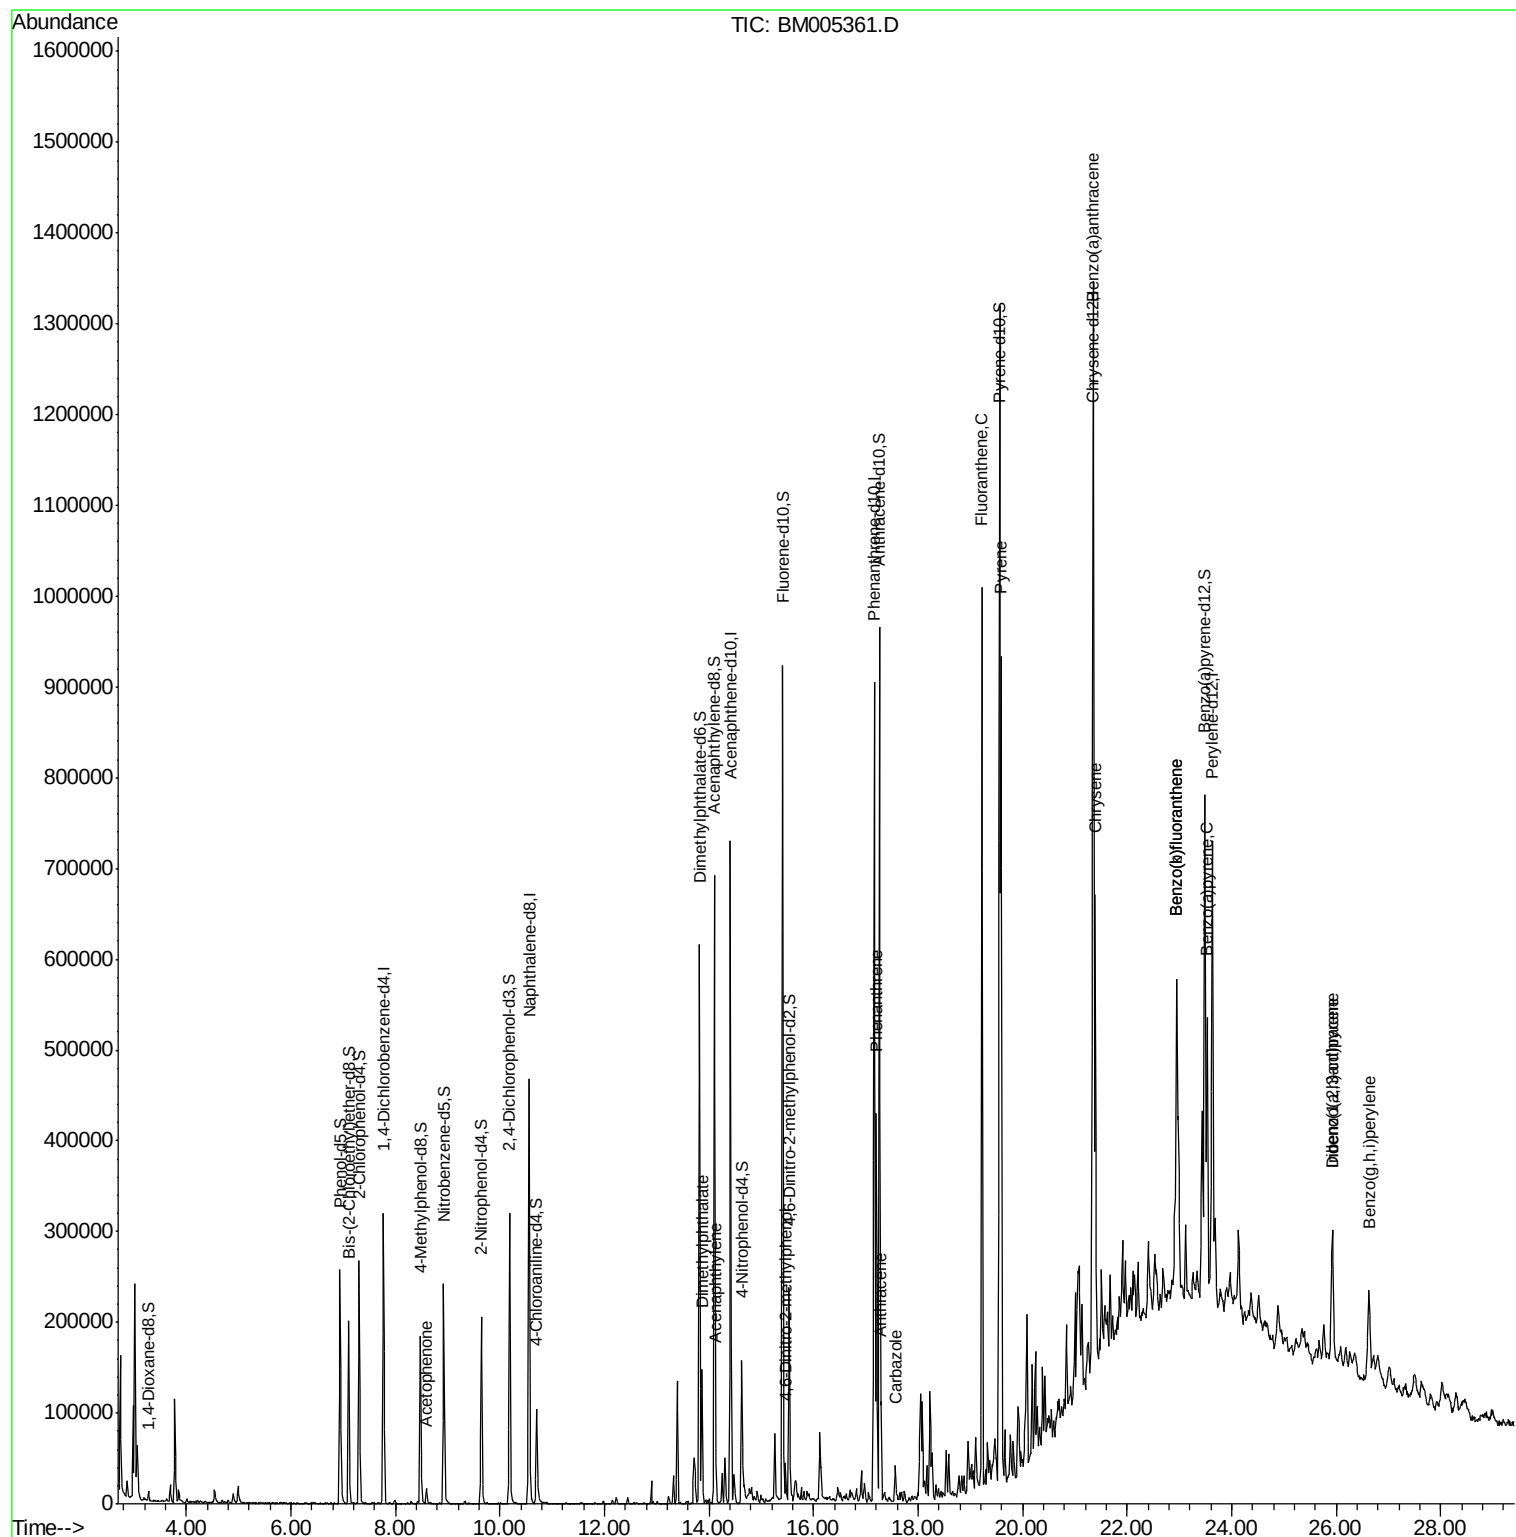


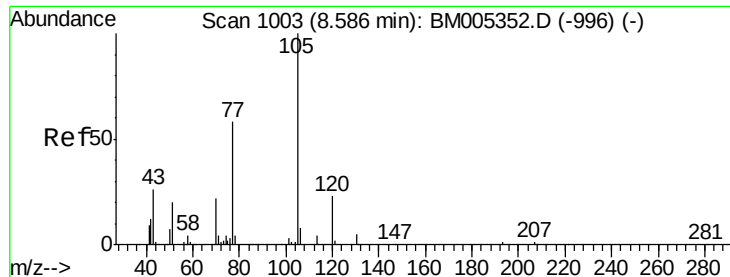

#14
Acetophenone
Concen: 1.06 ng/ul
RT: 8.59 min Scan# 1004
Delta R.T. 0.01 min
Lab File: BM005361.D
Acq: 09 May 2016 15:37




Instrument :
BNA_M
ClientSampleId :
D9WW2


Tgt Ion:105 Resp: 10255
Ion Ratio Lower Upper
105 100
77 81.2 61.2 91.8
51 26.5 21.2 31.8

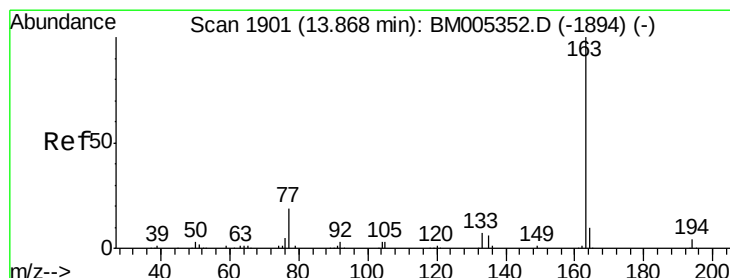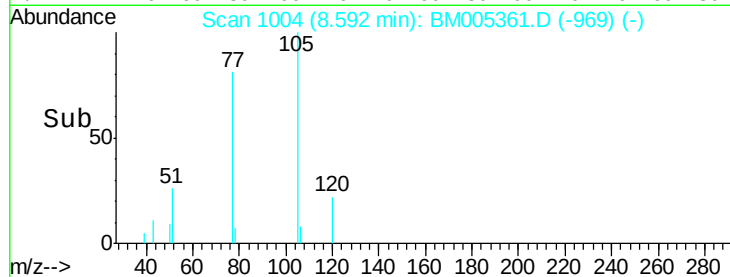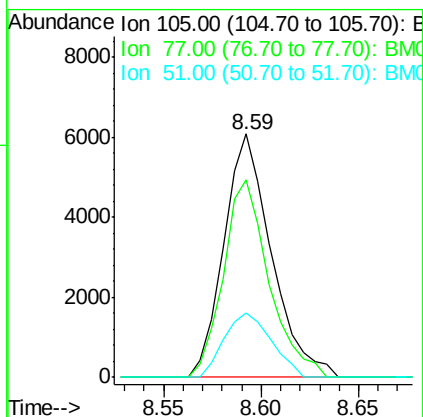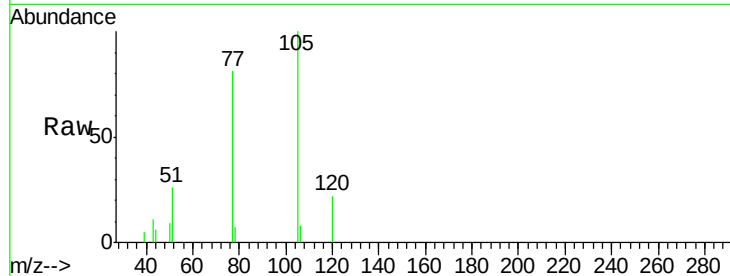

#44
Dimethylphthalate
Concen: 4.56 ng/ul
RT: 13.86 min Scan# 1900
Delta R.T. -0.01 min
Lab File: BM005361.D
Acq: 09 May 2016 15:37

Tgt Ion:163 Resp: 86817
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.0
164 9.6 7.9 11.9

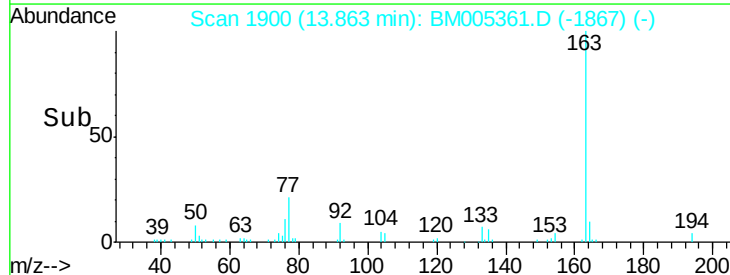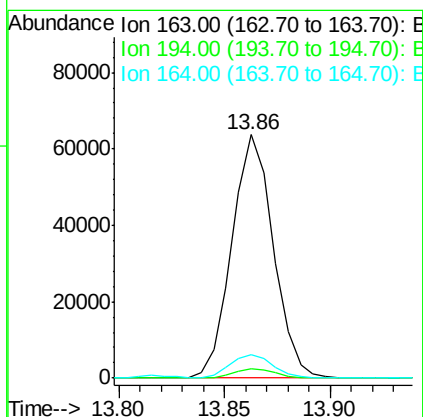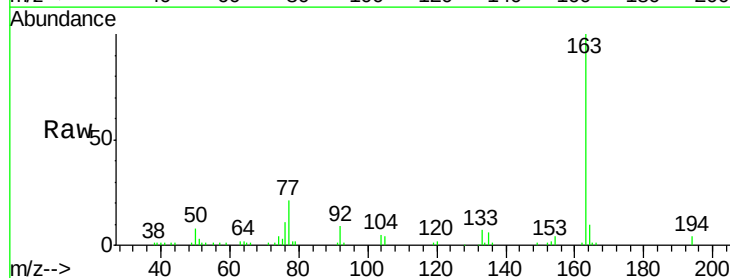

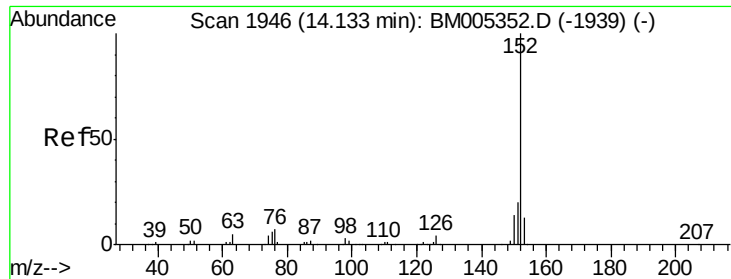

#47

Acenaphthylene

Concen: 1.27 ng/ul

RT: 14.13 min Scan# 1945

Delta R.T. -0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion:152 Resp: 29966

Ion Ratio Lower Upper

152 100

151 20.6 16.0 24.0




153 12.3 10.3 15.5



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

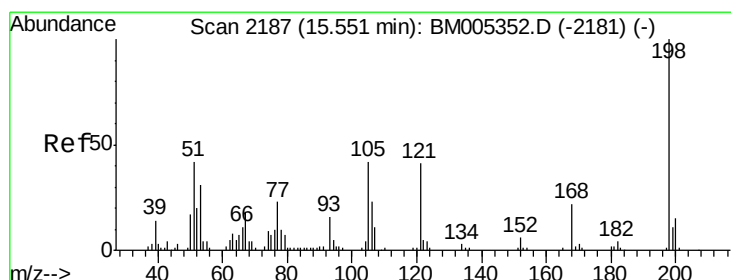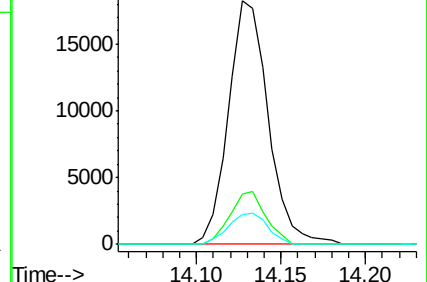

#63

4,6-Dinitro-2-methylphenol

Concen: 1.63 ng/ul

RT: 15.46 min Scan# 2172

Delta R.T. -0.09 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37


Tgt Ion:198 Resp: 5075

Ion Ratio Lower Upper

198 100

182 0.0 5.5 8.3#



77 0.0 24.2 36.2#

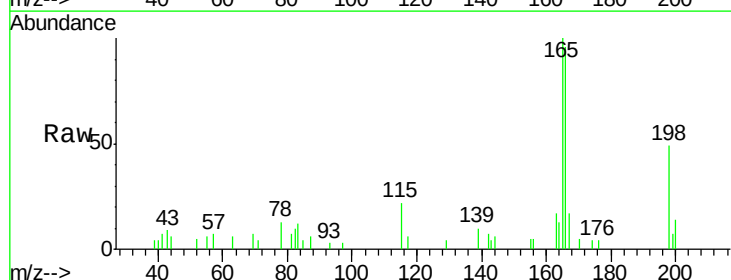


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): BM

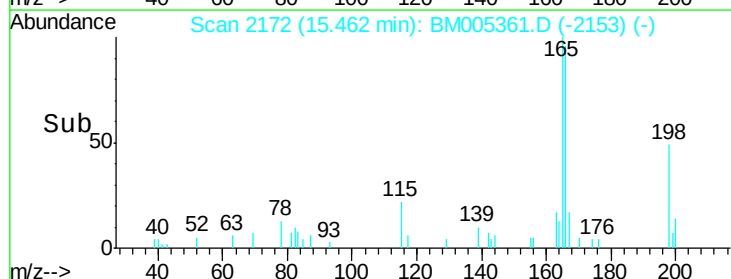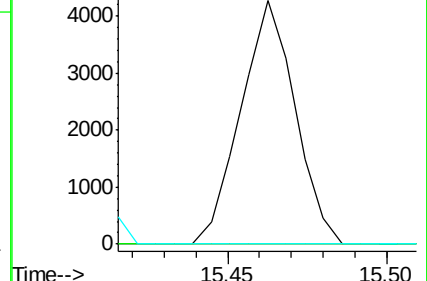



#69

Phenanthrene

Concen: 9.26 ng/ul

RT: 17.20 min Scan# 2467

Delta R.T. -0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion:178 Resp: 257343

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5




176 18.6 15.2 22.8

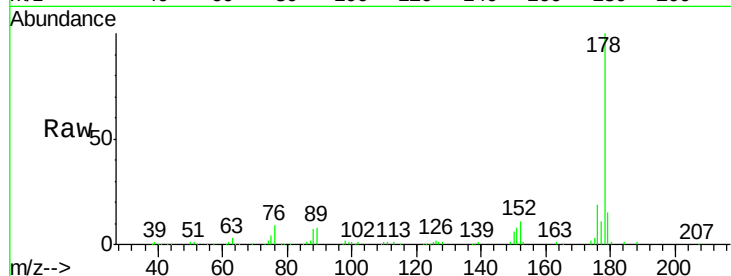

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

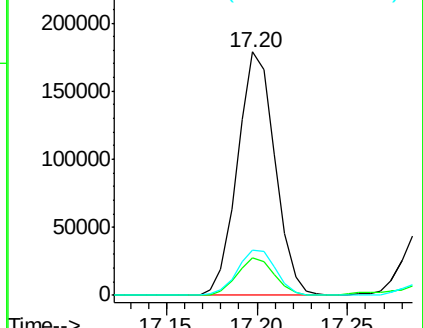

#71

Anthracene

Concen: 2.47 ng/ul

RT: 17.29 min Scan# 2483

Delta R.T. -0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37


Tgt Ion:178 Resp: 68457

Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6



176 17.9 15.1 22.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

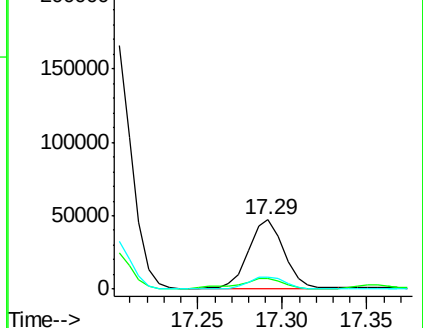

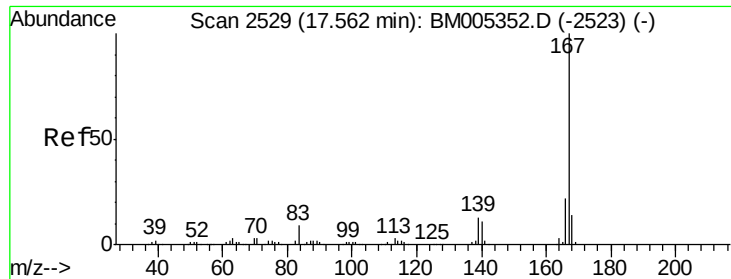

#72

Carbazole

Concen: 1.06 ng/ul

RT: 17.56 min Scan# 2529

Delta R.T. 0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion:167 Resp: 25899

Ion Ratio Lower Upper

167 100

166 23.0 17.1 25.7




139 14.6 10.2 15.2

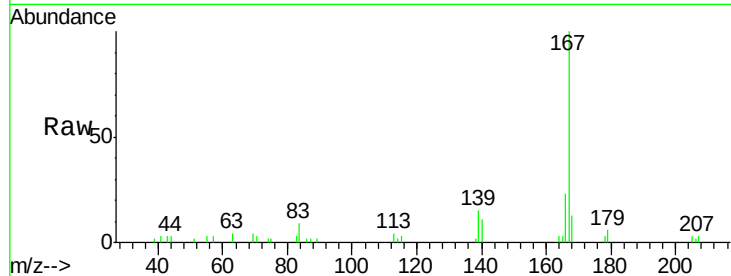

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

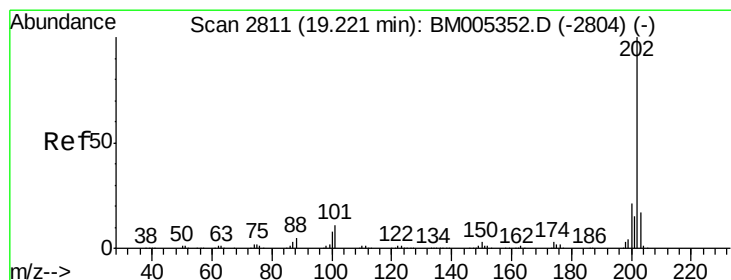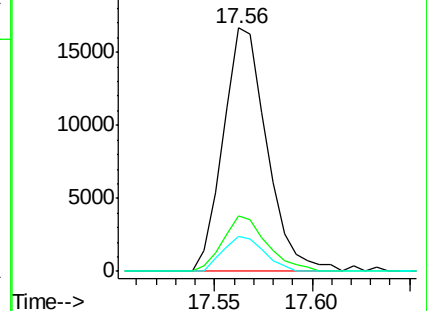

#74

Fluoranthene

Concen: 19.71 ng/ul

RT: 19.22 min Scan# 2811

Delta R.T. 0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37


Tgt Ion:202 Resp: 606552

Ion Ratio Lower Upper

202 100

101 10.8 9.2 13.8



100 7.9 7.1 10.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

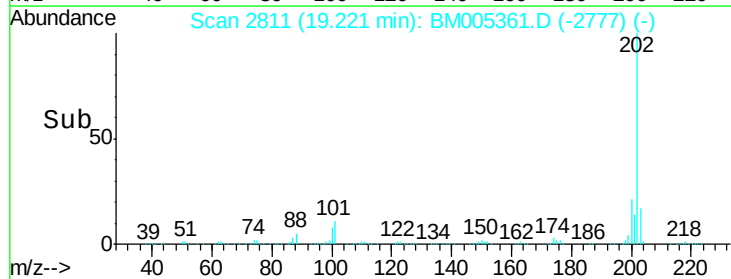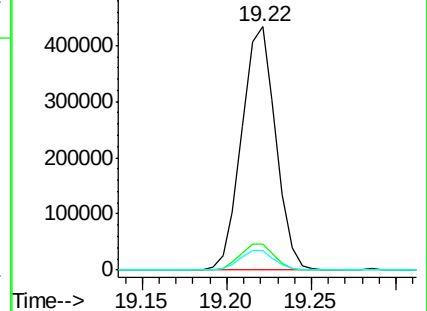

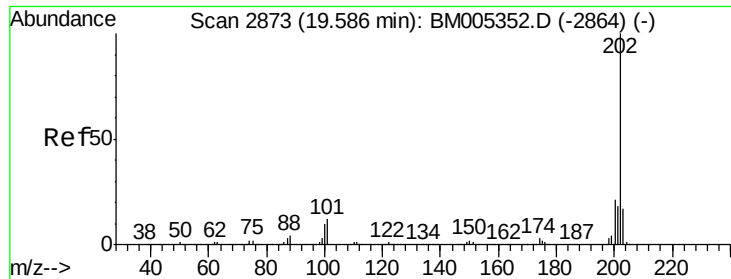

#77

Pyrene

Concen: 20.63 ng/ul

RT: 19.59 min Scan# 2873

Delta R.T. 0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion:202 Resp: 567459

Ion Ratio Lower Upper

202 100

101 11.9 10.8 16.2




100 9.5 8.4 12.6

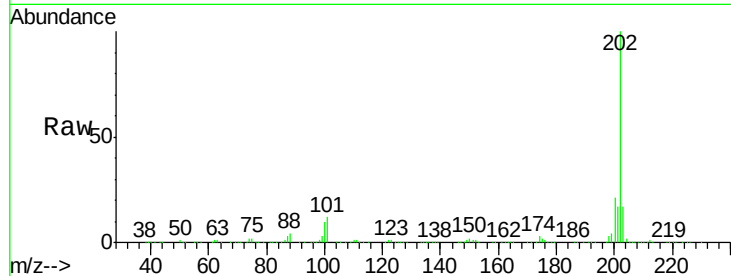

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

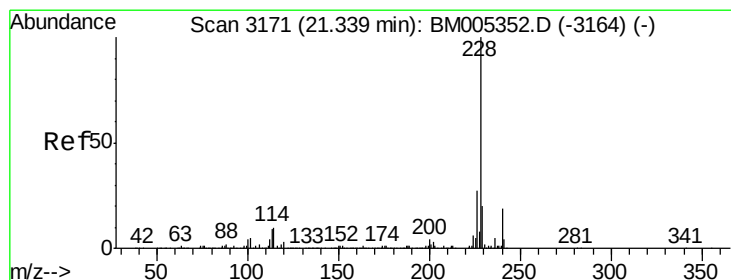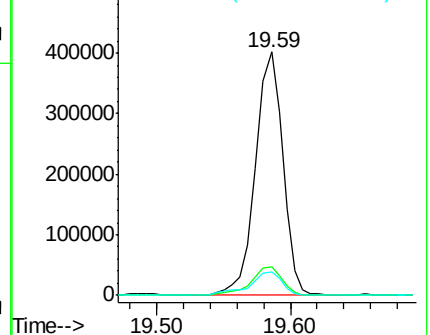

#80

Benzo(a)anthracene

Concen: 10.64 ng/ul

RT: 21.34 min Scan# 3171

Delta R.T. -0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37


Tgt Ion:228 Resp: 290304

Ion Ratio Lower Upper

228 100

229 21.0 15.5 23.3



226 28.8 21.8 32.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

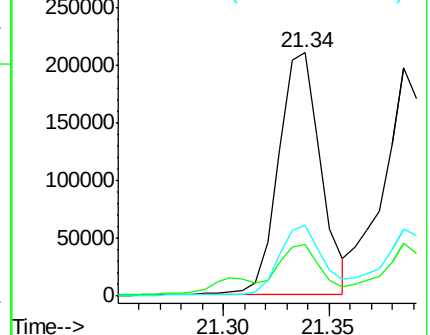

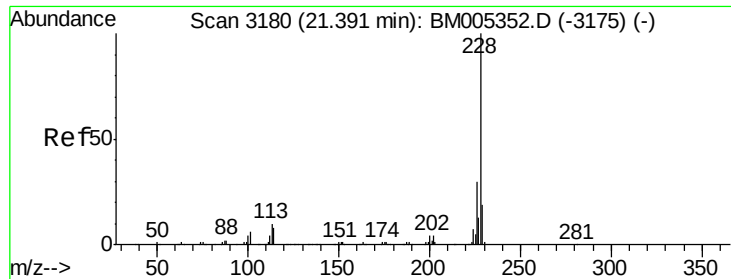

#82

Chrysene

Concen: 10.94 ng/ul

RT: 21.39 min Scan# 3179

Delta R.T. -0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion:228 Resp: 283016

Ion Ratio Lower Upper

228 100

226 29.5 23.6 35.4




229 23.0 15.4 23.0

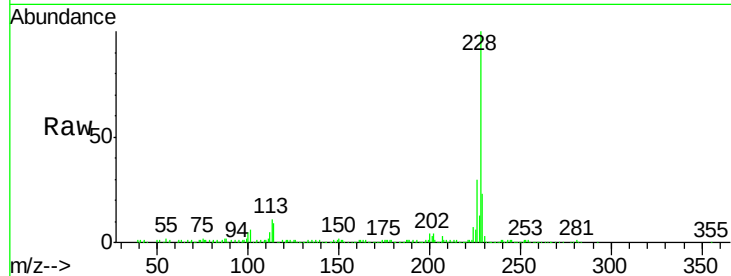

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

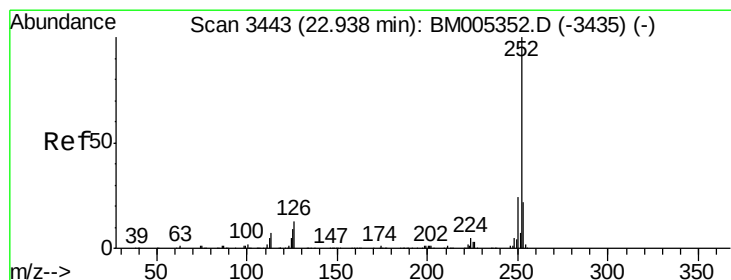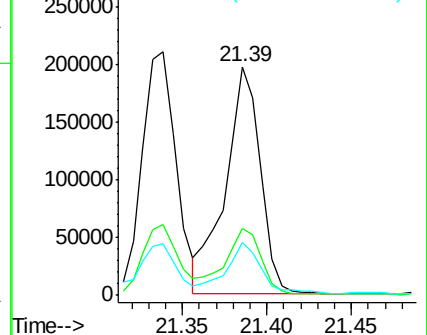

#85

Benzo(b)fluoranthene

Concen: 15.04 ng/ul

RT: 22.94 min Scan# 3444

Delta R.T. 0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37


Tgt Ion:252 Resp: 327702

Ion Ratio Lower Upper

252 100

253 23.1 17.4 26.2



125 10.4 8.4 12.6




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




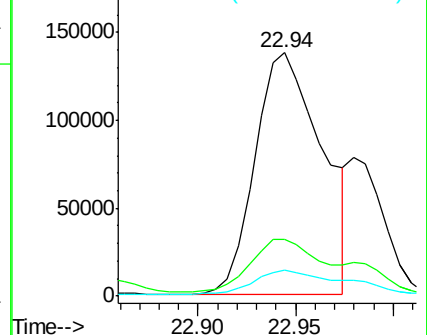


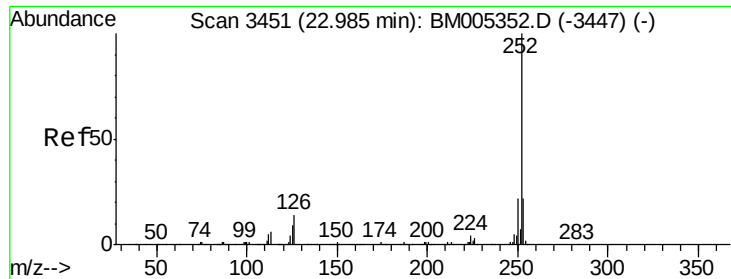

#86
Benzo(k)fluoranthene
Concen: 15.97 ng/ul
RT: 22.94 min Scan# 3444
Delta R.T. -0.04 min
Lab File: BM005361.D
Acq: 09 May 2016 15:37




Instrument :
BNA_M
ClientSampleId :
D9WW2


Tgt Ion:252 Resp: 327702
Ion Ratio Lower Upper
252 100
253 23.1 17.3 25.9
125 10.4 8.0 12.0

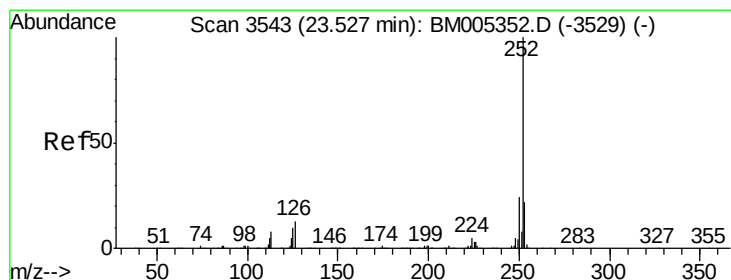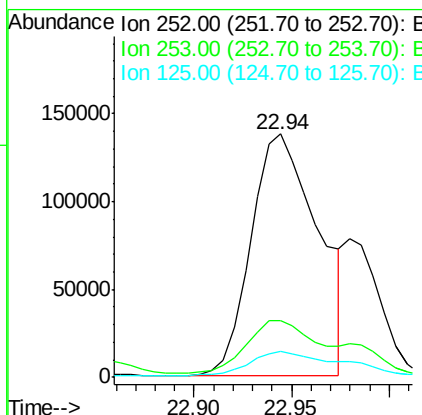

#88
Benzo(a)pyrene
Concen: 10.24 ng/ul
RT: 23.53 min Scan# 3543
Delta R.T. 0.00 min
Lab File: BM005361.D
Acq: 09 May 2016 15:37

Tgt Ion:252 Resp: 211036
Ion Ratio Lower Upper
252 100
253 23.5 17.5 26.3
125 10.4 8.7 13.1

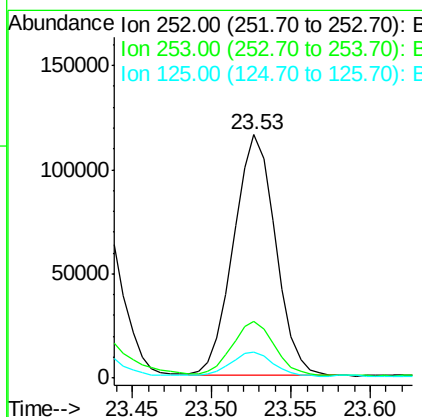



#89

Indeno(1,2,3-cd)pyrene

Concen: 5.94 ng/ul

RT: 25.92 min Scan# 3950

Delta R.T. 0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2





Tgt Ion:276 Resp: 133639

Ion Ratio Lower Upper

276 100

138 20.4 21.0 31.6#

277 23.3 19.9 29.9

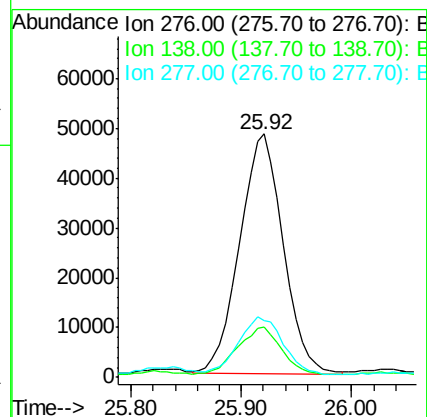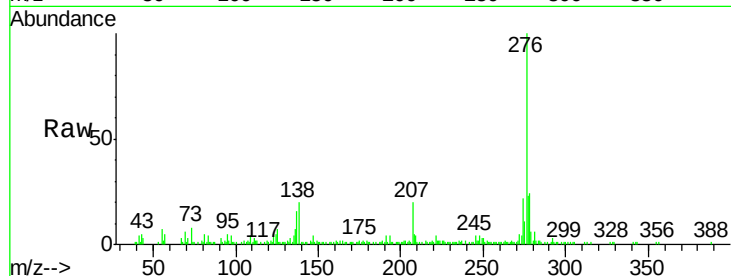

#90

Dibenzo(a,h)anthracene

Concen: 1.91 ng/ul

RT: 25.92 min Scan# 3950

Delta R.T. -0.01 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37




Tgt Ion:278 Resp: 35866


Ion Ratio Lower Upper

278 100

139 0.0 13.8 20.6#

279 27.0 18.9 28.3

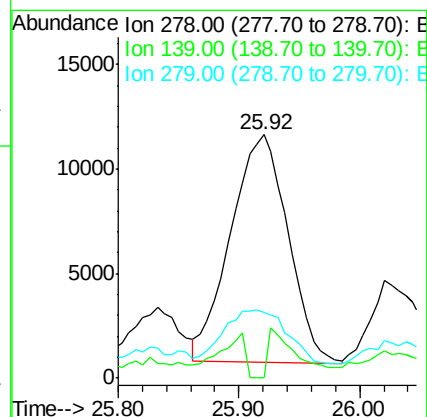



#91

Benzo(g,h,i)perylene

Concen: 6.29 ng/ul

RT: 26.62 min Scan# 4069

Delta R.T. 0.00 min

Lab File: BM005361.D

Acq: 09 May 2016 15:37

Instrument :

BNA_M

ClientSampleId :

D9WW2


Tgt Ion: 276 Resp: 119726

Ion Ratio Lower Upper

276 100

138 20.2 18.2 27.4

277 24.5 19.4 29.2



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

