

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
 Data File : BM005364.D
 Acq On : 09 May 2016 18:04
 Operator : UM/SJ
 Sample : H2888-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW6

Quant Time: May 10 04:25:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	78631	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	373076	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	228584	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	524644	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	553556	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	428259	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	7516	4.49	ng/uL	0.00
5) Phenol-d5	6.94	99	168384	23.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	97411	23.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	133429	24.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	108295	18.37	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	67177	25.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	77143	25.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	139011	24.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	149306	22.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	473943	25.87	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	562637	26.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	64861	19.39	ng/ul	0.00
57) Fluorene-d10	15.40	176	416070	26.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	58319	19.76	ng/ul	0.00
70) Anthracene-d10	17.26	188	626024	26.99	ng/ul	0.00
76) Pyrene-d10	19.56	212	723489	28.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	520495	27.46	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	134974	7.37	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
Data File : BM005364.D
Acq On : 09 May 2016 18:04
Operator : UM/SJ
Sample : H2888-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WW6

Quant Time: May 10 04:25:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration

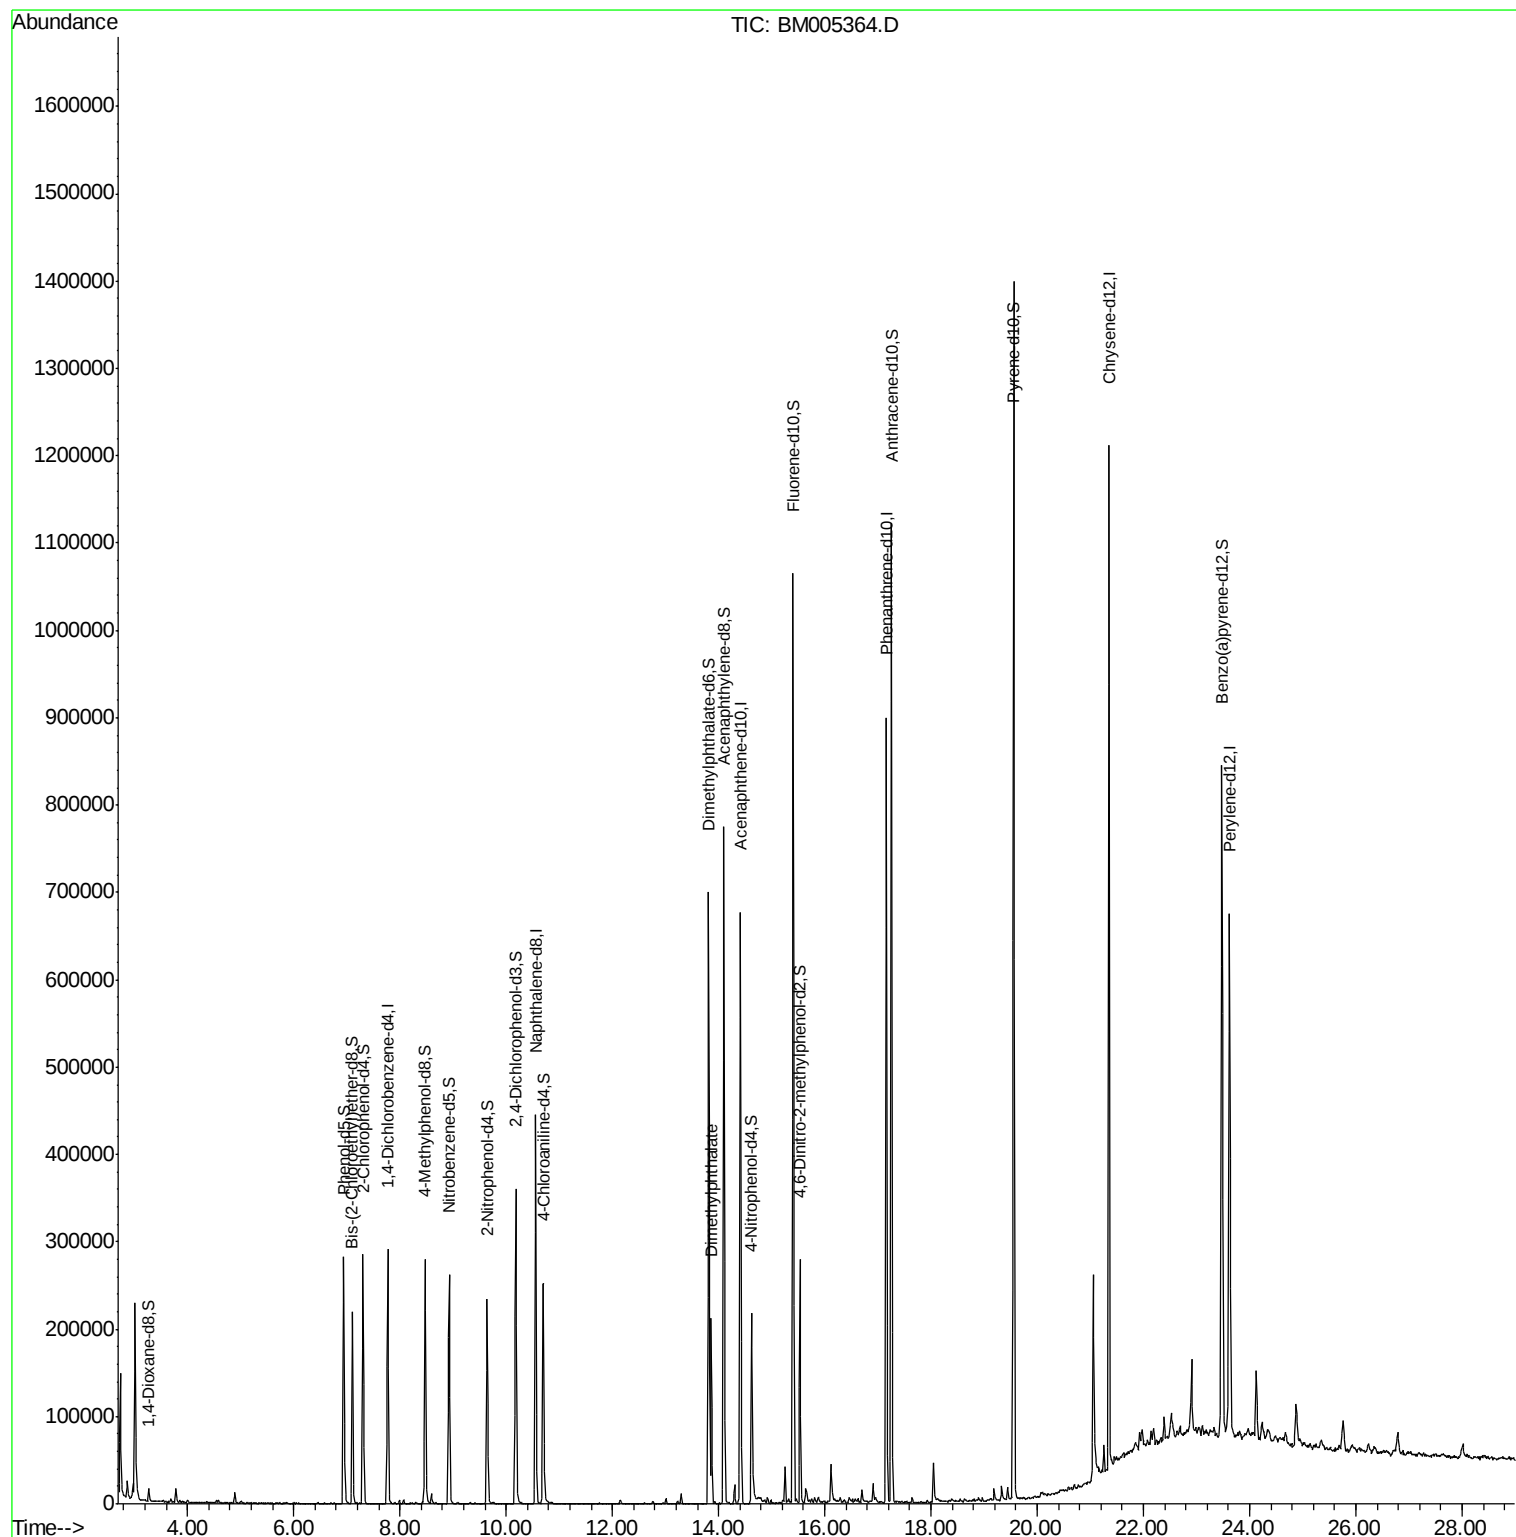

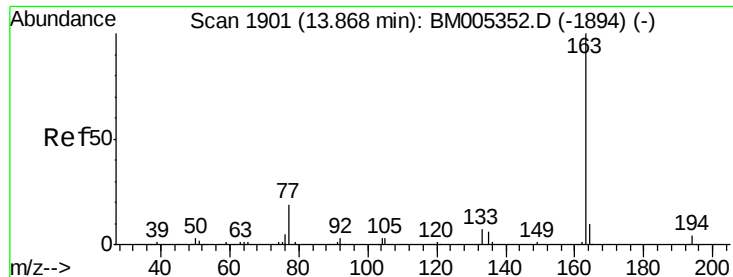

#44

Dimethylphthalate

Concen: 7.37 ng/ul

RT: 13.86 min Scan# 1900

Delta R.T. -0.01 min

Lab File: BM005364.D

Acq: 09 May 2016 18:04

Instrument :

BNA_M

ClientSampleId :

D9WW6


Tgt Ion:163 Resp: 134974

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 9.5 7.9 11.9

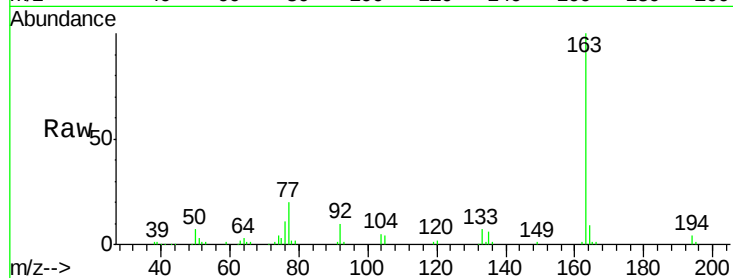

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

