

(QT Reviewed)


```
Data Path   : Z:\HPCHEM1\BNA_M\DATA\BM050916\  
Data File  : BM005362.D  
Acq On     : 09 May 2016   16:14  
Operator   : UM/SJ  
Sample     : H2888-06  
Misc       :  
ALS Vial   : 12      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
D9WW3

Manual Integrations

sohil
5/10/2016 6:45:40 PM

Quant Time: May 10 05:10:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration

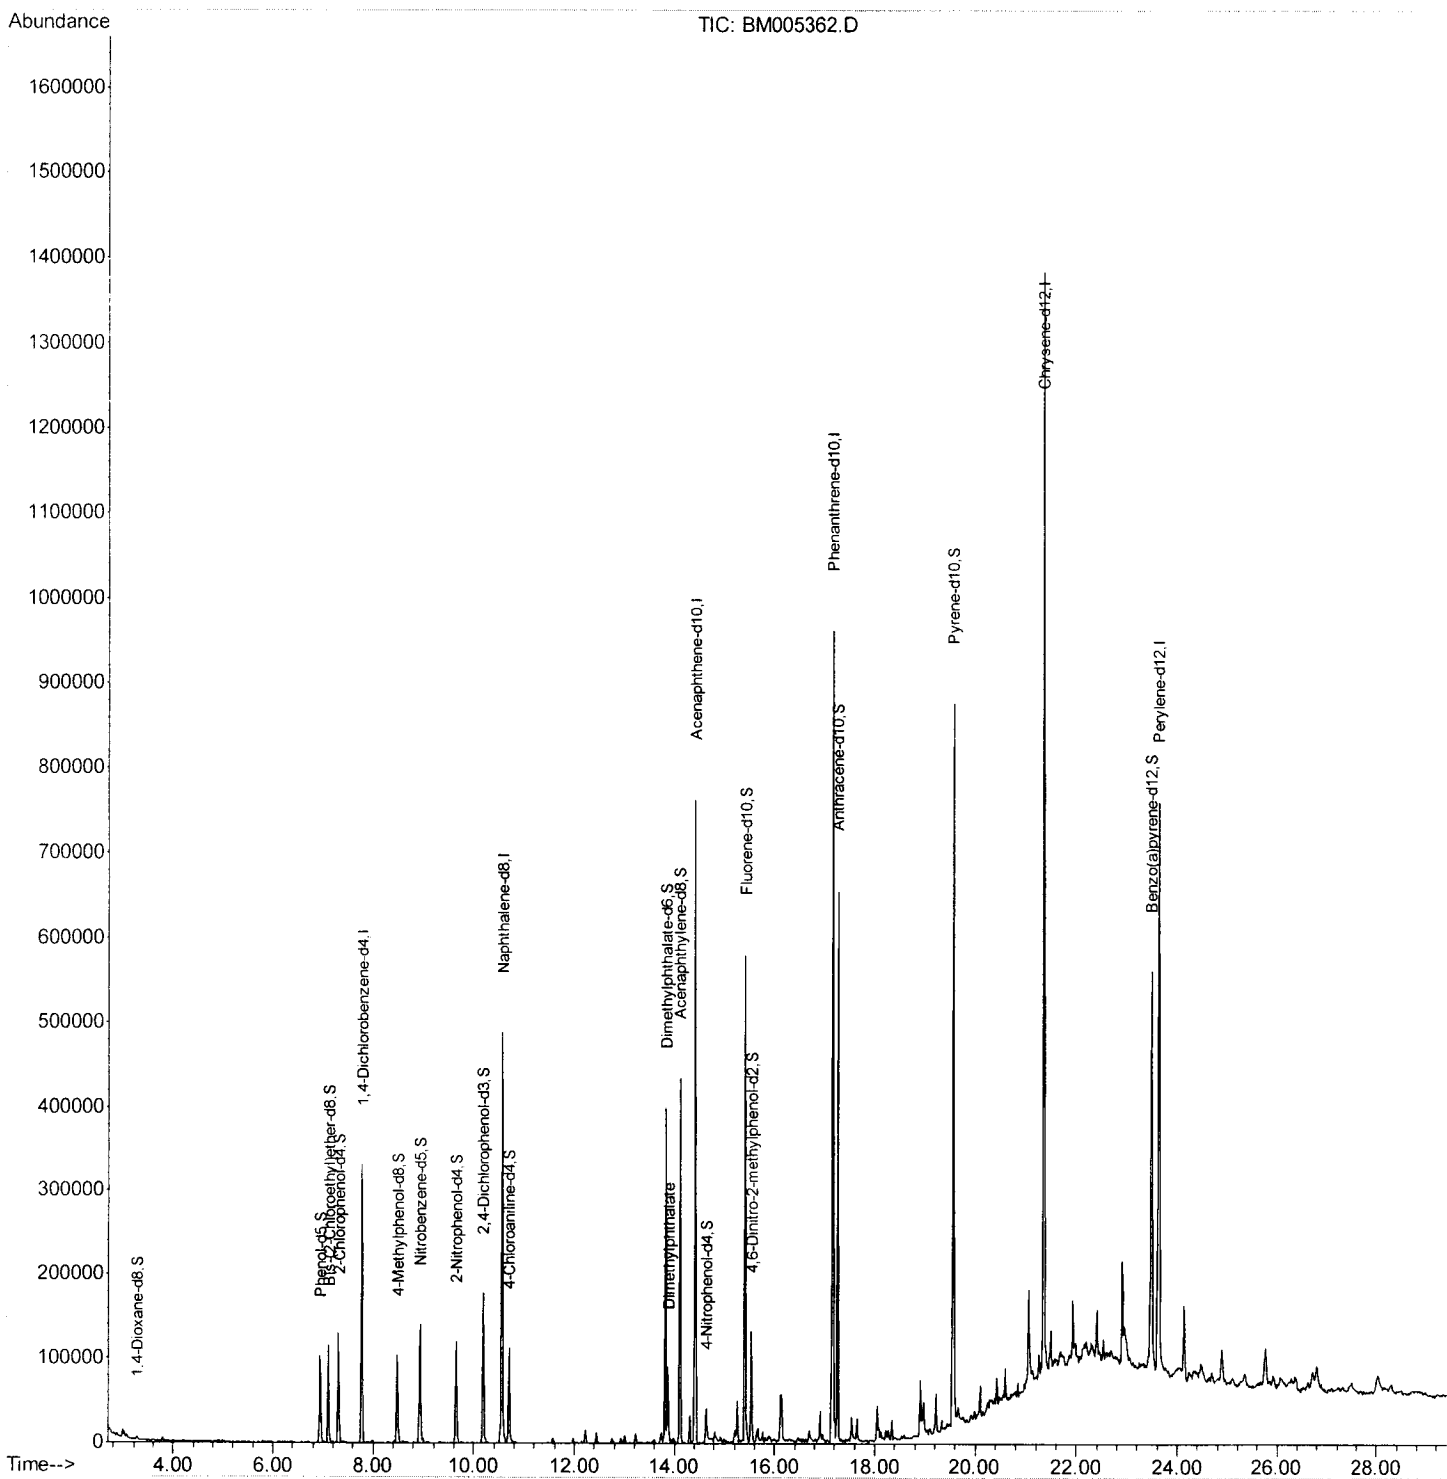

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
 Data File : BM005362.D
 Acq On : 09 May 2016 16:14
 Operator : UM/SJ
 Sample : H2888-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW3

Manual Integrations
 APPROVED

sohil
 5/10/2016 6:45:40 PM

Quant Time: May 10 04:25:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

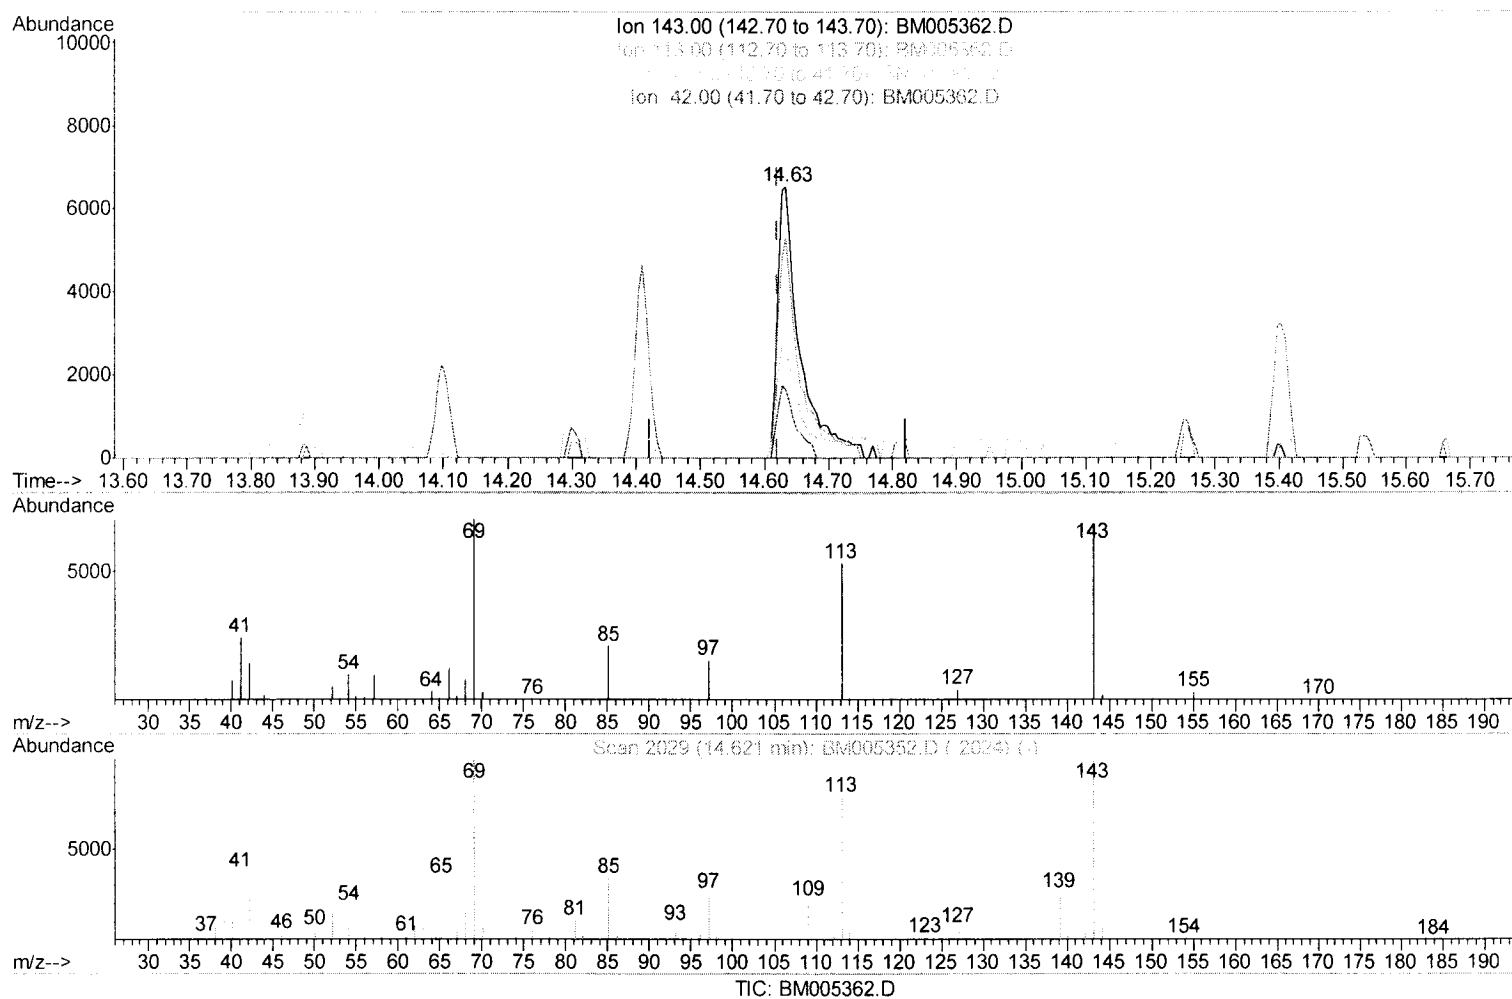

(51) 4-Nitrophenol-d4 (S)

14.633min (+0.012) 4.41ng/ul m

response 16359

Ion	Exp%	Act%
143.00	100	100
113.00	75.60	81.26
41.00	38.10	39.85
42.00	26.00	25.39

U.M
 05/11/2016

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
Data File : BM005362.D
Acq On : 09 May 2016 16:14
Operator : UM/SJ
Sample : H2888-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WW3

Quant Time: May 10 04:25:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
5/10/2016 6:45:40 PM

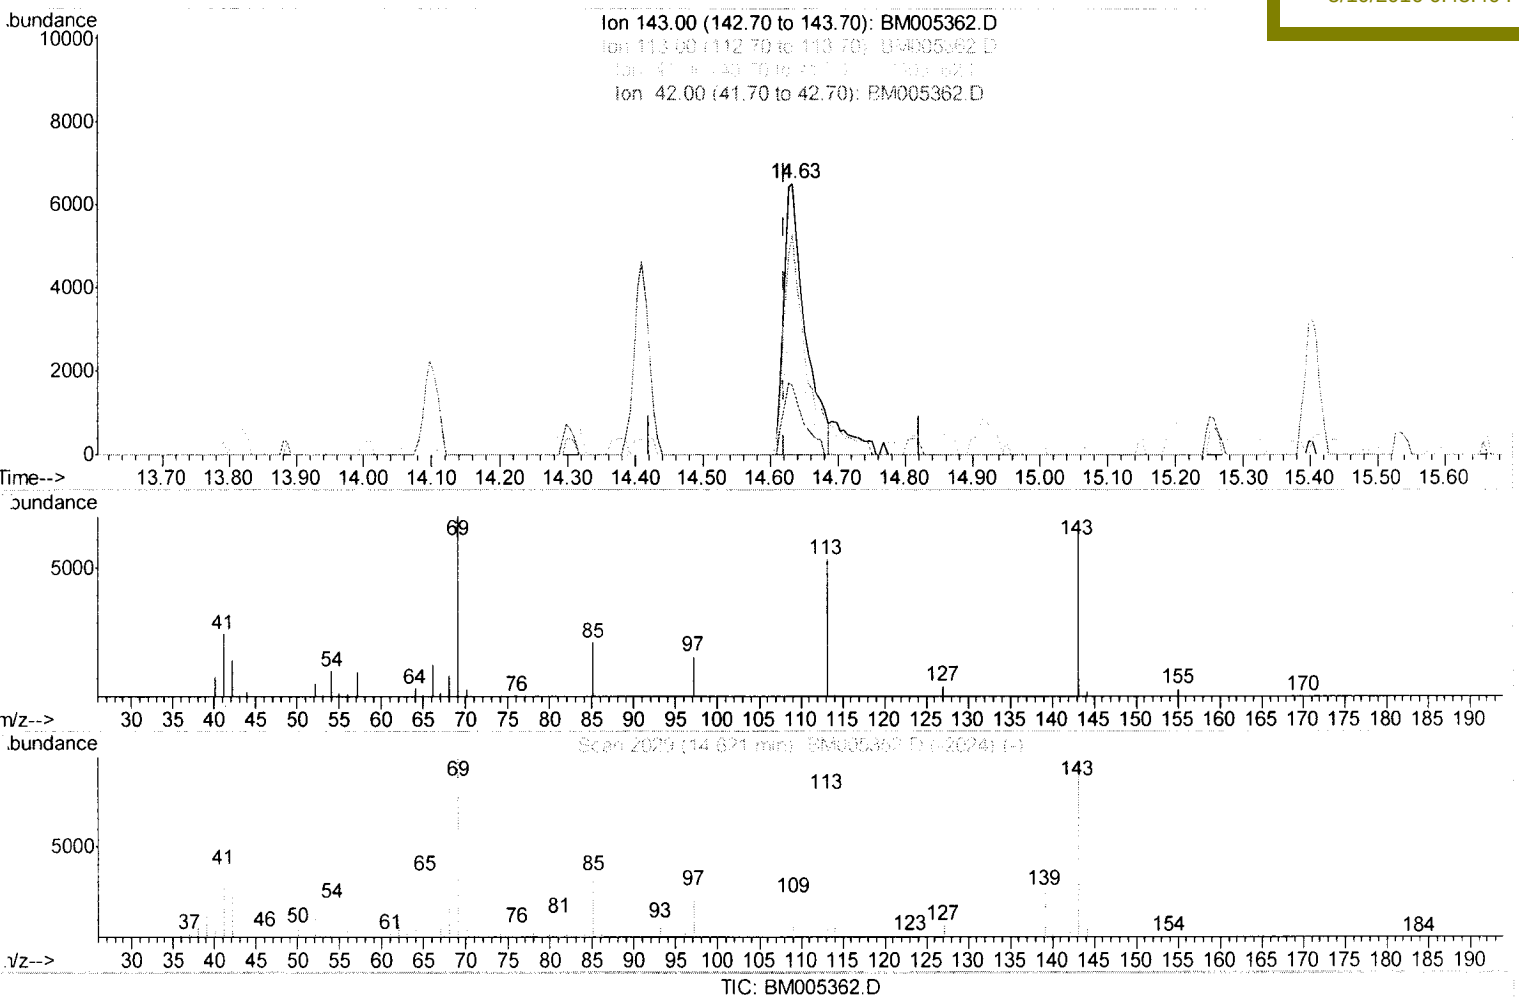

(51) 4-Nitrophenol-d4 (S)

14.633min (+0.012) 3.86ng/ul

response 14322

Ion	Exp%	Act%
143.00	100	100
113.00	75.60	81.26
41.00	38.10	39.85
42.00	26.00	25.39

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050916\
 Data File : BM005362.D
 Acq On : 09 May 2016 16:14
 Operator : UM/SJ
 Sample : H2888-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW3

Quant Time: May 10 05:10:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 5/10/2016 6:45:40 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	89929	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	413576	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	253449	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	571391	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	611543	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	497301	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	2564	1.34	ng/uL	0.00
5) Phenol-d5	6.94	99	64560	7.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	51923	11.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	61808	10.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	42515	6.31	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	35469	12.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	39990	11.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	71119	11.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	66589	8.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	264218	13.01	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	315131	13.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	16359m	4.41	ng/ul	0.01
57) Fluorene-d10	15.40	176	232807	13.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	27883	8.67	ng/ul	0.00
70) Anthracene-d10	17.26	188	356747	14.12	ng/ul	0.00
76) Pyrene-d10	19.56	212	416891	14.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	302837	13.76	ng/ul	0.00

U.M
 5/11/2016

Target Compounds					Qvalue
44) Dimethylphthalate	13.86	163	53300	2.63 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed